


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080321\
 Data File : VW019655.D
 Acq On : 03 Aug 2021 09:26
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/5.00mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W080321S.M
 Title : SW846 8260
 Last Update : Tue Aug 03 16:22:46 2021

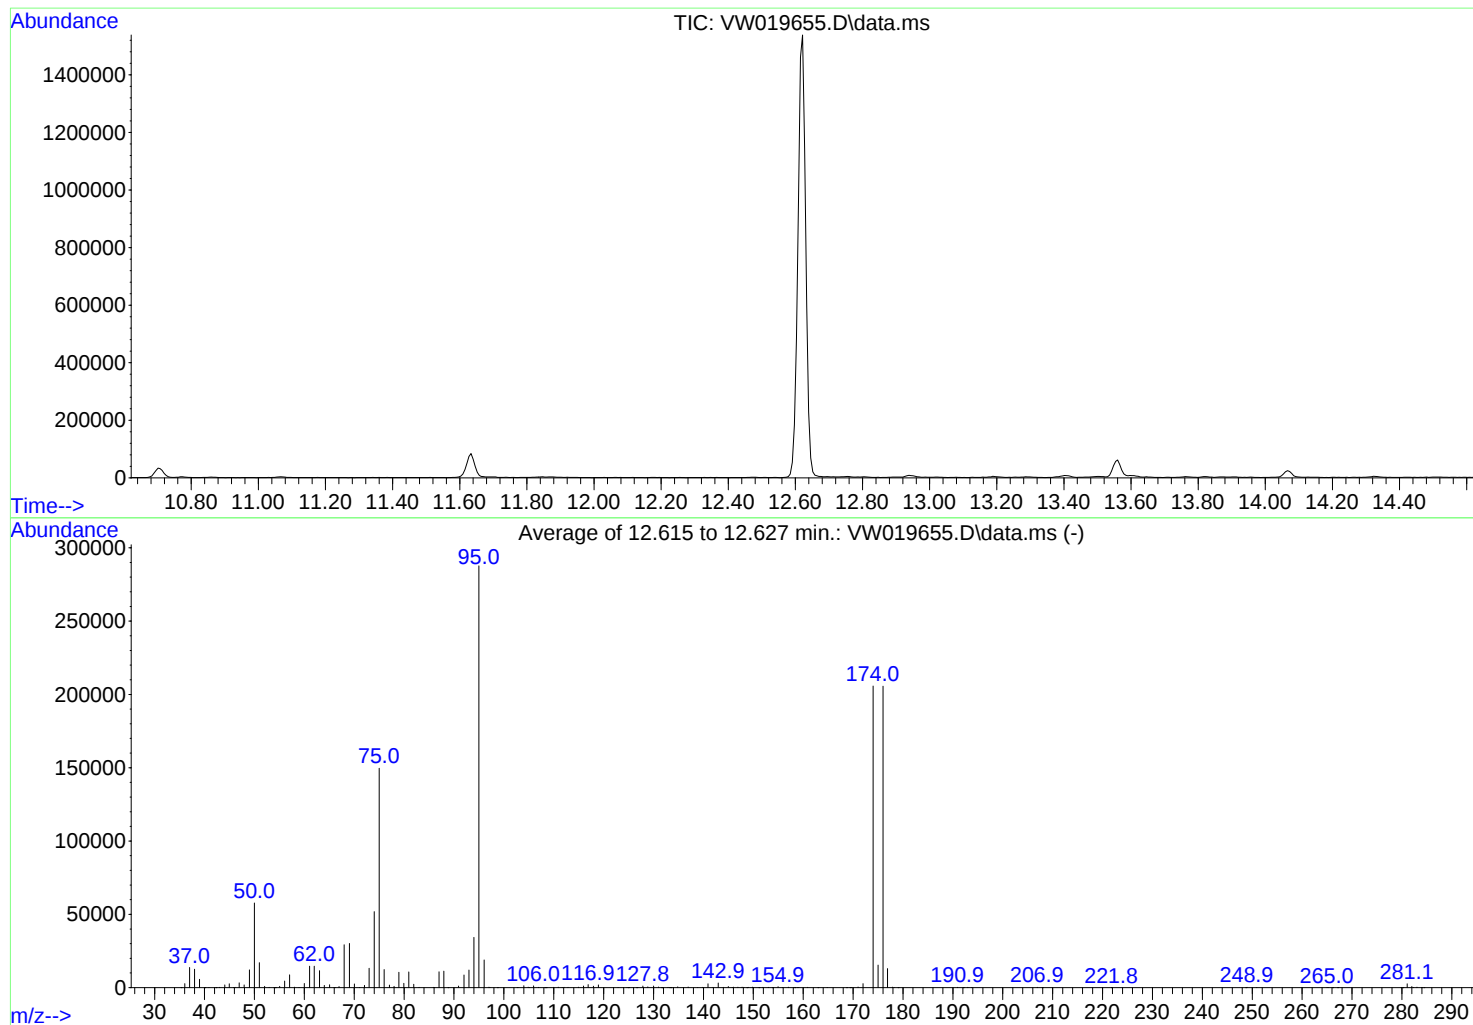

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	57768	PASS
75	95	30	60	52.0	149616	PASS
95	95	100	100	100.0	287723	PASS
96	95	5	9	6.6	18908	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.5	205760	PASS
175	174	5	9	7.5	15446	PASS
176	174	95	101	99.9	205568	PASS
177	176	5	9	6.3	12960	PASS