


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080419\
 Data File : VW011679.D
 Acq On : 03 Aug 2019 21:49
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
 Title : SW846 8260
 Last Update : Sat Jul 27 00:23:30 2019

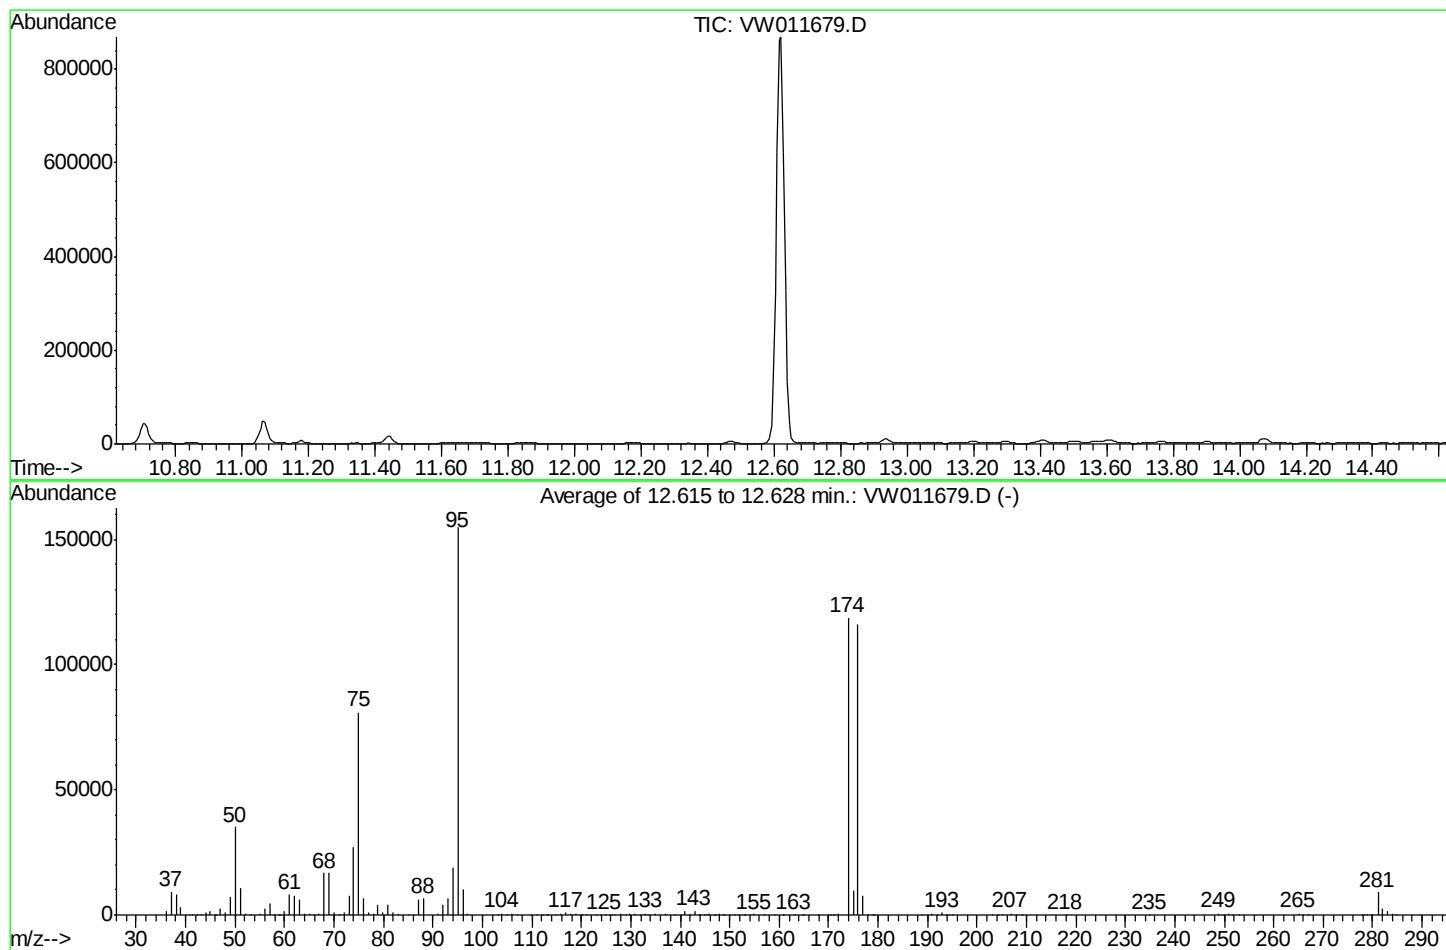

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	35168	PASS
75	95	30	60	52.2	80861	PASS
95	95	100	100	100.0	154818	PASS
96	95	5	9	6.6	10256	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.7	118770	PASS
175	174	5	9	8.2	9728	PASS
176	174	95	101	97.7	116034	PASS
177	176	5	9	6.6	7630	PASS