

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080521\
 Data File : VW019677.D
 Acq On : 05 Aug 2021 12:34
 Operator : SY/VA
 Sample : M3264-07
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 06 01:38:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 06 01:35:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	531027	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	493803	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	247892	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	146420	19.460	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	77.840%	
7) Chloroethane-d5	2.891	69	122816	22.890	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	91.560%	
11) 1,1-Dichloroethene-d2	4.031	63	308280	21.235	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	84.960%	
21) 2-Butanone-d5	7.074	46	92413	42.318	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	84.640%	
24) Chloroform-d	7.653	84	324727	22.131	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	88.520%	
26) 1,2-Dichloroethane-d4	8.311	65	193732	24.060	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	96.240%	
32) Benzene-d6	8.281	84	656285	22.327	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	89.320%	
36) 1,2-Dichloropropane-d6	9.274	67	198677	21.686	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	86.760%	
41) Toluene-d8	10.323	98	597817	22.558	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	90.240%	
43) trans-1,3-Dichloroprop...	10.579	79	87367	22.268	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	89.080%	
47) 2-Hexanone-d5	10.927	63	74803	44.009	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	88.020%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	169711	22.925	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	91.680%	
66) 1,2-Dichlorobenzene-d4	13.853	152	202072	23.104	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	92.400%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.221	50	108721	16.749	ug/L	100
6) Bromomethane	2.782	94	41907	8.483	ug/L	100
9) Trichlorofluoromethane	3.269	101	97449	17.956	ug/L	98
12) 1,1-Dichloroethene	4.050	96	139341	20.099	ug/L	88
13) Acetone	4.123	43	122933	76.398	ug/L	92
15) Methyl Acetate	4.672	43	135505	37.836	ug/L	99
16) Methylene chloride	4.928	84	117465	11.096	ug/L	95
17) trans-1,2-Dichloroethene	5.428	96	76677	10.171	ug/L	99
18) Methyl tert-butyl Ether	5.428	73	325213	31.223	ug/L	98
20) cis-1,2-Dichloroethene	7.171	96	197345	24.749	ug/L	95
23) Bromochloromethane	7.513	128	52483	14.615	ug/L	97
27) 1,2-Dichloroethane	8.403	62	98900	10.736	ug/L	98
29) Cyclohexane	7.958	56	115277	9.103	ug/L	94
30) 1,1,1-Trichloroethane	7.878	97	110523	10.845	ug/L	99
31) Carbon tetrachloride	8.073	117	127538	13.450	ug/L	100
34) Trichloroethene	9.091	95	312247	39.582	ug/L	91
35) Methylcyclohexane	9.335	83	356208	25.517	ug/L	97
37) 1,2-Dichloropropane	9.372	63	97891	12.498	ug/L	99
38) Bromodichloromethane	9.646	83	200240	20.617	ug/L	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080521\
 Data File : VW019677.D
 Acq On : 05 Aug 2021 12:34
 Operator : SY/VA
 Sample : M3264-07
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 06 01:38:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 06 01:35:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


39) cis-1,3-Dichloropropene	10.073	75	193018	16.114	ug/L	98
42) Toluene	10.390	91	658839	20.451	ug/L	95
44) trans-1,3-Dichloropropene	10.603	75	80256	7.617	ug/L	96
46) Tetrachloroethene	10.866	164	237844	39.559	ug/L	94
48) 2-Hexanone	10.969	43	118432	35.174	ug/L	97
49) Dibromochloromethane	11.128	129	127560	20.352	ug/L	98
52) Ethylbenzene	11.731	91	537837	15.335	ug/L	97
53) m,p-Xylene	11.847	106	133243	10.053	ug/L	98
54) o-Xylene	12.164	106	152254	12.156	ug/L	96
55) Styrene	12.164	104	8907	0.410	ug/L #	1
60) Isopropylbenzene	12.463	105	423268	12.705	ug/L	100
61) 1,2,3-Trichloropropane	12.743	75	28293	5.210	ug/L #	1
64) 1,3-Dichlorobenzene	13.499	146	297404	19.508	ug/L	90
67) 1,2-Dichlorobenzene	13.865	146	143499	10.448	ug/L	96
68) 1,2-Dibromo-3-chloropr...	14.481	75	24322	20.525	ug/L	93
69) 1,3,5-Trichlorobenzene	14.627	180	270354	24.270	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080521\
Data File : VW019677.D
Acq On : 05 Aug 2021 12:34
Operator : SY/VA
Sample : M3264-07
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 06 01:38:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 06 01:35:48 2021
Response via : Initial Calibration




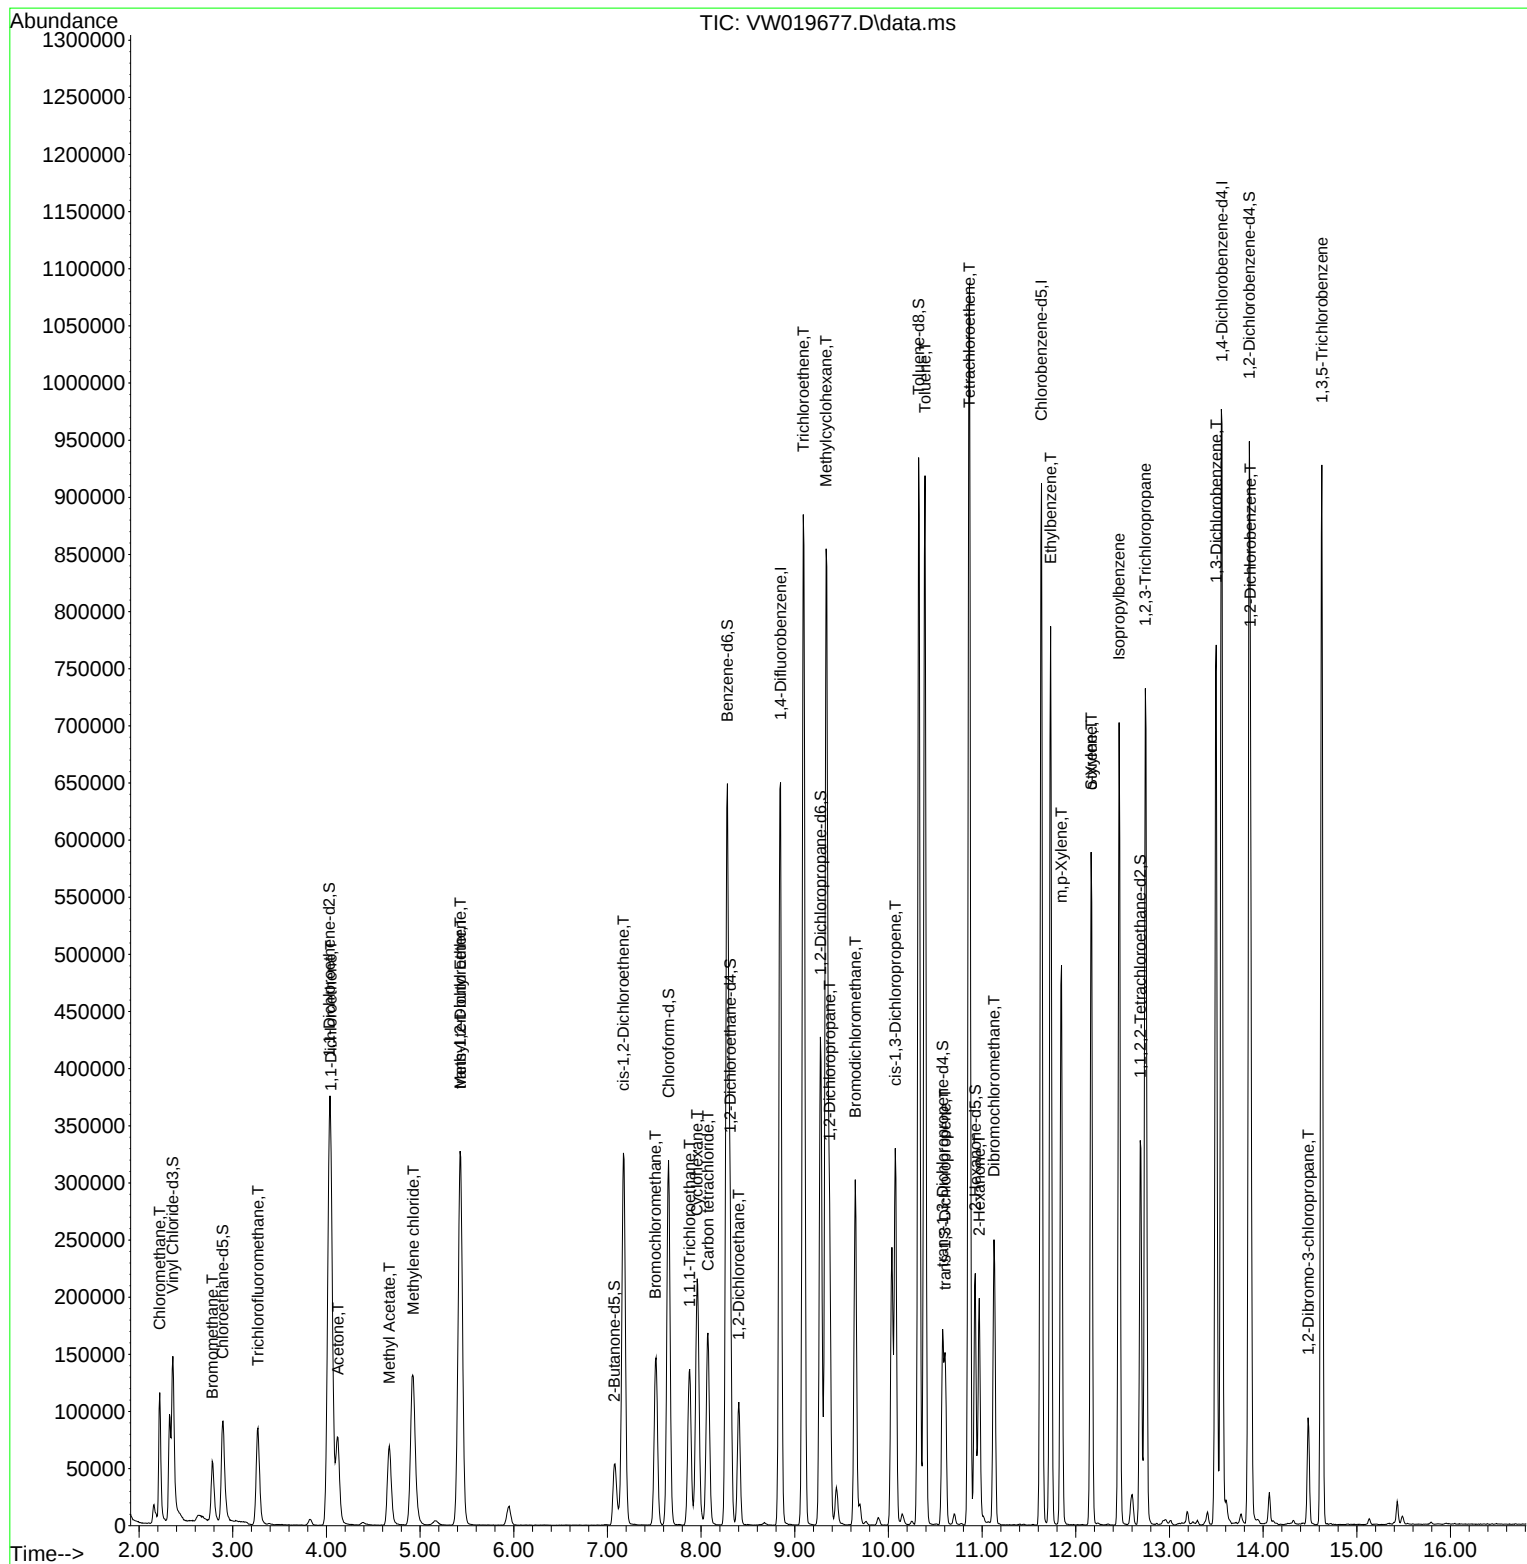




#3
Chloromethane
Concen: 16.749 ug/L
RT: 2.221 min Scan# 52
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampled :


Tgt Ion: 50 Resp: 108721
Ion Ratio Lower Upper
50 100
52 32.1 22.5 41.9

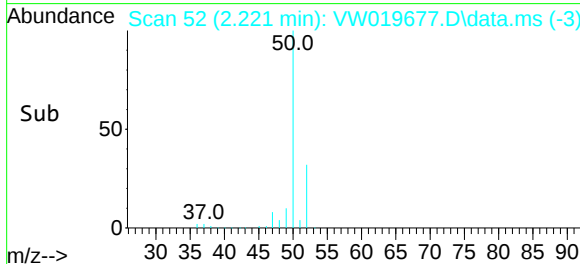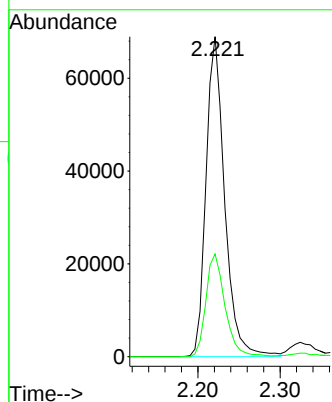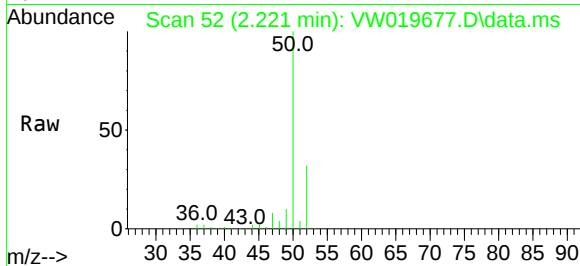

#6
Bromomethane
Concen: 8.483 ug/L
RT: 2.782 min Scan# 144
Delta R.T. -0.006 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

Tgt Ion: 94 Resp: 41907
Ion Ratio Lower Upper
94 100
96 93.0 65.3 121.3


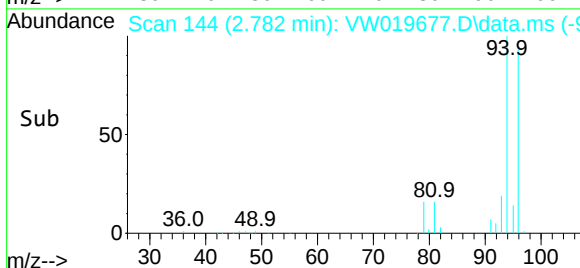

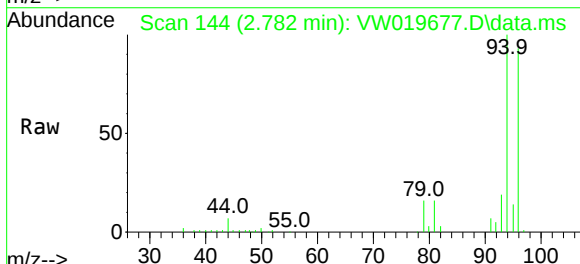


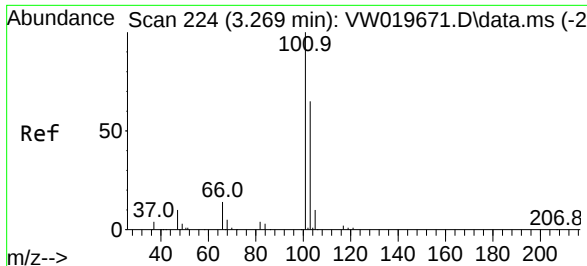

#9
 Trichlorofluoromethane
 Concen: 17.956 ug/L
 RT: 3.269 min Scan# 224
 Delta R.T. -0.000 min
 Lab File: VW019677.D
 Acq: 05 Aug 2021 12:34




Instrument :
 MSVOA_W
 ClientSampled :


Tgt Ion:101 Resp: 97449
 Ion Ratio Lower Upper
 101 100
 103 65.2 51.0 76.4

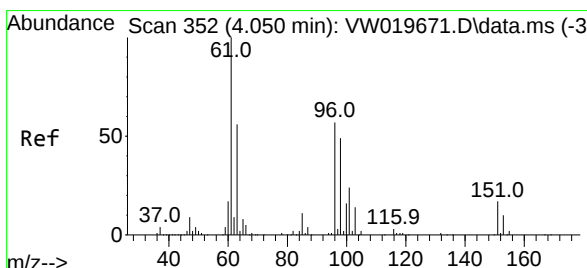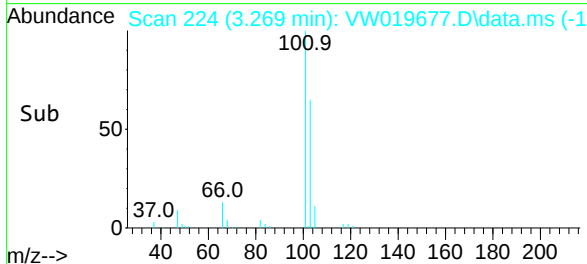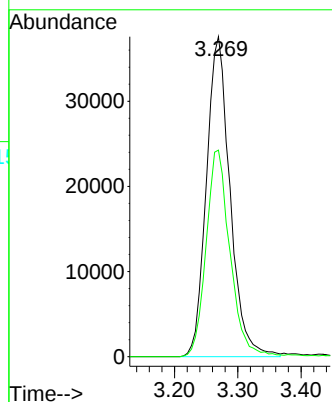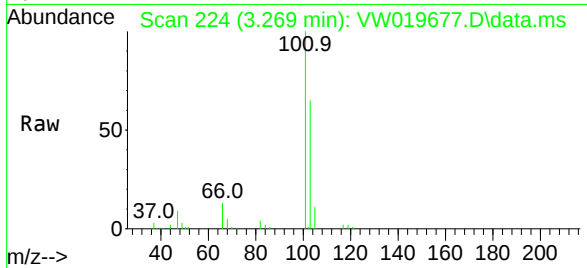

#12
 1,1-Dichloroethene
 Concen: 20.099 ug/L
 RT: 4.050 min Scan# 352
 Delta R.T. -0.000 min
 Lab File: VW019677.D
 Acq: 05 Aug 2021 12:34

Tgt Ion: 96 Resp: 139341
 Ion Ratio Lower Upper
 96 100
 61 182.9 118.1 219.3
 63 136.0 83.7 155.5


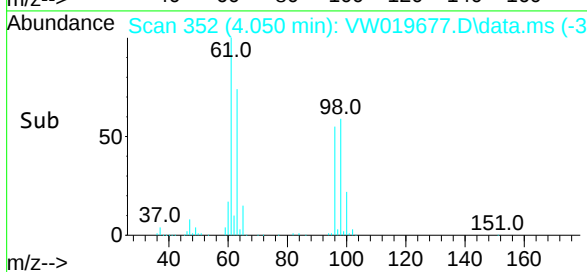
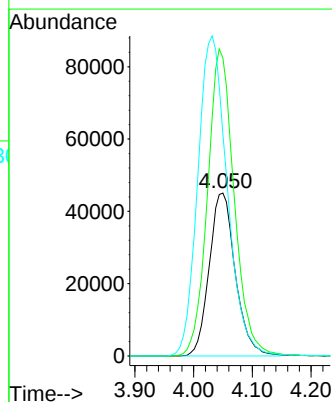
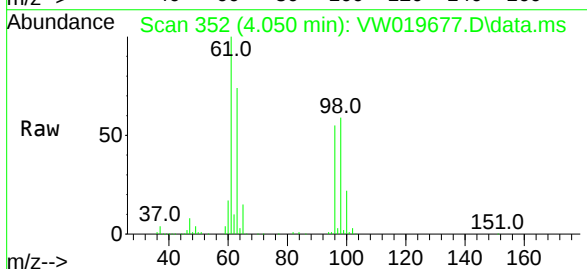


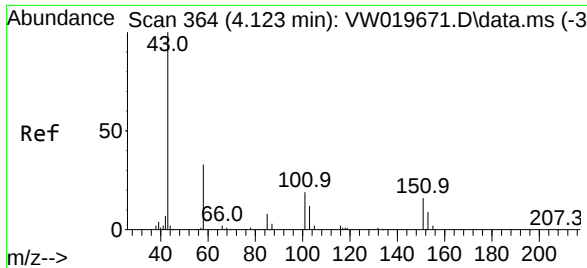

#13
Acetone
Concen: 76.398 ug/L
RT: 4.123 min Scan# 364
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampled :


Tgt Ion: 43 Resp: 122933
Ion Ratio Lower Upper
43 100
58 31.1 0.0 53.8

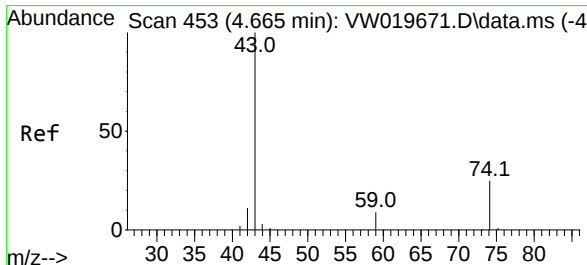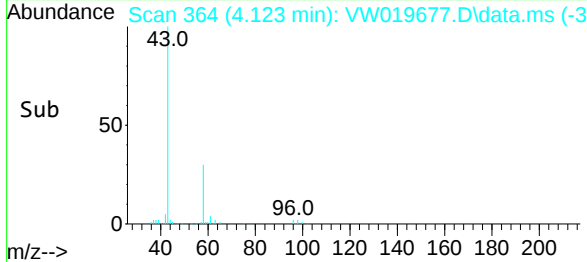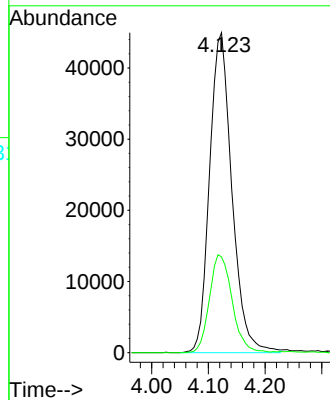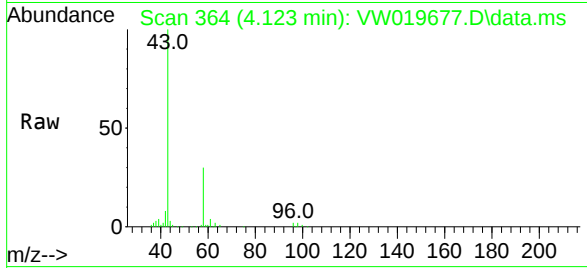

#15
Methyl Acetate
Concen: 37.836 ug/L
RT: 4.672 min Scan# 454
Delta R.T. 0.006 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

Tgt Ion: 43 Resp: 135505
Ion Ratio Lower Upper
43 100
74 24.4 20.0 30.0


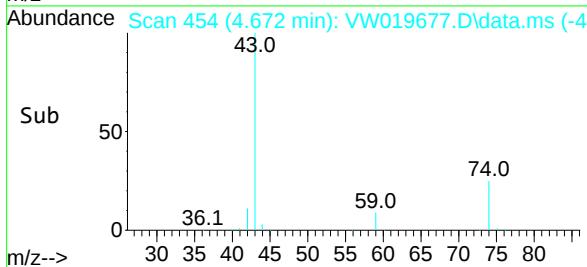
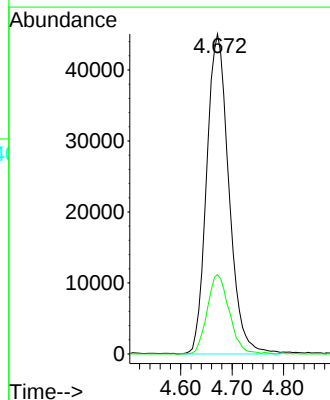
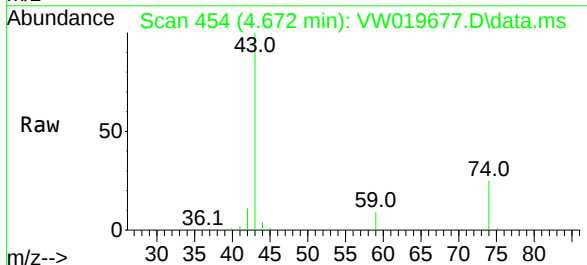




#16
Methylene chloride
Concen: 11.096 ug/L
RT: 4.928 min Scan# 496
Delta R.T. 0.006 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 84 Resp: 117465
Ion Ratio Lower Upper
84 100
86 62.5 45.3 84.1
49 117.5 86.6 160.8

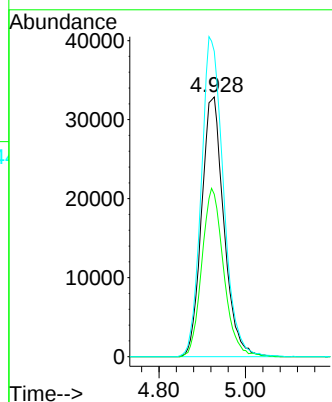

#17
trans-1,2-Dichloroethene
Concen: 10.171 ug/L
RT: 5.428 min Scan# 578
Delta R.T. -0.006 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

Tgt Ion: 96 Resp: 76677
Ion Ratio Lower Upper
96 100
61 139.5 98.3 182.7
98 64.0 46.1 85.7


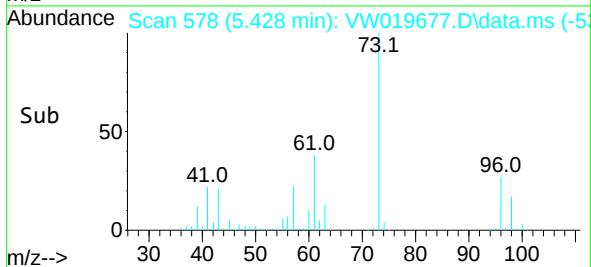
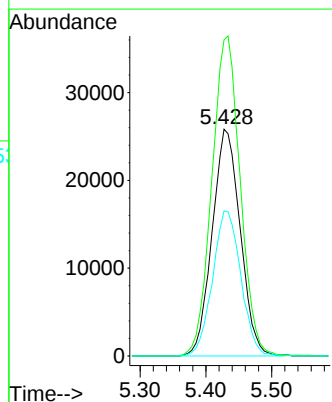
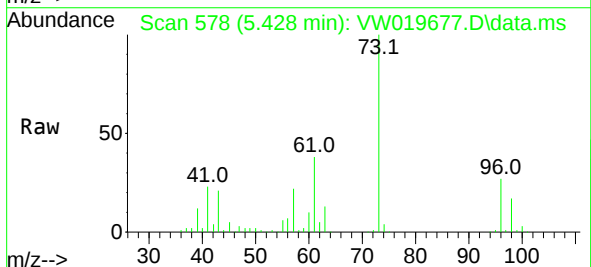




#18
Methyl tert-butyl Ether
Concen: 31.223 ug/L
RT: 5.428 min Scan# 578
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 73 Resp: 325213
Ion Ratio Lower Upper
73 100
43 20.9 17.7 26.5
57 22.0 17.0 25.4

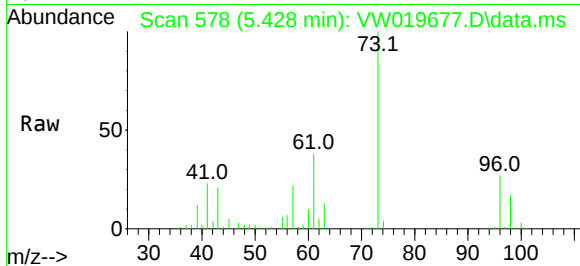

#20
cis-1,2-Dichloroethene
Concen: 24.749 ug/L
RT: 7.171 min Scan# 864
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

Tgt Ion: 96 Resp: 197345
Ion Ratio Lower Upper
96 100
61 131.8 88.5 164.3
68 0.0 0.0 0.0


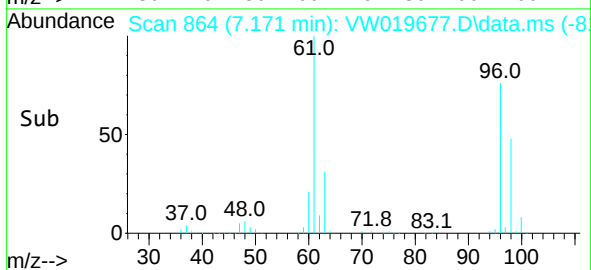

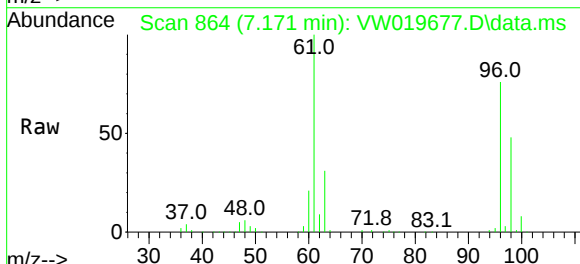


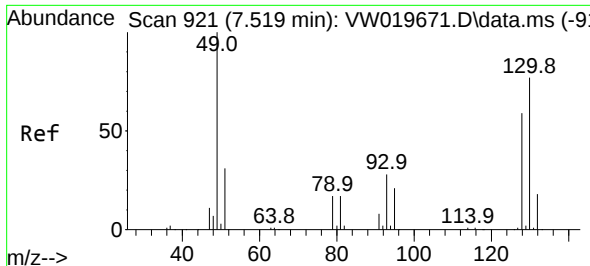

#23
Bromochloromethane
Concen: 14.615 ug/L
RT: 7.513 min Scan# 920
Delta R.T. -0.006 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:128 Resp: 52483
Ion Ratio Lower Upper
128 100
49 168.7 116.3 215.9
130 122.3 82.4 153.0
51 52.0 42.6 64.0

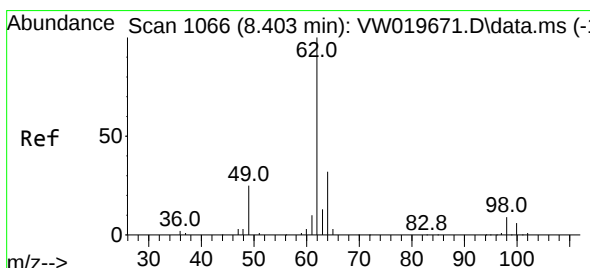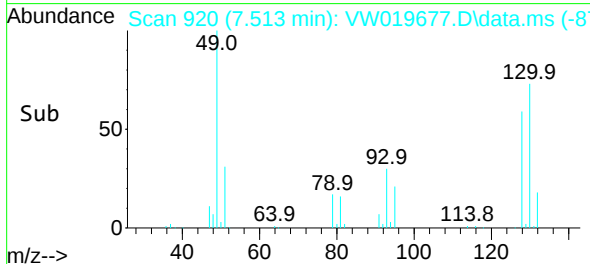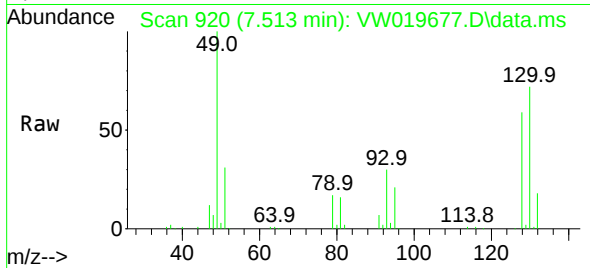

#27
1,2-Dichloroethane
Concen: 10.736 ug/L
RT: 8.403 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34


Tgt Ion: 62 Resp: 98900
Ion Ratio Lower Upper
62 100
98 9.4 6.9 10.3

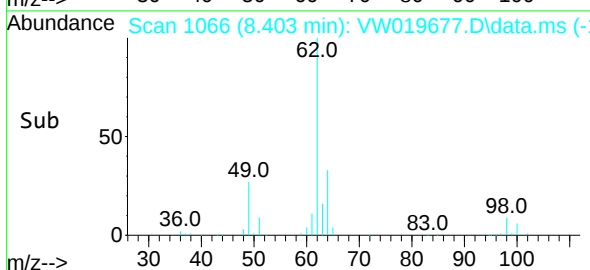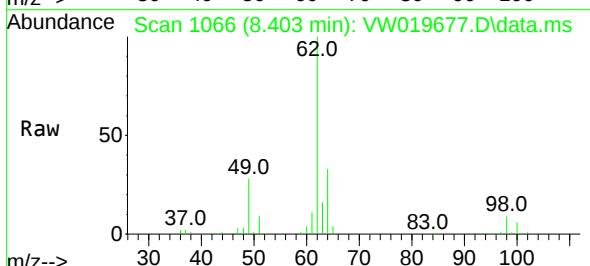






#29
Cyclohexane
Concen: 9.103 ug/L
RT: 7.958 min Scan# 993
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34


Instrument :
MSVOA_W
ClientSampleId :

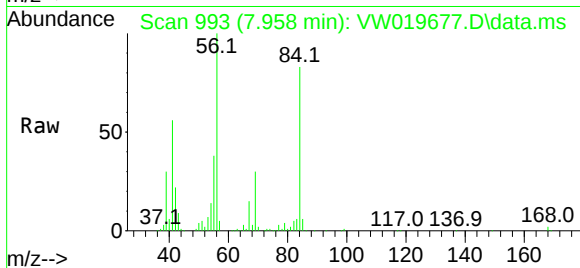



Tgt Ion: 56 Resp: 115277
Ion Ratio Lower Upper
56 100
69 31.7 24.5 36.7
84 87.0 75.0 112.4

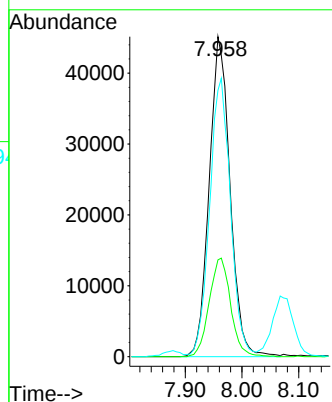


#30
1,1,1-Trichloroethane
Concen: 10.845 ug/L
RT: 7.878 min Scan# 980
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

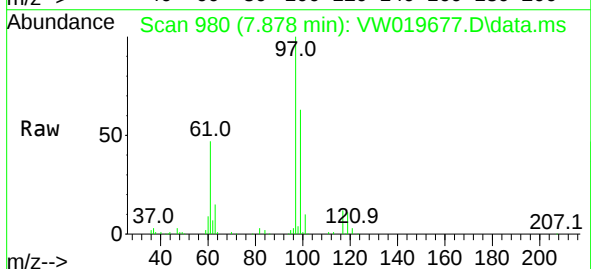

Tgt Ion: 97 Resp: 110523
Ion Ratio Lower Upper
97 100
99 64.1 51.4 77.2
61 48.1 37.8 56.6









#31
Carbon tetrachloride
Concen: 13.450 ug/L
RT: 8.073 min Scan# 1012
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampled :


Tgt Ion:117 Resp: 127538
Ion Ratio Lower Upper
117 100
119 95.5 76.5 114.7

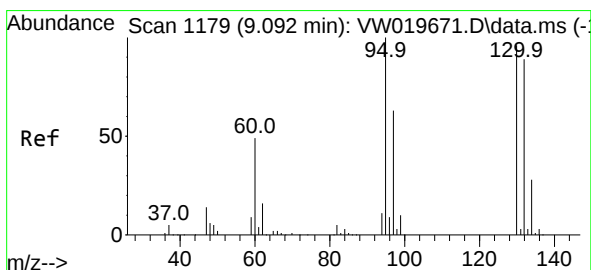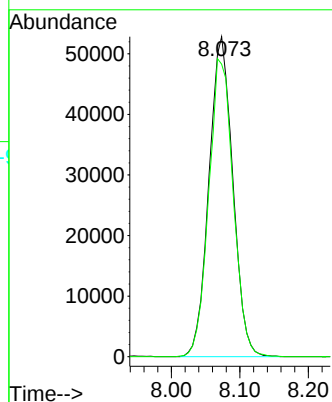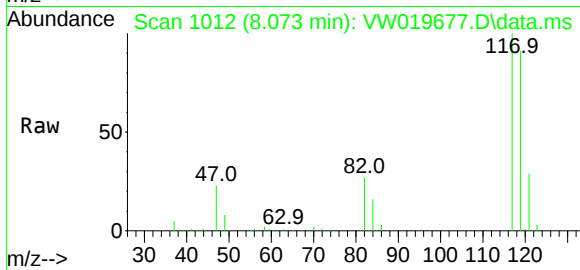

#34
Trichloroethene
Concen: 39.582 ug/L
RT: 9.091 min Scan# 1179
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

Tgt Ion: 95 Resp: 312247
Ion Ratio Lower Upper
95 100
97 64.8 47.3 87.8
132 85.6 71.0 131.8
130 98.9 65.1 120.9


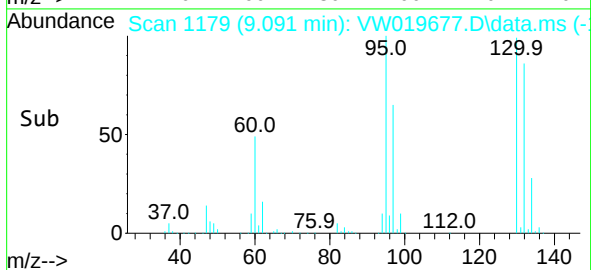

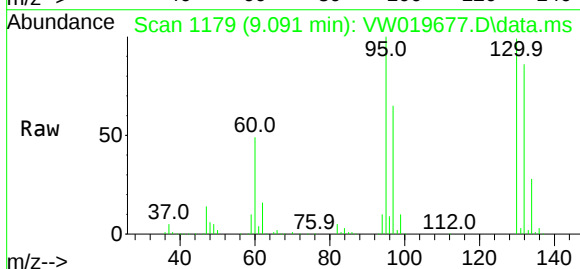




#35
Methylcyclohexane
Concen: 25.517 ug/L
RT: 9.335 min Scan# 1219
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampled :


Tgt Ion: 83 Resp: 356208
Ion Ratio Lower Upper
83 100
55 76.6 58.9 88.3
98 48.0 40.1 60.1

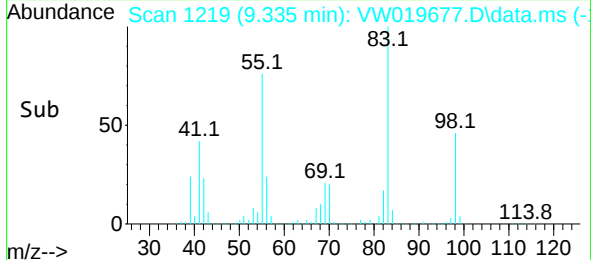

#37
1,2-Dichloropropane
Concen: 12.498 ug/L
RT: 9.372 min Scan# 1225
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

Tgt Ion: 63 Resp: 97891
Ion Ratio Lower Upper
63 100
112 4.7 3.9 5.9


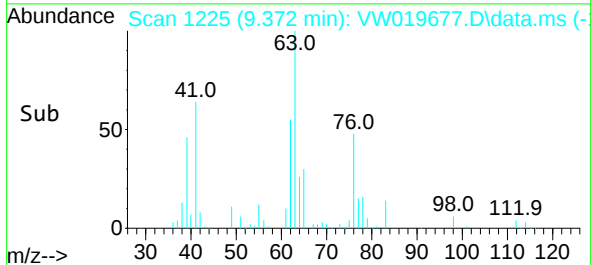

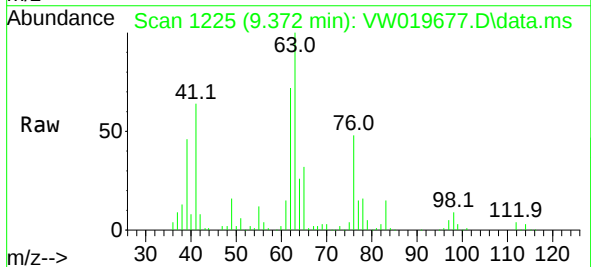




#38
Bromodichloromethane
Concen: 20.617 ug/L
RT: 9.646 min Scan# 1270
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 83 Resp: 200240
Ion Ratio Lower Upper
83 100
85 62.2 42.3 78.5
127 7.6 6.6 9.8

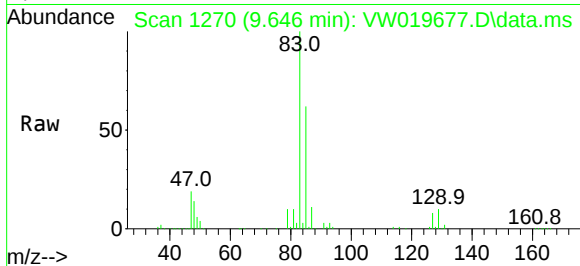

#39
cis-1,3-Dichloropropene
Concen: 16.114 ug/L
RT: 10.073 min Scan# 1340
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

Tgt Ion: 75 Resp: 193018
Ion Ratio Lower Upper
75 100
77 31.2 22.6 42.0

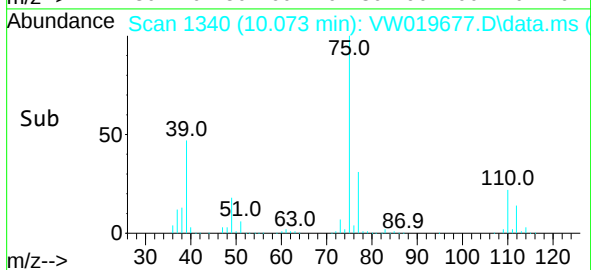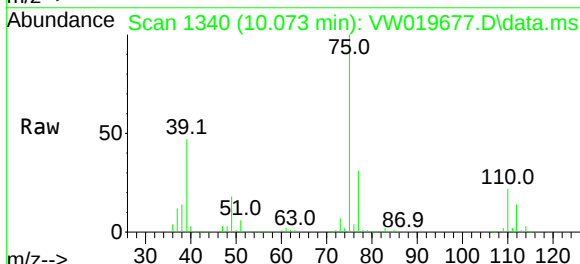



#42

Toluene

Concen: 20.451 ug/L

RT: 10.390 min Scan# 1392

Delta R.T. -0.000 min

Lab File: VW019677.D





Acq: 05 Aug 2021 12:34

Tgt Ion: 91 Resp: 658839

Ion Ratio Lower Upper

91 100

92 60.2 39.5 73.3



#44

trans-1,3-Dichloropropene

Concen: 7.617 ug/L

RT: 10.603 min Scan# 1427

Delta R.T. -0.006 min

Lab File: VW019677.D




Acq: 05 Aug 2021 12:34


Tgt Ion: 75 Resp: 80256

Ion Ratio Lower Upper

75 100

77 32.2 21.1 39.1


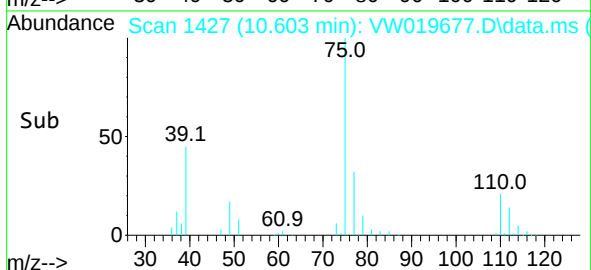






#46
Tetrachloroethene
Concen: 39.559 ug/L
RT: 10.866 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:164 Resp: 237844
Ion Ratio Lower Upper
164 100
129 97.1 66.7 123.9
131 94.8 61.1 113.5
166 133.7 87.0 161.6

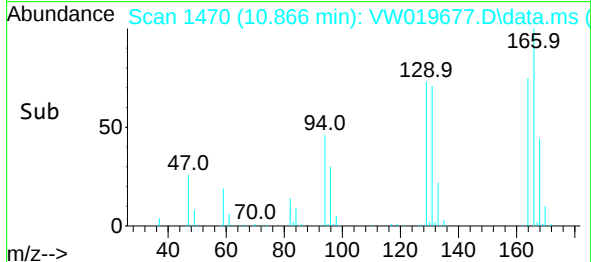

#48
2-Hexanone
Concen: 35.174 ug/L
RT: 10.969 min Scan# 1487
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

Tgt Ion: 43 Resp: 118432
Ion Ratio Lower Upper
43 100
58 56.5 42.7 64.1
57 19.4 15.8 23.8
100 13.0 10.0 15.0

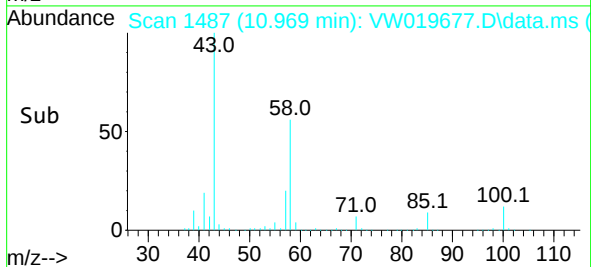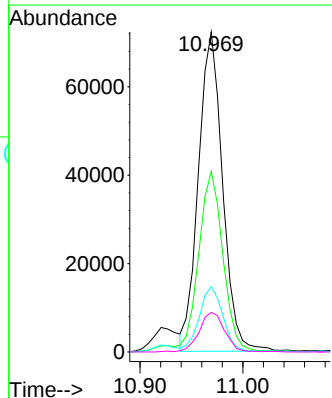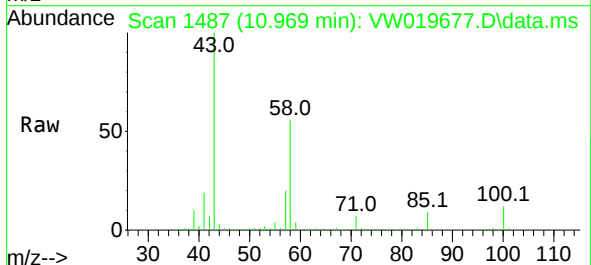



#49

Dibromochloromethane

Concen: 20.352 ug/L

RT: 11.128 min Scan# 1513

Delta R.T. -0.000 min

Lab File: VW019677.D





Acq: 05 Aug 2021 12:34

Tgt Ion:129 Resp: 127560

Ion Ratio Lower Upper

129 100

127 75.6 51.7 95.9

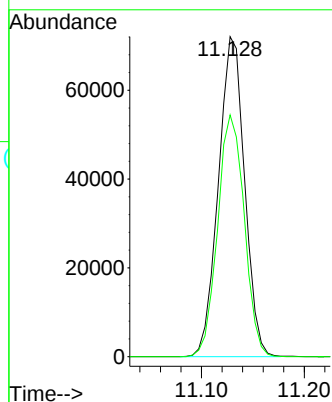

#52

Ethylbenzene

Concen: 15.335 ug/L

RT: 11.731 min Scan# 1612

Delta R.T. -0.000 min

Lab File: VW019677.D




Acq: 05 Aug 2021 12:34


Tgt Ion: 91 Resp: 537837

Ion Ratio Lower Upper

91 100

106 30.5 22.5 41.7


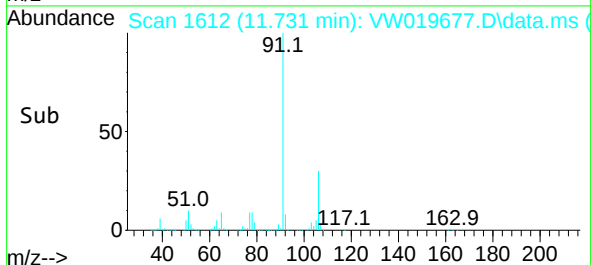

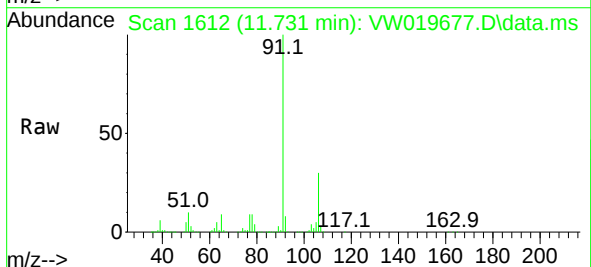




#53
m,p-Xylene
Concen: 10.053 ug/L
RT: 11.847 min Scan# 1631
Delta R.T. 0.006 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampled :


Tgt Ion:106 Resp: 133243
Ion Ratio Lower Upper
106 100
91 199.5 141.3 262.3

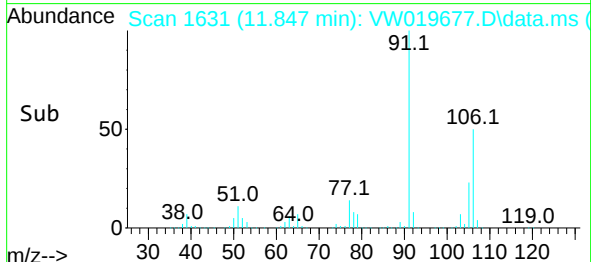

#54
o-Xylene
Concen: 12.156 ug/L
RT: 12.164 min Scan# 1683
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

Tgt Ion:106 Resp: 152254
Ion Ratio Lower Upper
106 100
91 221.0 150.0 278.6





#55

Styrene

Concen: 0.410 ug/L

RT: 12.164 min Scan# 1683

Delta R.T. -0.018 min

Lab File: VW019677.D

Acq: 05 Aug 2021 12:34

Tgt Ion:104 Resp: 8907

Ion Ratio Lower Upper





104 100

78 289.1 32.5 60.3#

Instrument :

MSVOA_W

ClientSampled :

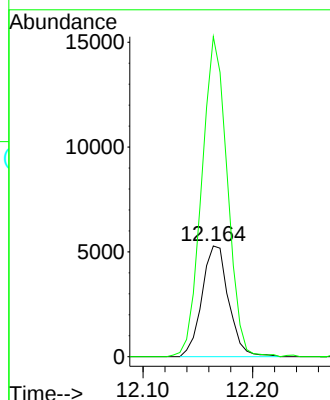

#60

Isopropylbenzene

Concen: 12.705 ug/L

RT: 12.463 min Scan# 1732

Delta R.T. -0.000 min

Lab File: VW019677.D

Acq: 05 Aug 2021 12:34




Tgt Ion:105 Resp: 423268


Ion Ratio Lower Upper

105 100

120 26.1 21.1 31.7

77 16.5 13.2 19.8


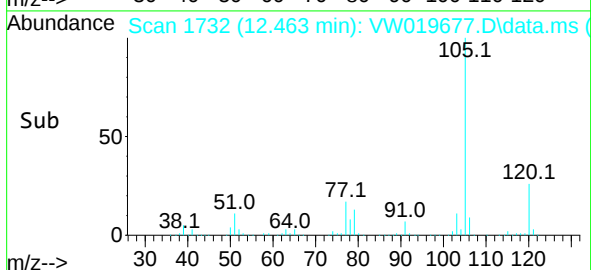
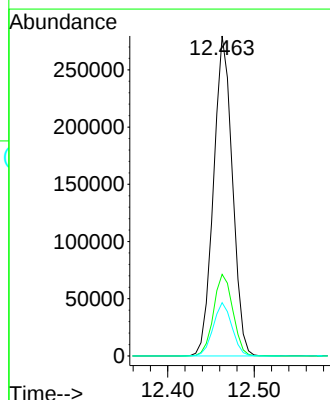





#61
1,2,3-Trichloropropane
Concen: 5.210 ug/L
RT: 12.743 min Scan# 1778
Delta R.T. -0.024 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampled :


Tgt Ion: 75 Resp: 28293
Ion Ratio Lower Upper
75 100
77 1189.7 25.3 37.9#
110 0.0 32.6 48.8#

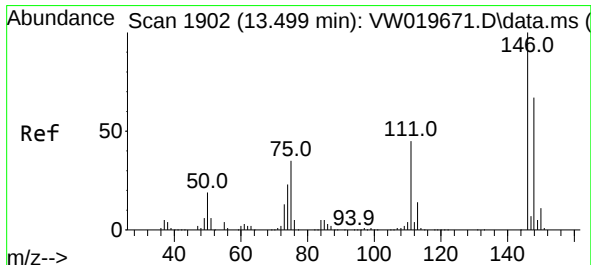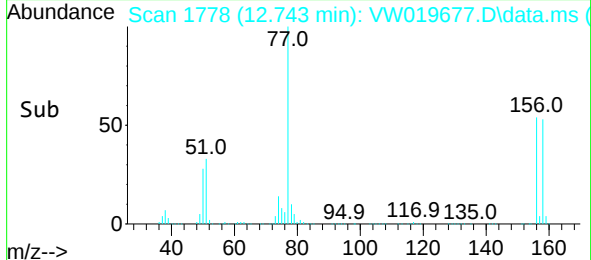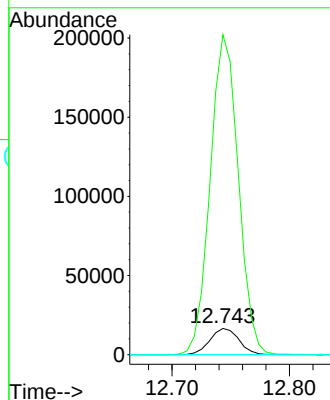

#64
1,3-Dichlorobenzene
Concen: 19.508 ug/L
RT: 13.499 min Scan# 1902
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34

Tgt Ion:146 Resp: 297404
Ion Ratio Lower Upper
146 100
111 41.0 26.7 49.7
148 68.5 41.1 76.3


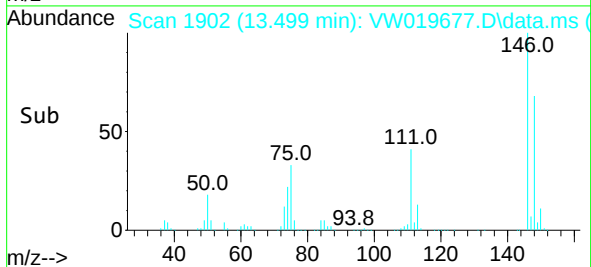
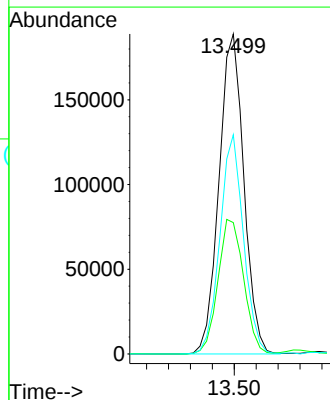
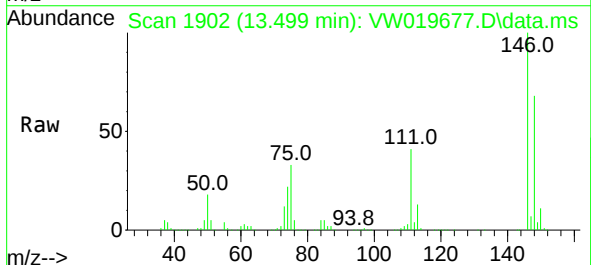




#67
1,2-Dichlorobenzene
Concen: 10.448 ug/L
RT: 13.865 min Scan# 1962
Delta R.T. -0.006 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:146 Resp: 143499
Ion Ratio Lower Upper
146 100
111 45.1 33.2 49.8
148 64.8 50.4 75.6

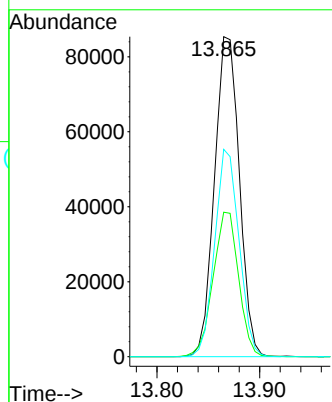

#68
1,2-Dibromo-3-chloropropane
Concen: 20.525 ug/L
RT: 14.481 min Scan# 2063
Delta R.T. -0.000 min
Lab File: VW019677.D
Acq: 05 Aug 2021 12:34


Tgt Ion: 75 Resp: 24322
Ion Ratio Lower Upper
75 100
155 65.1 59.4 89.0
157 94.3 72.2 108.2

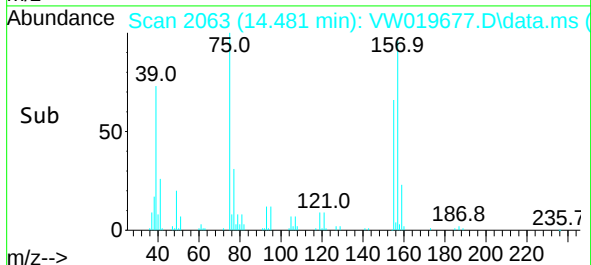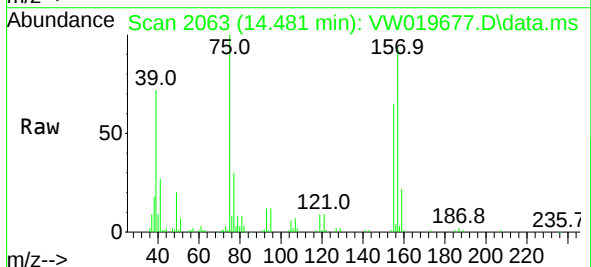



#69
 1,3,5-Trichlorobenzene
 Concen: 24.270 ug/L
 RT: 14.627 min Scan# 2087
 Delta R.T. -0.000 min
 Lab File: VW019677.D
 Acq: 05 Aug 2021 12:34

Instrument :
 MSVOA_W
 ClientSampleId :

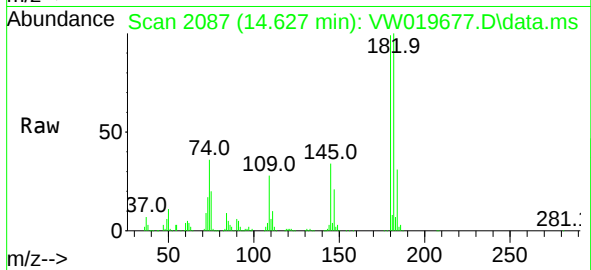

Tgt Ion:	180	Resp:	270354
Ion	Ratio	Lower	Upper
180	100		
182	94.2	73.4	110.2
184	30.1	23.6	35.4
145	31.6	24.9	37.3

