
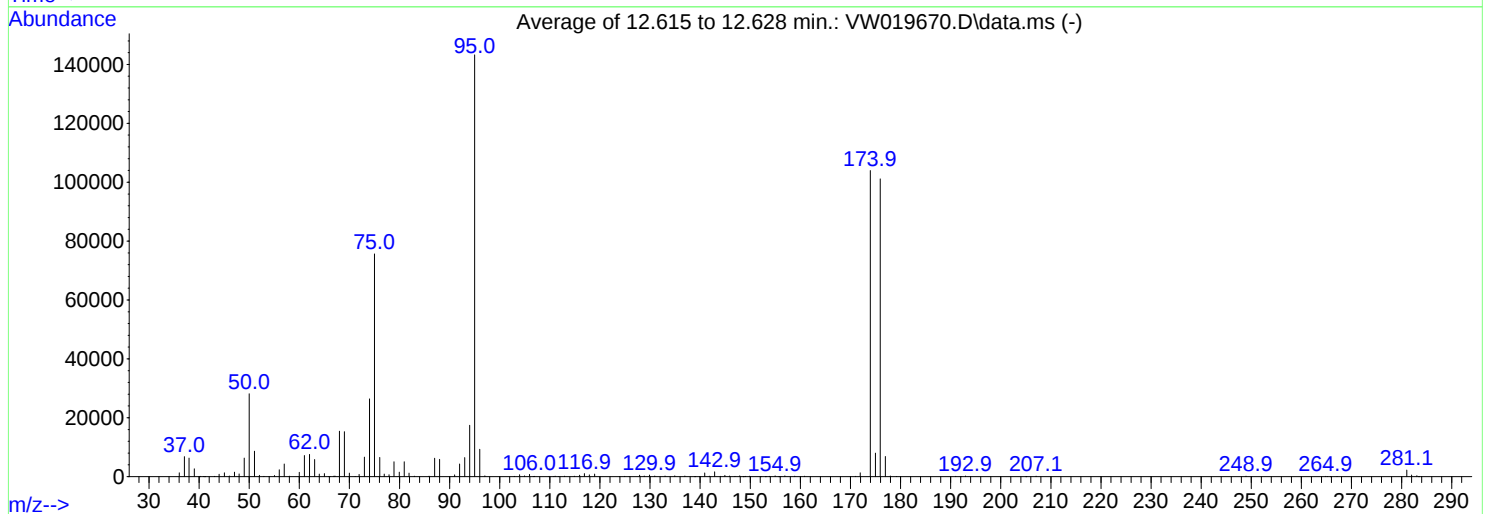


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080521\
 Data File : VW019670.D
 Acq On : 05 Aug 2021 08:49
 Operator : SY/VA
 Sample : BFB412
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB412

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Title : SFAM01.0
 Last Update : Sat Aug 07 01:03:00 2021

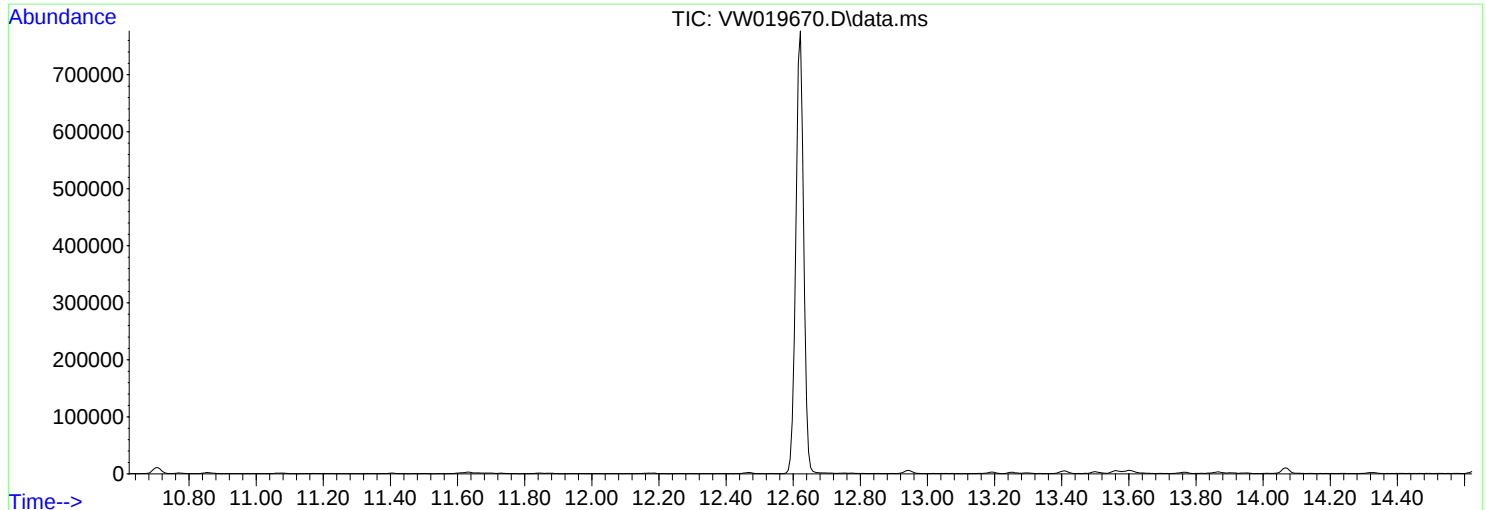

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	28147	PASS
75	95	30	80	52.8	75672	PASS
95	95	100	100	100.0	143267	PASS
96	95	5	9	6.5	9296	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.6	103955	PASS
175	174	5	9	7.7	8009	PASS
176	174	95	105	97.3	101136	PASS
177	176	5	10	6.8	6865	PASS

m/z	Abundance
36.00	1155.0
37.00	5511.0
38.10	4545.0
39.10	2049.0
40.20	289.0
41.10	61.0
43.00	86.0
44.00	987.0
45.00	942.0
46.10	133.0
47.00	1370.0
48.10	770.0
49.00	4953.0
50.00	21808.0
51.10	6794.0
52.10	365.0
55.00	265.0
56.00	1999.0
57.00	3551.0
58.00	144.0
60.00	1123.0
61.00	5291.0
62.00	6007.0
63.00	4593.0
64.00	554.0
65.00	873.0
66.20	112.0
67.10	194.0
68.00	12097.0
69.00	12526.0
70.00	996.0
71.20	54.0
72.00	680.0
73.00	5227.0
74.00	21072.0
75.00	60032.0
76.00	4940.0
77.00	612.0
77.80	462.0
78.90	4279.0
79.90	1390.0
80.90	4202.0
81.90	1061.0
83.00	176.0
85.80	122.0
87.00	4963.0
88.00	5084.0
91.00	498.0
92.00	3615.0
93.00	5307.0
94.00	14231.0
95.00	118440.0
96.00	6900.0
97.00	217.0
104.00	523.0
104.80	187.0
105.10	186.0
105.90	601.0
106.70	158.0
109.90	167.0
111.00	141.0
111.80	86.0
112.90	111.0
114.80	100.0
116.00	493.0
116.90	860.0
117.90	422.0
118.90	767.0
127.80	475.0
128.80	229.0
129.90	491.0
130.90	198.0
132.90	74.0
135.00	258.0
136.90	251.0
138.90	63.0
139.80	60.0
140.90	978.0
141.80	170.0
142.90	1341.0
144.00	97.0
145.00	272.0
145.90	198.0
146.90	94.0
147.80	205.0
148.90	74.0
149.90	97.0
153.90	120.0
154.90	282.0
156.10	62.0
156.90	291.0
158.80	148.0

Instrument :
MSVOA_W
ClientSampleId :
BFB412

160.90	175.0
170.90	101.0
171.90	997.0
173.90	99832.0
175.00	7976.0
176.00	91792.0
177.00	5992.0
177.90	193.0
190.90	73.0
207.00	75.0
248.90	118.0
281.10	940.0
282.10	230.0
283.00	96.0
283.40	70.0

Instrument :
MSVOA_W
ClientSampleId :
BFB412

Scan 1749 (12.567 min): VW019670.D\data.ms
BFB412

m/z	Abundance
40.00	183.0
44.10	249.0

Instrument :
MSVOA_W
ClientSampleId :
BFB412

m/z	Abundance
36.10	1431.0
37.00	7429.0
38.00	6968.0
39.00	3088.0
40.00	331.0
40.90	81.0
43.10	163.0
44.00	1261.0
45.00	1351.0
46.00	265.0
47.10	1543.0
48.00	976.0
49.00	7015.0
50.00	30712.0
51.10	9508.0
52.00	398.0
52.90	108.0
54.00	67.0
55.10	415.0
56.00	2584.0
57.00	4623.0
58.00	243.0
60.00	1578.0
61.00	8382.0
62.00	8497.0
63.00	6455.0
64.10	1100.0
65.00	1255.0
65.90	173.0
66.90	473.0
68.00	16576.0
69.00	16141.0
70.00	1443.0
71.20	83.0
71.90	887.0
73.00	7418.0
74.00	29008.0
75.00	81328.0
76.00	7288.0
76.90	887.0
77.90	781.0
78.90	5511.0
79.90	1509.0
81.00	5423.0
81.90	1152.0
83.00	173.0
85.90	265.0
87.00	6468.0
88.00	6202.0
91.00	585.0
92.00	4854.0
93.00	6560.0
94.00	18408.0
95.00	146752.0
96.00	10140.0
97.00	359.0
102.90	185.0
103.90	666.0
105.00	176.0
105.90	844.0
107.00	139.0
109.80	91.0
110.80	155.0
111.20	121.0
113.00	138.0
114.90	143.0
115.90	517.0
116.90	1098.0
117.90	674.0
119.00	1057.0
123.90	79.0
125.00	161.0
125.90	144.0
128.00	505.0
128.90	272.0
129.90	562.0
130.90	230.0
133.00	315.0
134.90	204.0
136.90	276.0
140.00	53.0
140.90	1656.0
141.90	211.0
142.90	1706.0
144.10	86.0
144.90	557.0
145.90	186.0
146.90	119.0
147.90	295.0
148.60	92.0
149.20	131.0
149.90	226.0

Instrument :
MSVOA_W
ClientSampleId :
BFB412

153.00	57.0
153.70	60.0
155.00	388.0
156.10	61.0
156.90	218.0
158.90	189.0
160.80	136.0
171.00	197.0
172.10	1325.0
173.90	100128.0
175.00	7962.0
176.00	96216.0
177.00	6859.0
178.00	170.0
179.20	96.0
191.10	161.0
191.90	57.0
192.90	420.0
194.00	94.0
205.00	88.0
207.00	259.0
248.90	263.0
250.10	108.0
264.80	269.0
265.20	167.0
267.10	130.0
281.10	3538.0
282.00	903.0
283.10	491.0
284.00	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB412

m/z	Abundance
36.00	1321.0
37.10	7441.0
38.00	7407.0
39.00	2928.0
40.00	289.0
40.80	61.0
43.20	94.0
44.00	1040.0
45.10	1557.0
46.10	206.0
47.00	1692.0
47.90	1099.0
49.00	6951.0
50.00	31920.0
51.00	9605.0
52.00	559.0
53.00	159.0
54.00	75.0
55.00	445.0
56.00	2464.0
57.00	4710.0
58.00	121.0
60.00	1752.0
61.00	7922.0
62.10	8218.0
63.10	6430.0
63.90	951.0
65.00	996.0
66.10	99.0
67.10	412.0
68.00	17600.0
69.00	17096.0
70.00	1232.0
71.10	74.0
72.00	757.0
73.00	7339.0
74.00	29176.0
75.00	85656.0
76.10	7382.0
77.00	1090.0
77.90	766.0
78.90	5413.0
80.00	1631.0
80.90	5574.0
81.90	1431.0
82.90	142.0
85.90	168.0
87.00	7329.0
88.00	6292.0
91.00	649.0
92.00	4404.0
93.00	7519.0
94.00	19704.0
95.00	164608.0
96.00	10849.0
97.10	243.0
102.90	108.0
104.00	764.0
104.90	227.0
106.00	807.0
106.90	142.0
109.90	83.0
111.00	179.0
111.80	162.0
113.00	182.0
114.90	197.0
115.90	454.0
116.90	1181.0
117.90	731.0
118.90	781.0
123.90	103.0
124.90	104.0
125.80	111.0
127.90	441.0
128.80	241.0
129.90	542.0
131.00	279.0
133.00	221.0
135.00	294.0
137.00	208.0
139.90	59.0
140.90	1179.0
141.80	152.0
142.90	1831.0
144.10	95.0
145.00	498.0
145.80	264.0
147.00	122.0
147.90	395.0
149.00	127.0
149.90	112.0
152.00	66.0

Instrument :
MSVOA_W
ClientSampleId :
BFB412

153.80	136.0
155.00	236.0
155.70	66.0
156.90	256.0
159.00	157.0
160.80	183.0
171.10	111.0
171.90	1544.0
174.00	111904.0
175.00	8090.0
175.90	115400.0
176.90	7745.0
177.90	251.0
191.00	167.0
193.00	293.0
194.00	52.0
207.10	160.0
249.00	121.0
264.90	159.0
265.80	50.0
281.00	2146.0
282.00	471.0
283.00	352.0
284.00	101.0

Instrument :
MSVOA_W
ClientSampleId :
BFB412