

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
 Data File : VW024183.D
 Acq On : 05 Aug 2022 10:10
 Operator : SY/VA
 Sample : VW0805SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK570

Quant Time: Aug 05 23:44:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 23:43:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	441947	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	413711	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	207398	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	188461	20.401	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.600%
7) Chloroethane-d5	2.879	69	108646	18.880	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.520%
11) 1,1-Dichloroethene-d2	4.013	63	169888	16.137	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.560%
21) 2-Butanone-d5	7.086	46	75872	44.146	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.300%
24) Chloroform-d	7.647	84	277104	20.722	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.880%
26) 1,2-Dichloroethane-d4	8.305	65	153064	20.617	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.480%
32) Benzene-d6	8.275	84	554326	22.719	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.880%
36) 1,2-Dichloropropane-d6	9.274	67	160079	22.221	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.880%
41) Toluene-d8	10.323	98	513490	22.516	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.080%
43) trans-1,3-Dichloroprop...	10.573	79	71026	22.510	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.040%
47) 2-Hexanone-d5	10.920	63	62425	46.915	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.820%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	144280	20.643	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	183928	24.235	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.920%
Target Compounds					Qvalue	
13) Acetone	4.135	43	4299	3.398	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
Data File : VW024183.D
Acq On : 05 Aug 2022 10:10
Operator : SY/VA
Sample : VW0805SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK570

Quant Time: Aug 05 23:44:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 23:43:03 2022
Response via : Initial Calibration

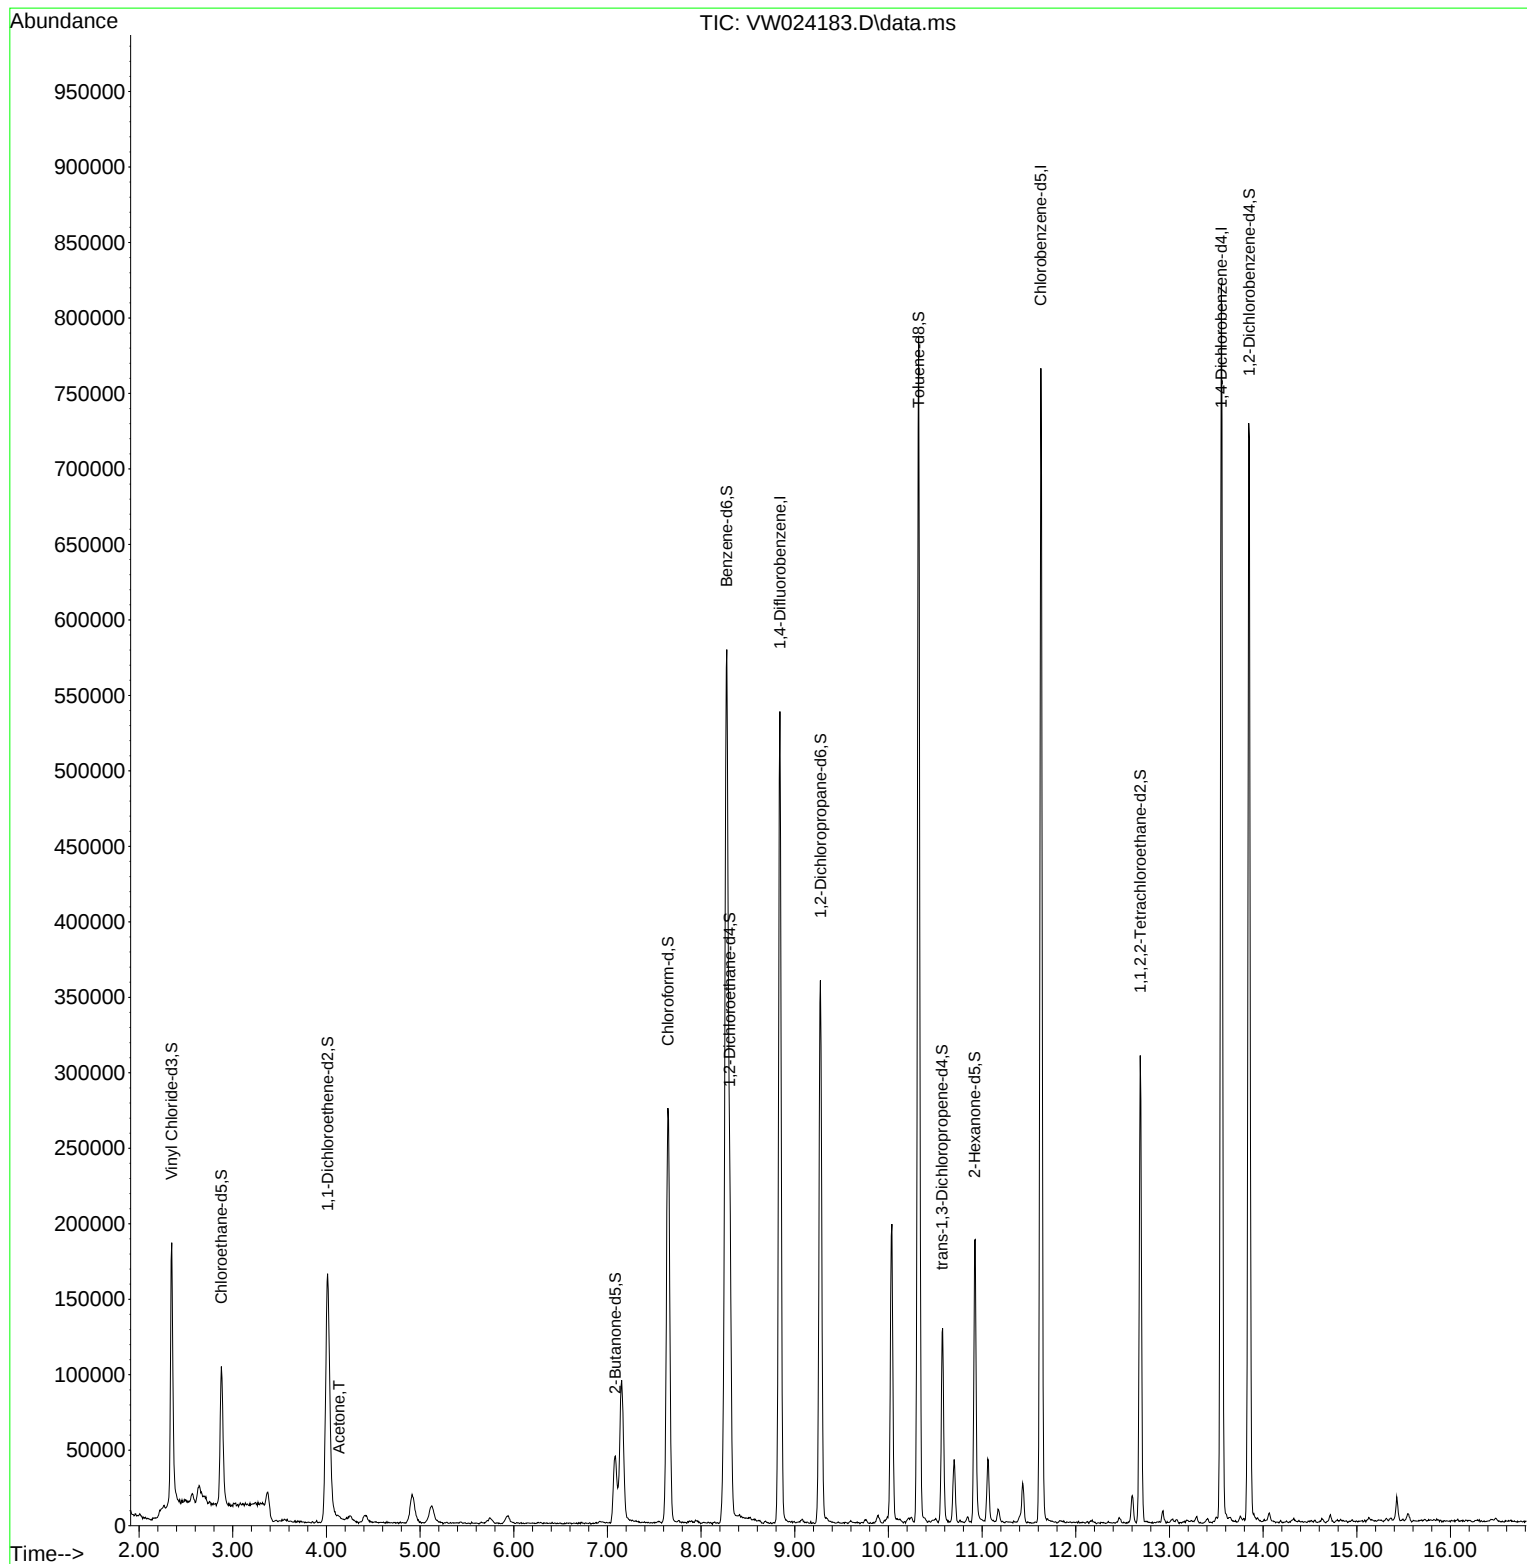

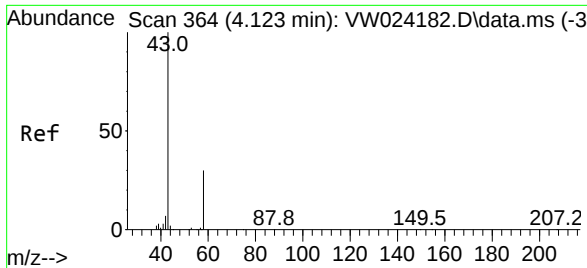

#13
 Acetone
 Concen: 3.398 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW024183.D
 Acq: 05 Aug 2022 10:10

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK570

Tgt Ion: 43 Resp: 4299
 Ion Ratio Lower Upper
 43 100
 58 16.3 0.0 31.8

