
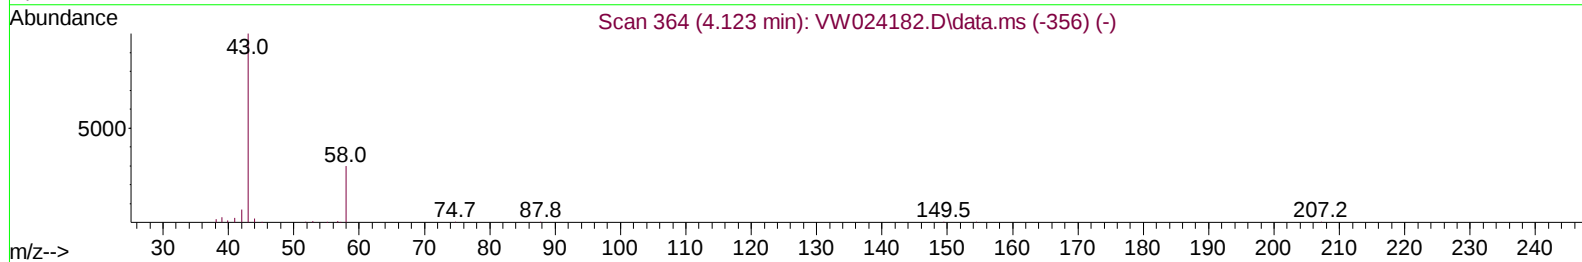
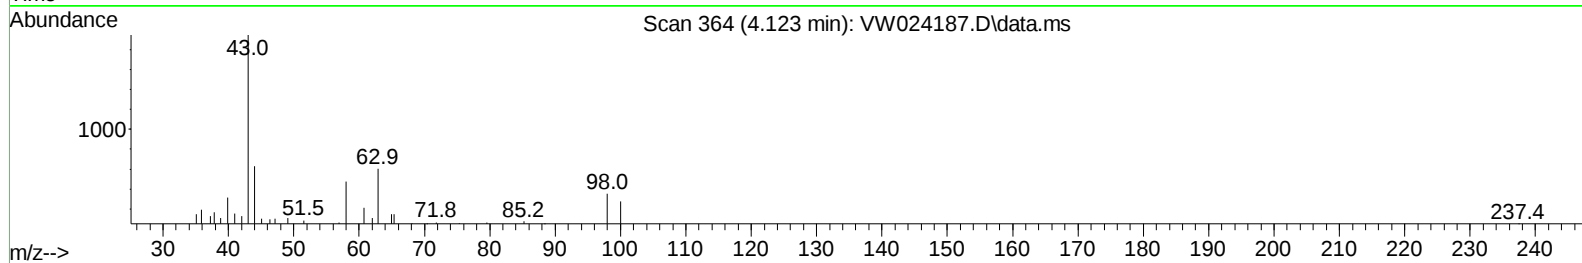


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
Data File : VW024187.D
Acq On : 05 Aug 2022 13:07
Operator : SY/VA
Sample : N4030-03
Misc : 6.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:45:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 23:43:03 2022
Response via : Initial Calibration

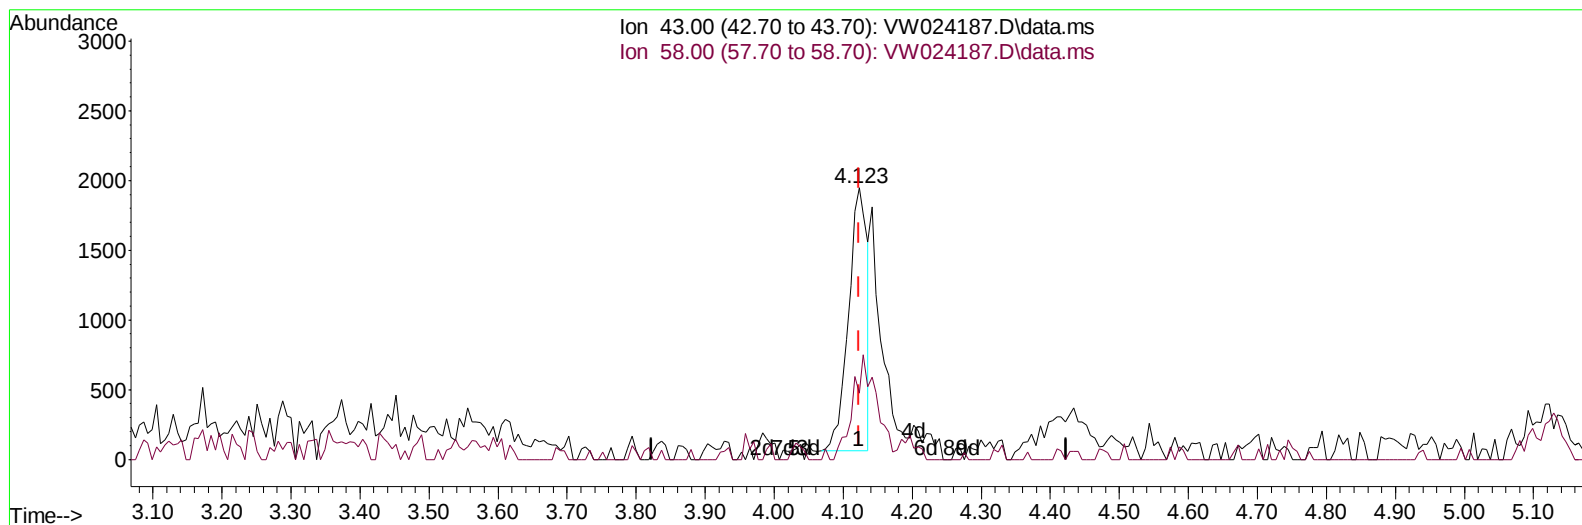

TIC: VW024187.D\data.ms

(13) Acetone (T)




4.123min (+ 0.000) 2.68 ug/L

response 3516

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	31.57
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
Data File : VW024187.D
Acq On : 05 Aug 2022 13:07
Operator : SY/VA
Sample : N4030-03
Misc : 6.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:45:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 23:43:03 2022
Response via : Initial Calibration

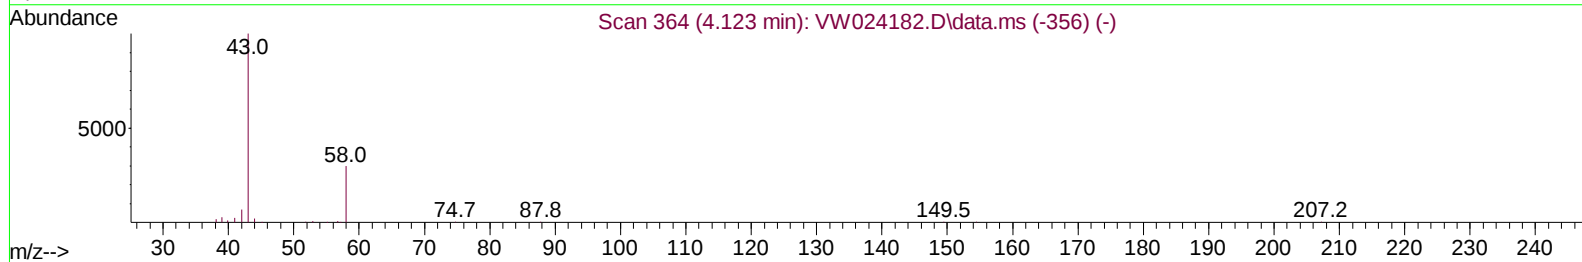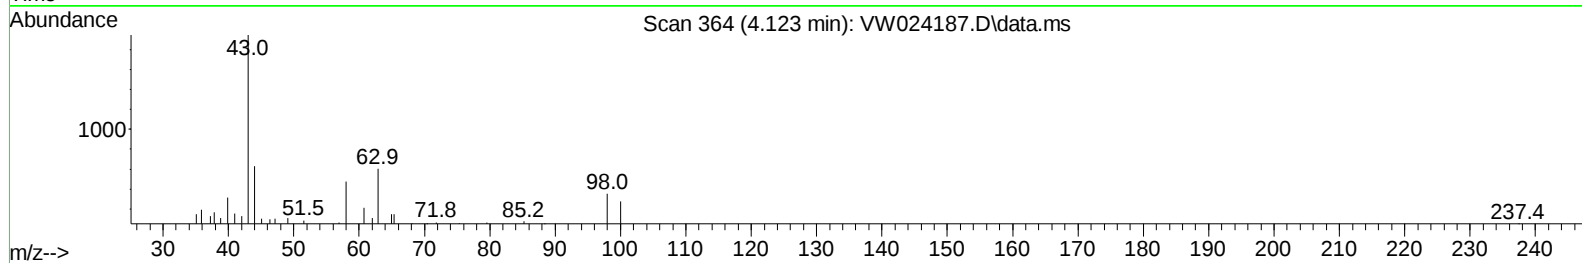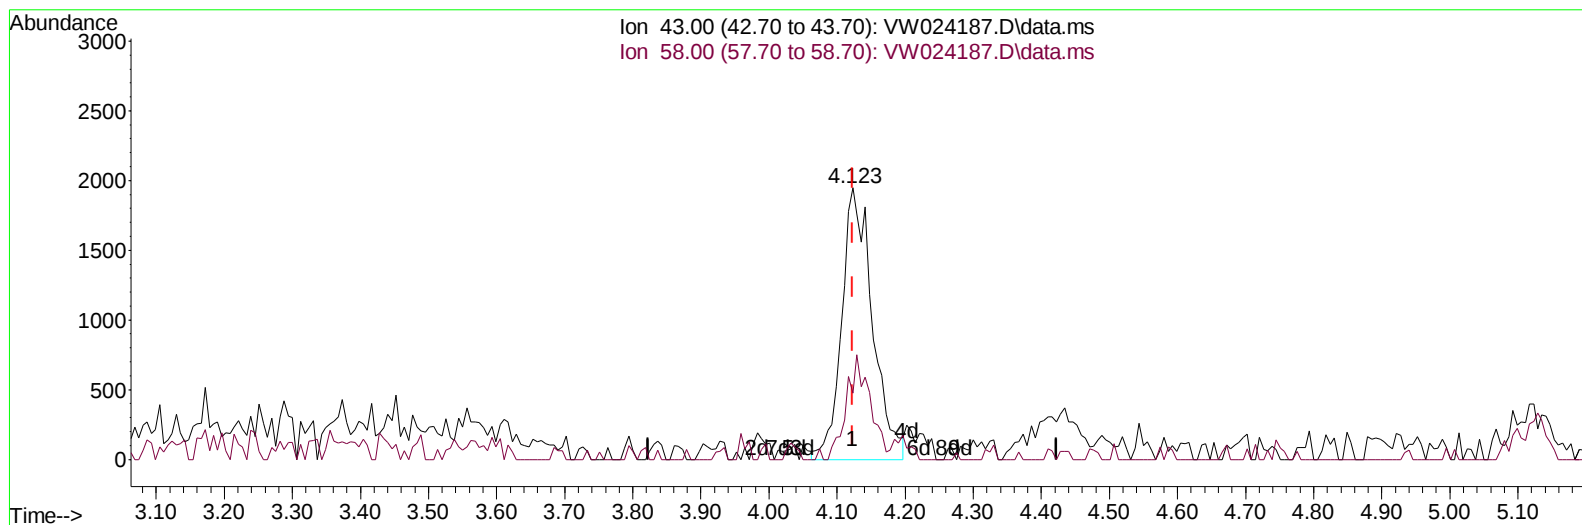

TIC: VW024187.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 4.63 ug/L m

response 6062

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	18.31
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
 Data File : VW024187.D
 Acq On : 05 Aug 2022 13:07
 Operator : SY/VA
 Sample : N4030-03
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:45:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 23:43:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.836	114	457676	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	416423	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	205797	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	252306	26.374	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	105.480%	
7) Chloroethane-d5	2.873	69	133913	22.471	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	89.880%	
11) 1,1-Dichloroethene-d2	3.995	63	197480	18.113	ug/L	-0.02
Spiked Amount 25.000	Range 45	- 110	Recovery	=	72.440%	
21) 2-Butanone-d5	7.080	46	77860	43.746	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	87.500%	
24) Chloroform-d	7.641	84	318737	23.017	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.080%	
26) 1,2-Dichloroethane-d4	8.299	65	176043	22.897	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	91.600%	
32) Benzene-d6	8.269	84	633226	25.784	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	103.120%	
36) 1,2-Dichloropropane-d6	9.269	67	182853	25.217	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	100.880%	
41) Toluene-d8	10.317	98	601150	26.188	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	104.760%	
43) trans-1,3-Dichloroprop...	10.573	79	80889	25.469	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	101.880%	
47) 2-Hexanone-d5	10.921	63	63738	47.589	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	95.180%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	157055	22.324	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	89.280%	
66) 1,2-Dichlorobenzene-d4	13.847	152	199177	26.448	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	105.800%	
Target Compounds						
13) Acetone	4.123	43	6062m	4.626	ug/L	
16) Methylene chloride	4.903	84	42758	5.298	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
Data File : VW024187.D
Acq On : 05 Aug 2022 13:07
Operator : SY/VA
Sample : N4030-03
Misc : 6.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:45:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 23:43:03 2022
Response via : Initial Calibration

