
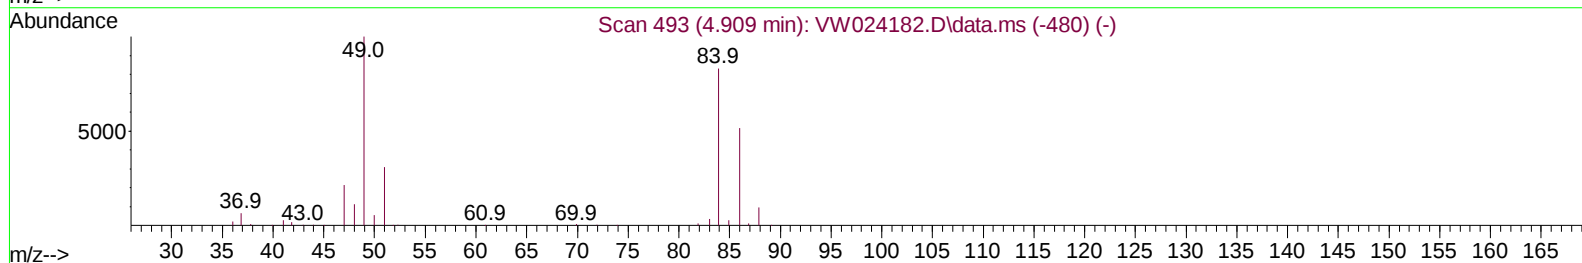
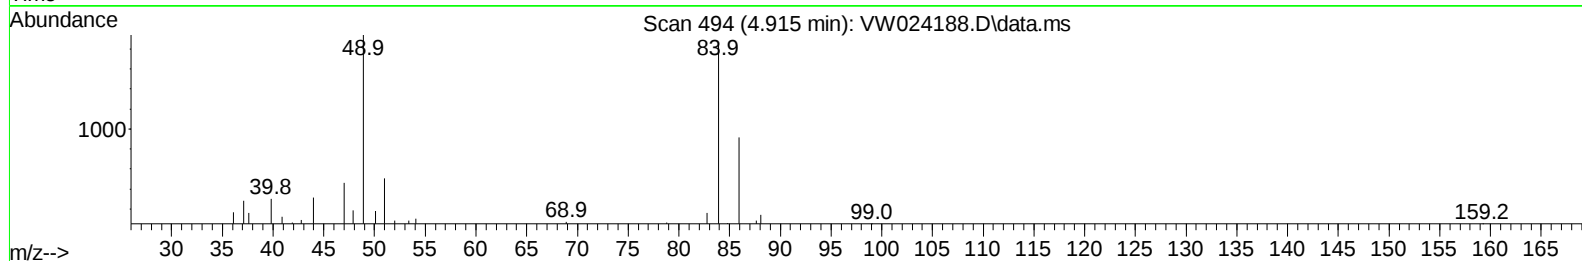


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
Data File : VW024188.D
Acq On : 05 Aug 2022 13:32
Operator : SY/VA
Sample : N4030-04
Misc : 5.16g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:45:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 23:43:03 2022
Response via : Initial Calibration

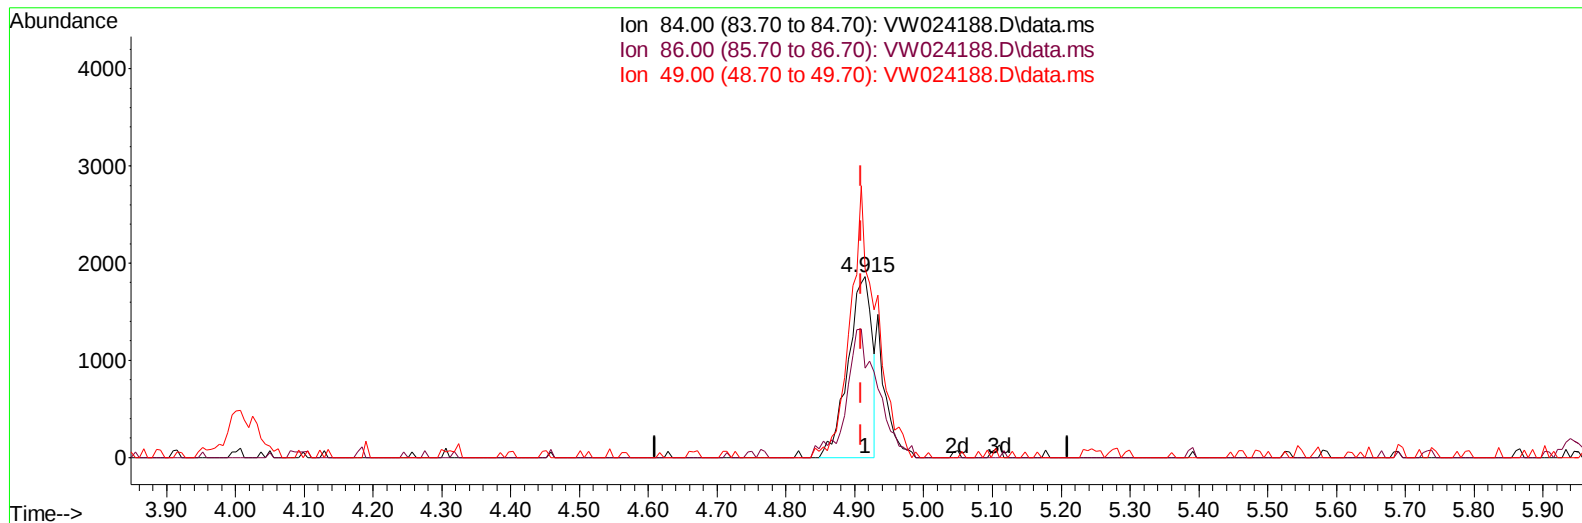

TIC: VW024188.D\data.ms

(16) Methylene chloride (T)




4.915min (+ 0.006) 4.86 ug/L

response 4435

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	49.38
49.00	121.80	104.30
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
Data File : VW024188.D
Acq On : 05 Aug 2022 13:32
Operator : SY/VA
Sample : N4030-04
Misc : 5.16g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:45:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 23:43:03 2022
Response via : Initial Calibration

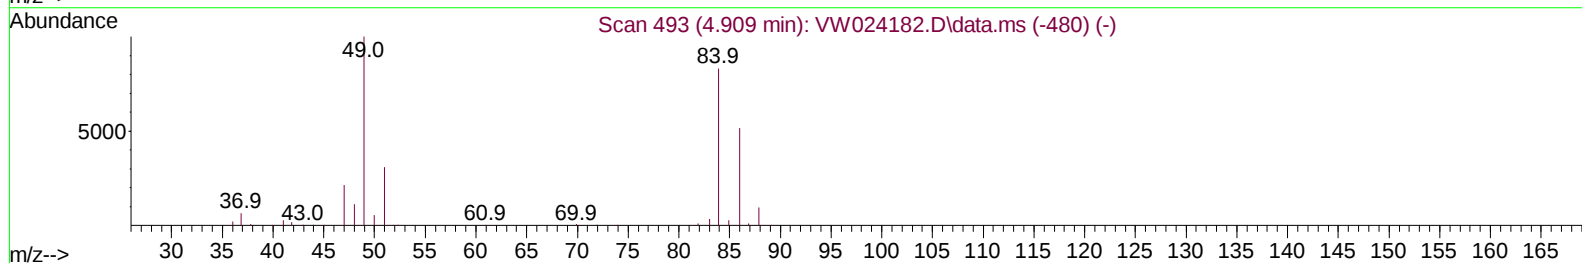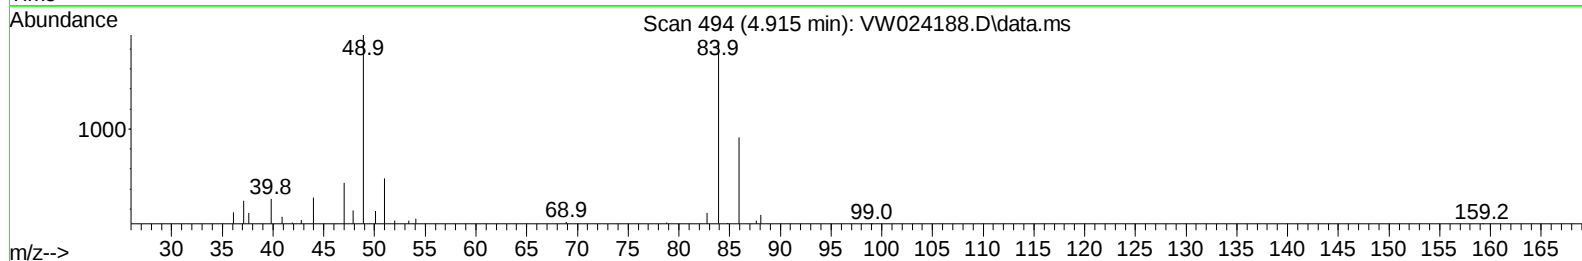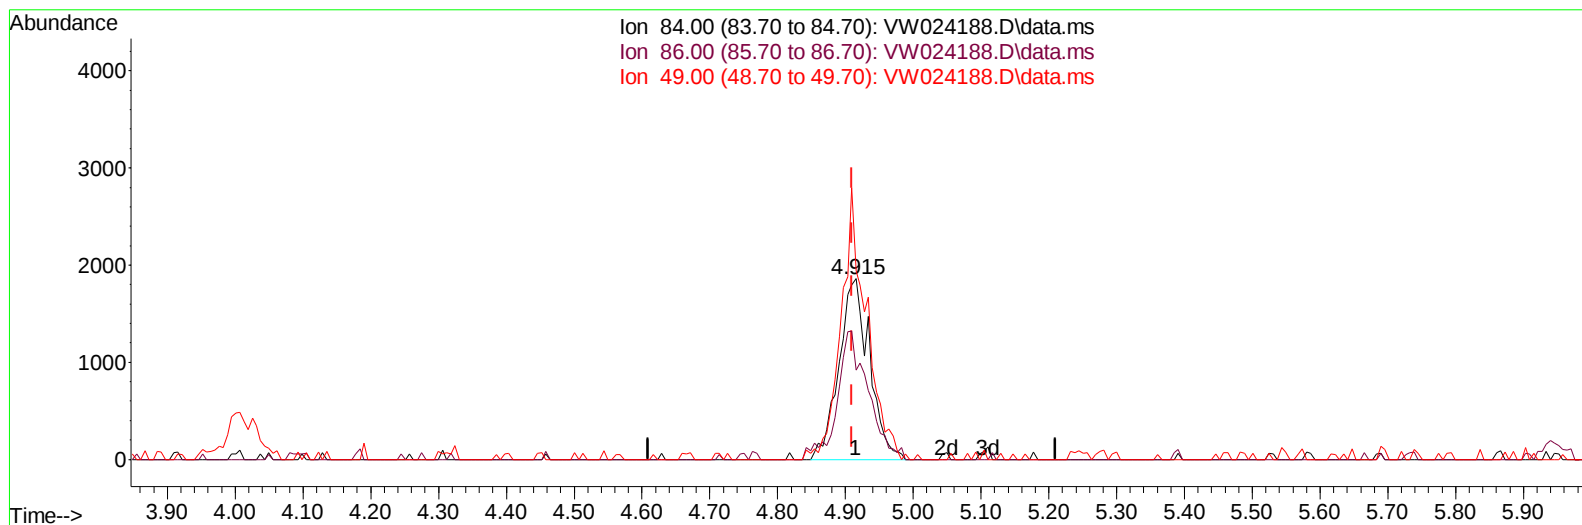

TIC: VW024188.D\data.ms

(16) Methylene chloride (T)

4.915min (+ 0.006) 6.39 ug/L m

response 5837

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	49.38
49.00	121.80	104.30
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
 Data File : VW024188.D
 Acq On : 05 Aug 2022 13:32
 Operator : SY/VA
 Sample : N4030-04
 Misc : 5.16g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:45:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 23:43:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	51801	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	48234	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	20441	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	33122	30.590	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 122.360%			
7) Chloroethane-d5	2.873	69	22681	33.626	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 134.520%			
11) 1,1-Dichloroethene-d2	4.013	63	27356	22.169	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 88.680%			
21) 2-Butanone-d5	7.080	46	10028	49.781	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 99.560%			
24) Chloroform-d	7.647	84	39495	25.198	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 100.800%			
26) 1,2-Dichloroethane-d4	8.305	65	24687	28.370	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 113.480%			
32) Benzene-d6	8.274	84	78020	27.427	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 109.720%			
36) 1,2-Dichloropropane-d6	9.274	67	23357	27.809	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 111.240%			
41) Toluene-d8	10.323	98	62755	23.602	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 94.400%			
43) trans-1,3-Dichloroprop...	10.579	79	9579	26.039	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 104.160%			
47) 2-Hexanone-d5	10.926	63	6050	38.999	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 78.000%			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	21785	26.734	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 106.920%			
66) 1,2-Dichlorobenzene-d4	13.853	152	19456	26.010	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 104.040%			
Target Compounds						
16) Methylene chloride	4.915	84	5837m	6.390	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
Data File : VW024188.D
Acq On : 05 Aug 2022 13:32
Operator : SY/VA
Sample : N4030-04
Misc : 5.16g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:45:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 23:43:03 2022
Response via : Initial Calibration

