
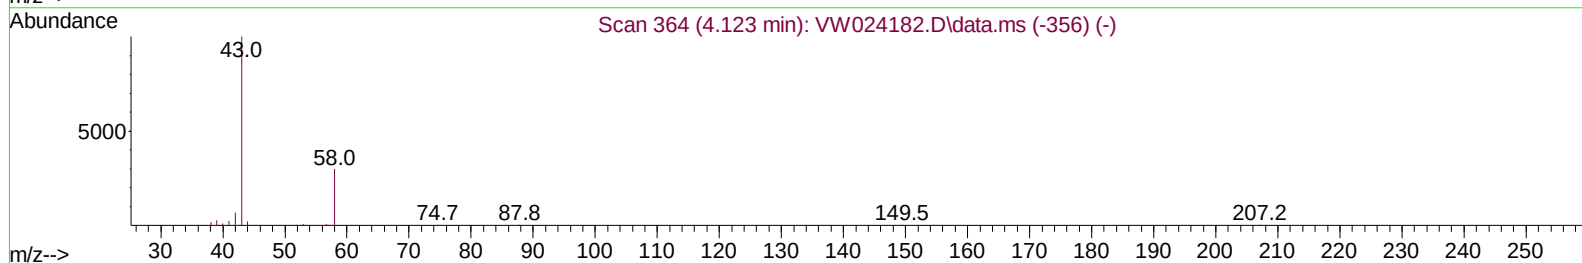
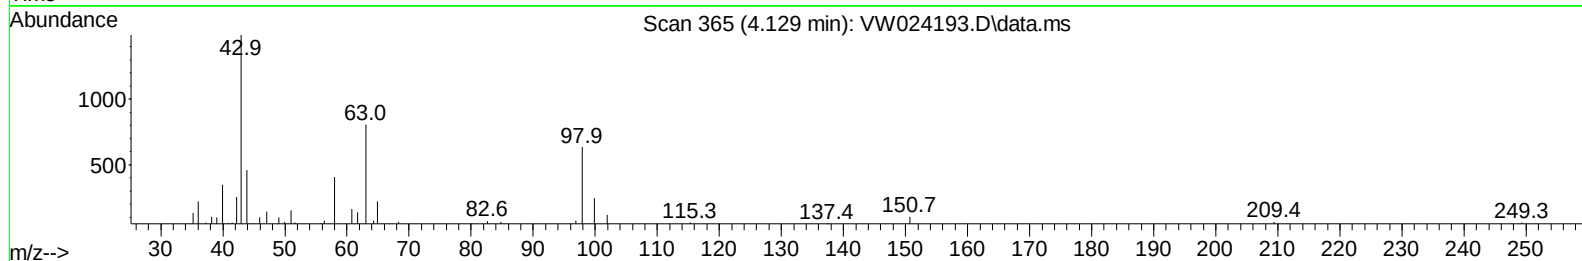


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
Data File : VW024193.D
Acq On : 05 Aug 2022 15:35
Operator : SY/VA
Sample : N4030-01
Misc : 4.67g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:46:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 23:43:03 2022
Response via : Initial Calibration

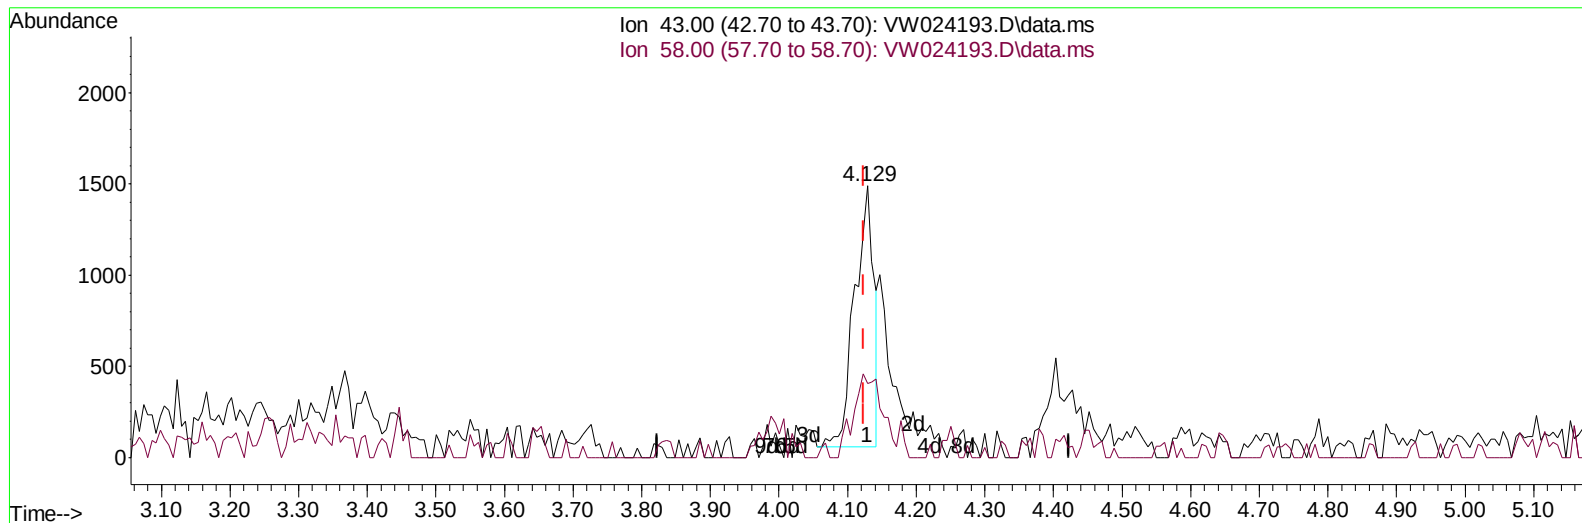

TIC: VW024193.D\data.ms

(13) Acetone (T)




4.129min (+ 0.006) 3.04 ug/L

response 2749

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	13.24
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
Data File : VW024193.D
Acq On : 05 Aug 2022 15:35
Operator : SY/VA
Sample : N4030-01
Misc : 4.67g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:46:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 23:43:03 2022
Response via : Initial Calibration

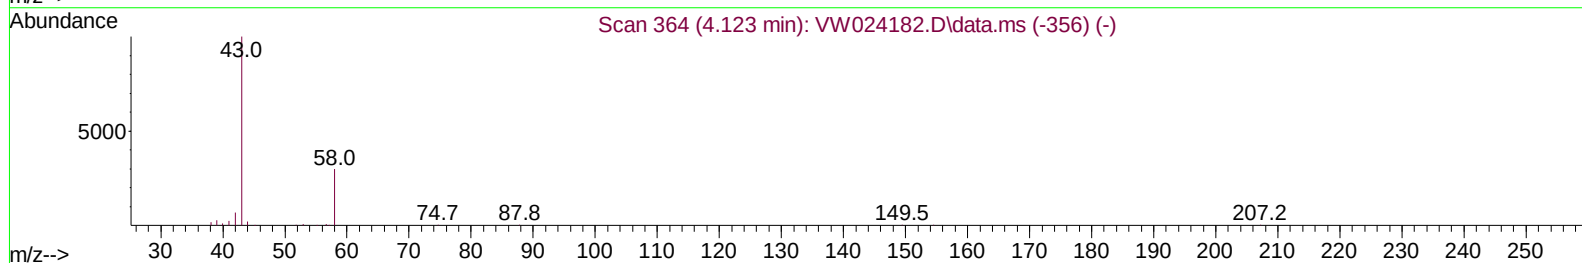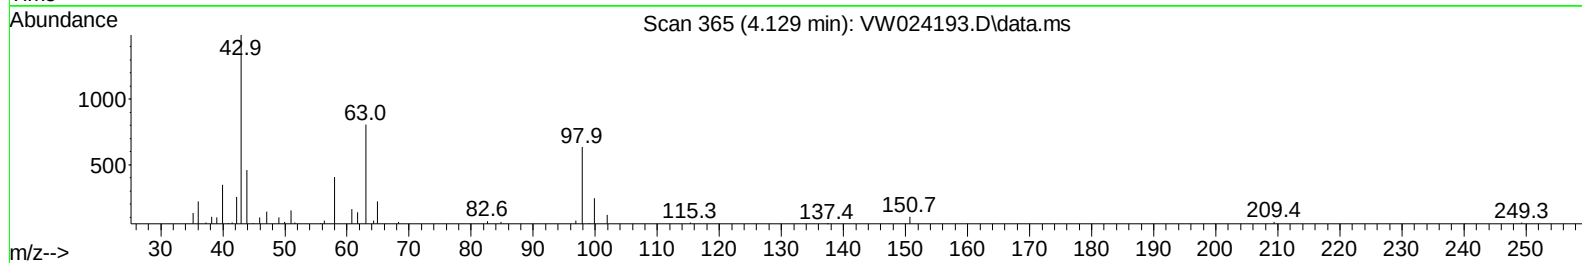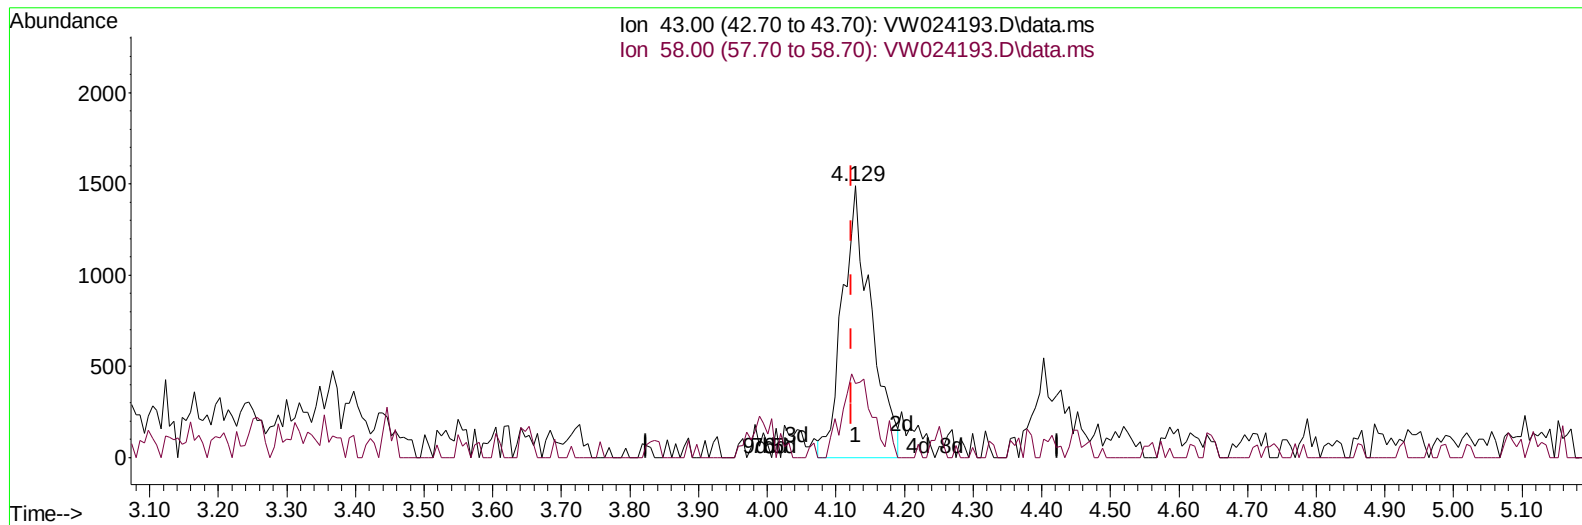

TIC: VW024193.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 4.79 ug/L m

response 4330

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	8.41
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
 Data File : VW024193.D
 Acq On : 05 Aug 2022 15:35
 Operator : SY/VA
 Sample : N4030-01
 Misc : 4.67g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:46:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 23:43:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	315596	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	289987	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	122746	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.342	65	197374	29.920	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	119.680%	
7) Chloroethane-d5	2.879	69	118569	28.853	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	115.400%	
11) 1,1-Dichloroethene-d2	4.007	63	137758	18.324	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	73.280%	
21) 2-Butanone-d5	7.079	46	64416	52.486	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	104.980%	
24) Chloroform-d	7.646	84	221481	23.194	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.760%	
26) 1,2-Dichloroethane-d4	8.305	65	133973	25.270	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	101.080%	
32) Benzene-d6	8.274	84	430981	25.200	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	100.800%	
36) 1,2-Dichloropropane-d6	9.274	67	129357	25.618	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	102.480%	
41) Toluene-d8	10.323	98	381877	23.889	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	95.560%	
43) trans-1,3-Dichloroprop...	10.579	79	56106	25.368	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	101.480%	
47) 2-Hexanone-d5	10.926	63	56114	60.164	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.320%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	123851	25.280	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	101.120%	
66) 1,2-Dichlorobenzene-d4	13.853	152	111771	24.884	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	99.520%	
Target Compounds						
					Qvalue	
13) Acetone	4.129	43	4330m	4.792	ug/L	
16) Methylene chloride	4.909	84	26397	4.743	ug/L	94
53) m,p-Xylene	11.835	106	5730	0.738	ug/L	97
54) o-Xylene	12.164	106	9683	1.320	ug/L	81
62) 1,3,5-Trimethylbenzene	12.938	105	83150	6.772	ug/L	99
63) 1,2,4-Trimethylbenzene	13.249	105	181971	15.047	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080522\
Data File : VW024193.D
Acq On : 05 Aug 2022 15:35
Operator : SY/VA
Sample : N4030-01
Misc : 4.67g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 23:46:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 23:43:03 2022
Response via : Initial Calibration

