

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080619\
 Data File : VW011714.D
 Acq On : 05 Aug 2019 17:23
 Operator : SY/VA
 Sample : K4135-14
 Misc : 4.94G/5ML/MSVOA W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 1S-B3-(0-1)

Quant Time: Aug 06 08:53:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 27 00:23:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	221833	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	370701	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	310593	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	122419	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	142743	56.04	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.08%	
35) Dibromofluoromethane	7.88	113	113938	54.79	ug/l	0.00
Spiked Amount	50.000		Recovery	=	109.58%	
50) Toluene-d8	10.32	98	457019	53.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.34%	
62) 4-Bromofluorobenzene	12.62	95	147965	48.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.48%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW080619\
Data File : VW011714.D
Acq On : 05 Aug 2019 17:23
Operator : SY/VA
Sample : K4135-14
Misc : 4.94G/5ML/MSVOA W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
1S-B3-(0-1)

Quant Time: Aug 06 08:53:30 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 27 00:23:30 2019
Response via : Initial Calibration

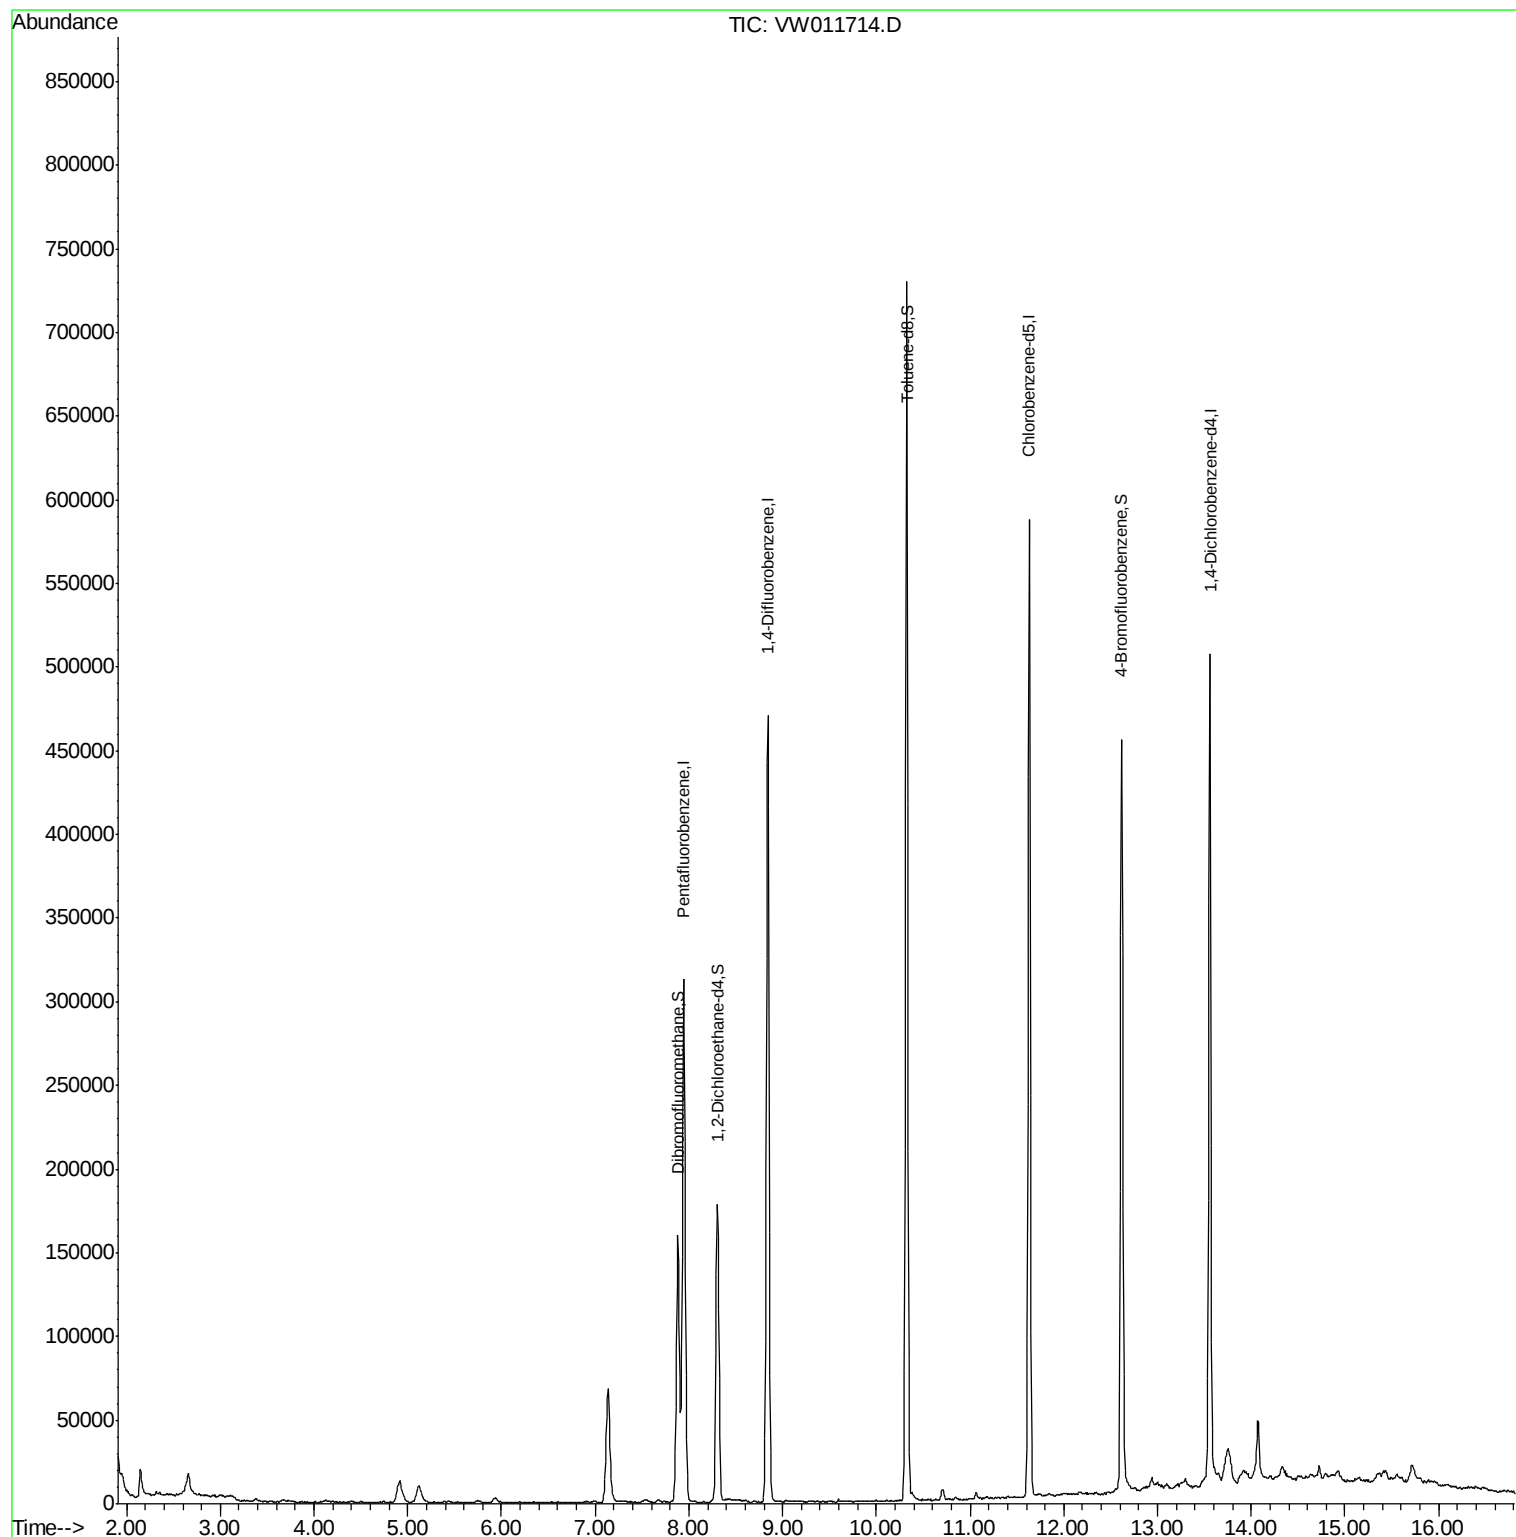



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW011714.D

Acq: 05 Aug 2019 17:23

Instrument :

MSVOA_W

ClientSampleId :


1S-B3-(0-1)

Tot Ion:168 Resp: 221833

Ion Ratio Lower Upper




168 100

99 61.0 48.2 72.4

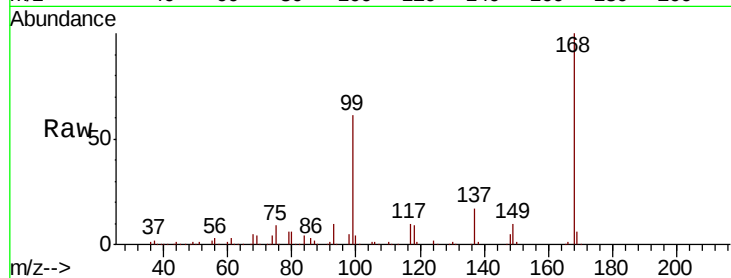

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

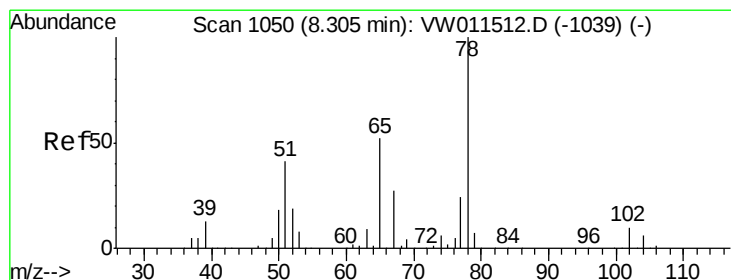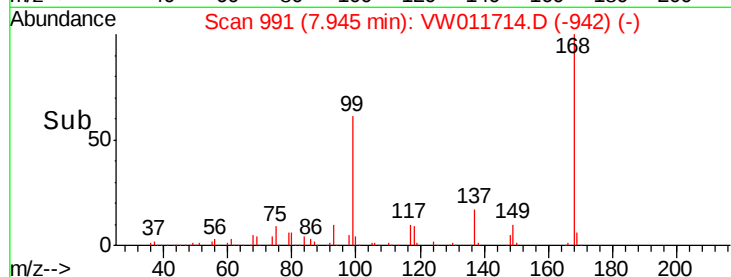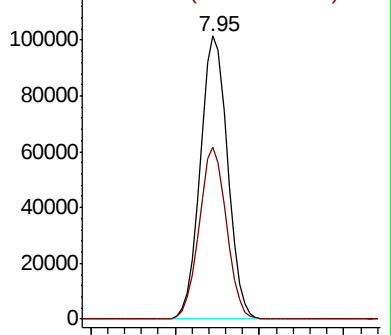

#33

1,2-Dichloroethane-d4

Concen: 56.038 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW011714.D


Acq: 05 Aug 2019 17:23

Tgt Ion: 65 Resp: 142743

Ion Ratio Lower Upper



65 100


67 51.3 0.0 105.2

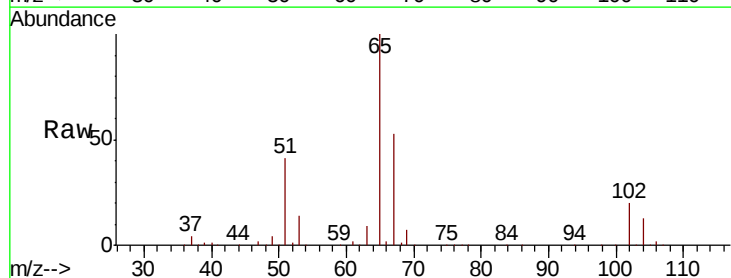

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW



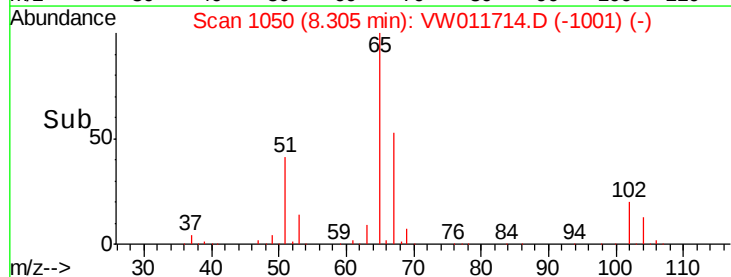
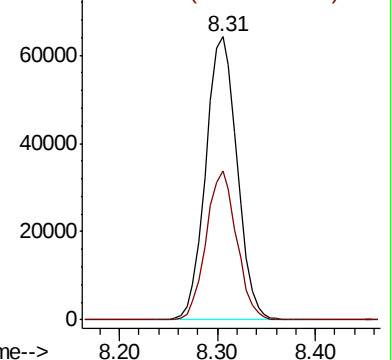


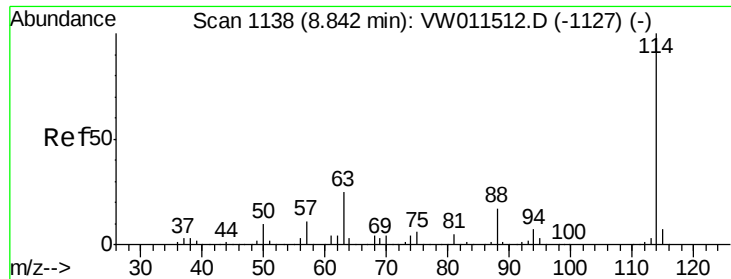

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VW011714.D
 Acq: 05 Aug 2019 17:23




Instrument :
 MSVOA_W
 ClientSampleId :
 1S-B3-(0-1)


Tot Ion	Ratio	Lower	Upper
114	100		
63	25.3	0.0	49.2
88	17.3	0.0	33.8

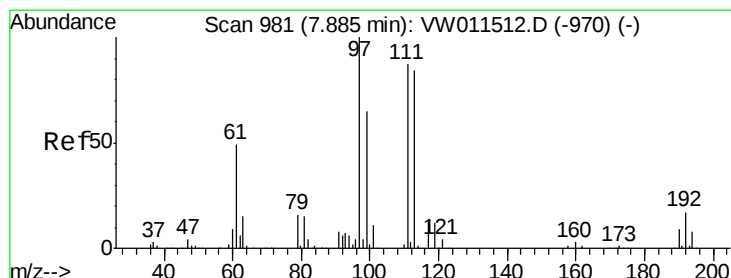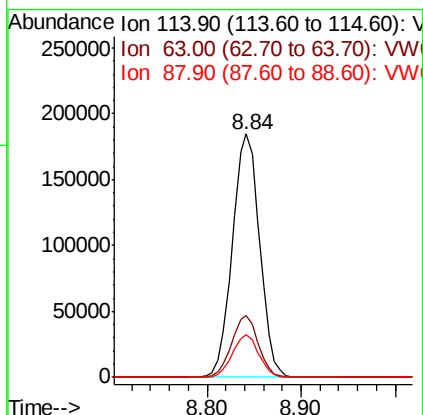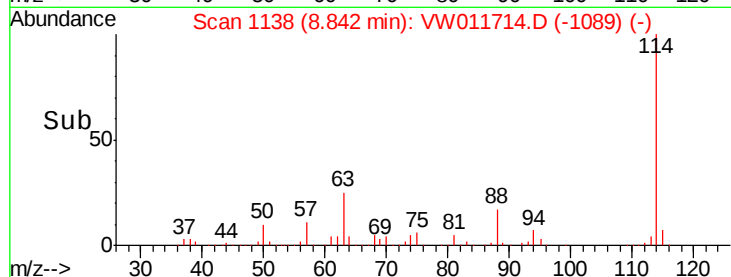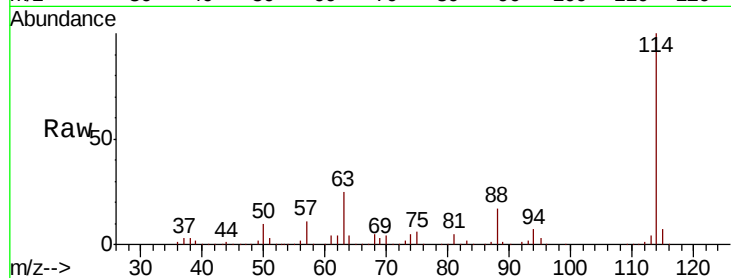

#35
 Dibromofluoromethane
 Concen: 54.786 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.00 min
 Lab File: VW011714.D
 Acq: 05 Aug 2019 17:23

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.6	82.7	124.1
192	20.2	16.1	24.1


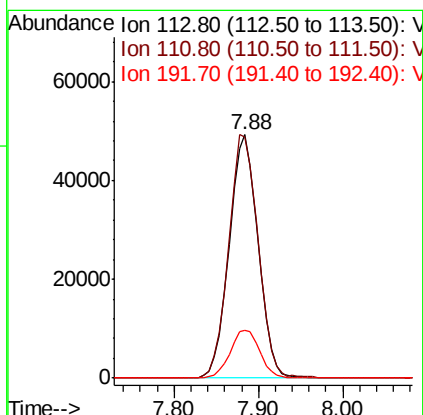
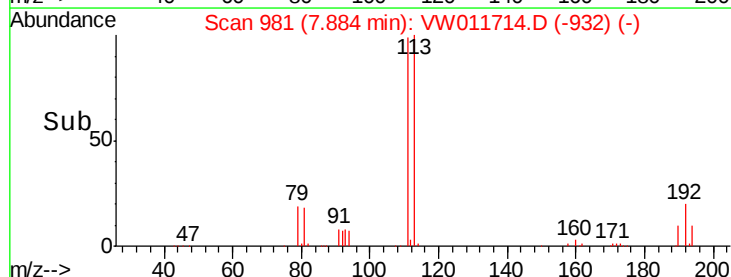
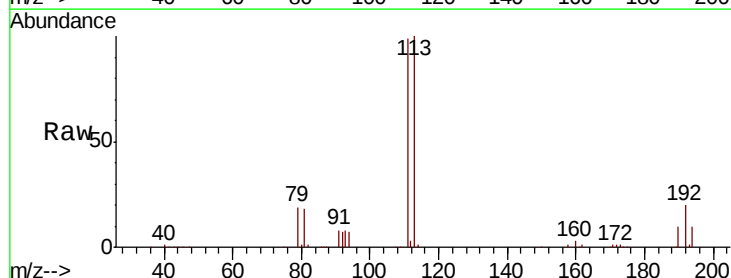


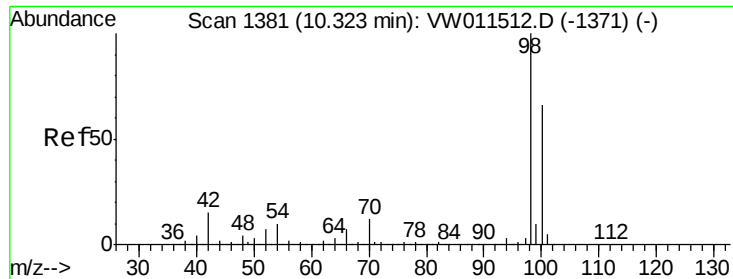

#50
Toluene-d8
Concen: 53.673 ug/l
RT: 10.32 min Scan# 1381
Delta R.T. -0.00 min
Lab File: VW011714.D
Acq: 05 Aug 2019 17:23




Instrument :
MSVOA_W
ClientSampleId :
1S-B3-(0-1)


Tot Ion: 98 Resp: 457019
Ion Ratio Lower Upper
98 100
100 65.3 52.7 79.1

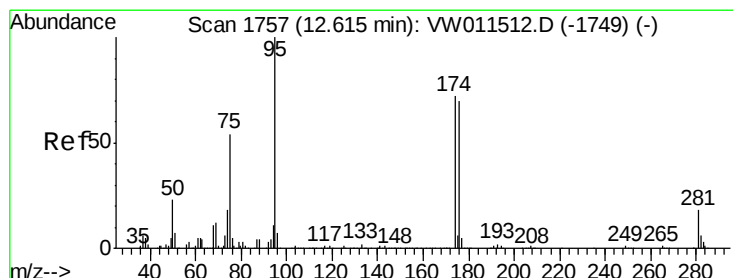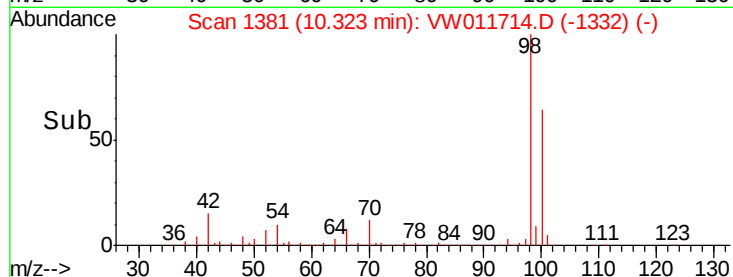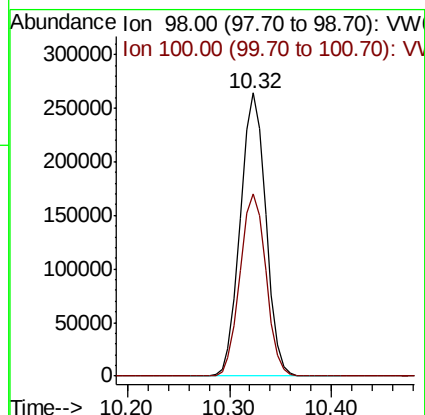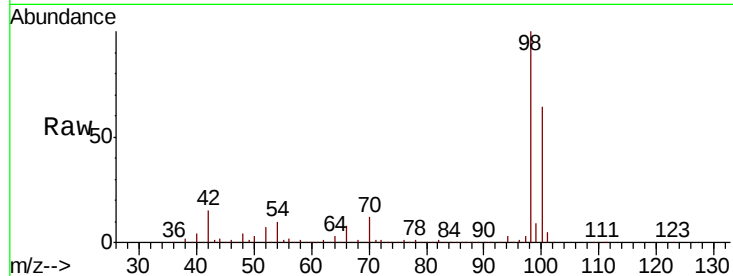

#62
4-Bromofluorobenzene
Concen: 48.741 ug/l
RT: 12.62 min Scan# 1757
Delta R.T. -0.00 min
Lab File: VW011714.D
Acq: 05 Aug 2019 17:23

Tgt Ion: 95 Resp: 147965
Ion Ratio Lower Upper
95 100
174 73.8 0.0 150.2
176 71.9 0.0 144.4

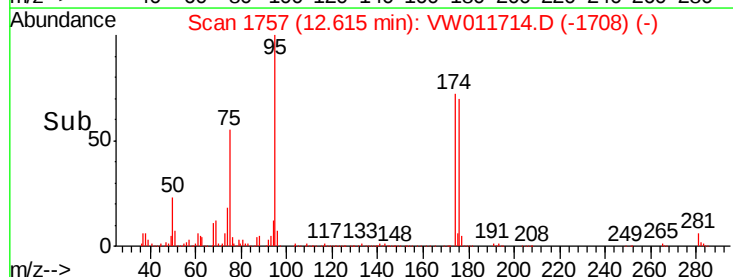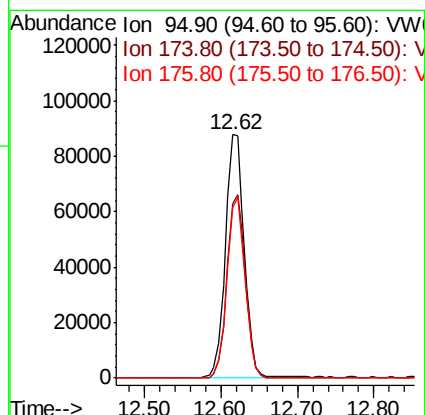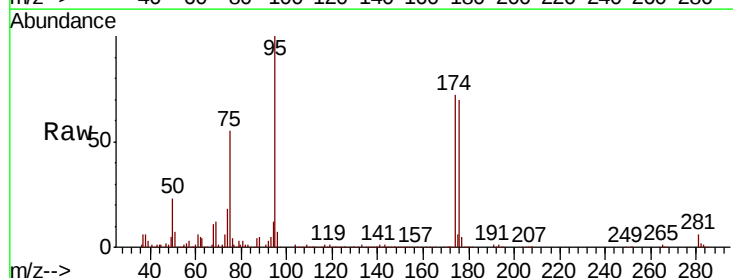


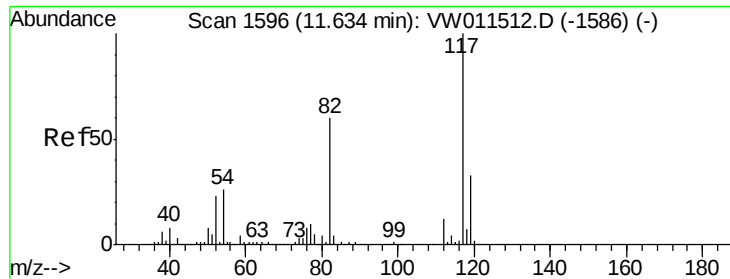

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW011714.D
Acq: 05 Aug 2019 17:23

Instrument :
MSVOA_W
ClientSampleId :
1S-B3-(0-1)

Tot Ion	Ratio	Lower	Upper
117	100		
82	60.5	47.9	71.9
119	31.8	26.2	39.2



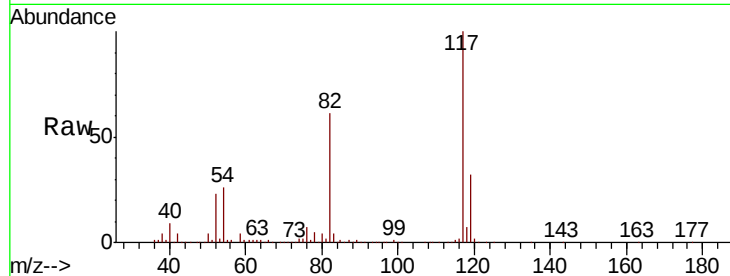


Abundance

Ion 116.90 (116.60 to 117.60): V


Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

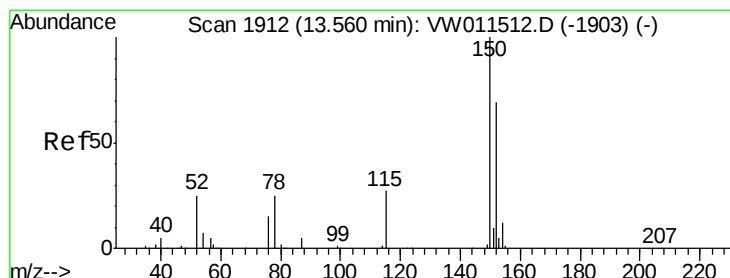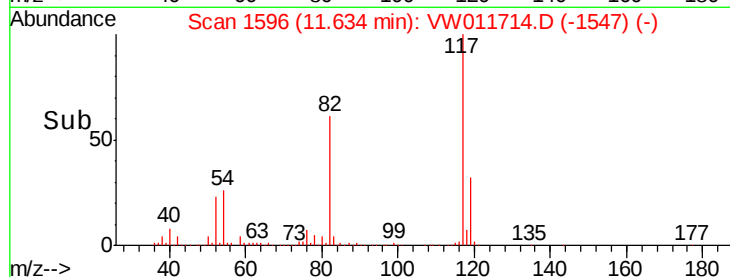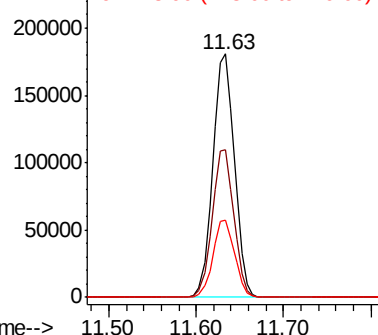

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW011714.D
Acq: 05 Aug 2019 17:23

Tgt Ion	Ratio	Lower	Upper
152	100		
115	60.0	30.5	91.5
150	157.5	0.0	352.6

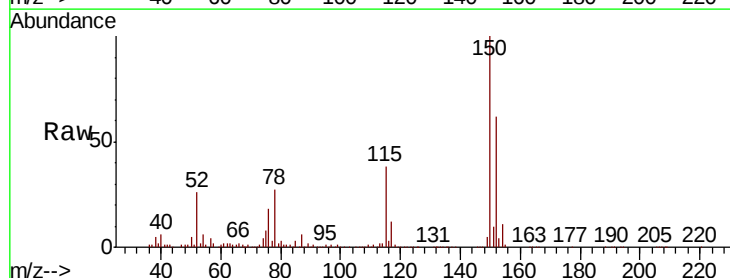

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

