


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080619\
Data File : VW011707.D
Acq On : 05 Aug 2019 13:53
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
Title : SW846 8260
Last Update : Sat Jul 27 00:23:30 2019

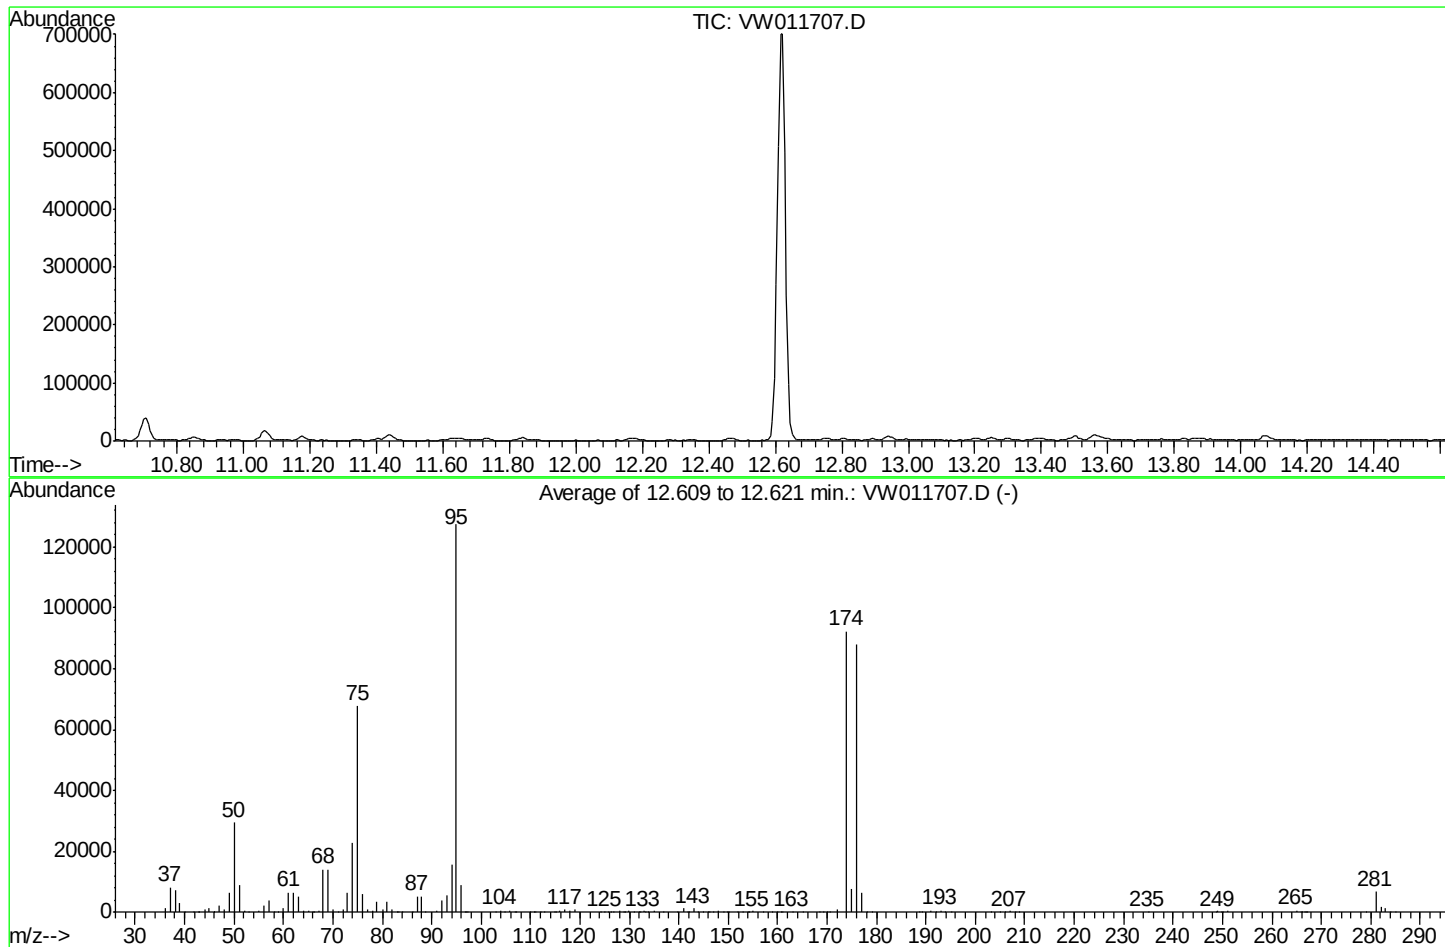

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	29344	PASS
75	95	30	60	53.3	67944	PASS
95	95	100	100	100.0	127504	PASS
96	95	5	9	6.9	8789	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.4	92304	PASS
175	174	5	9	8.2	7603	PASS
176	174	95	101	95.1	87826	PASS
177	176	5	9	7.1	6230	PASS