


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW080619\
 Data File : VW011708.D
 Acq On : 05 Aug 2019 14:27
 Operator : SY/VA
 Sample : VSTDCCC050
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 LabSampleId :
 VSTDCCC050

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
 Title : SW846 8260
 Last Update : Sat Jul 27 00:23:30 2019

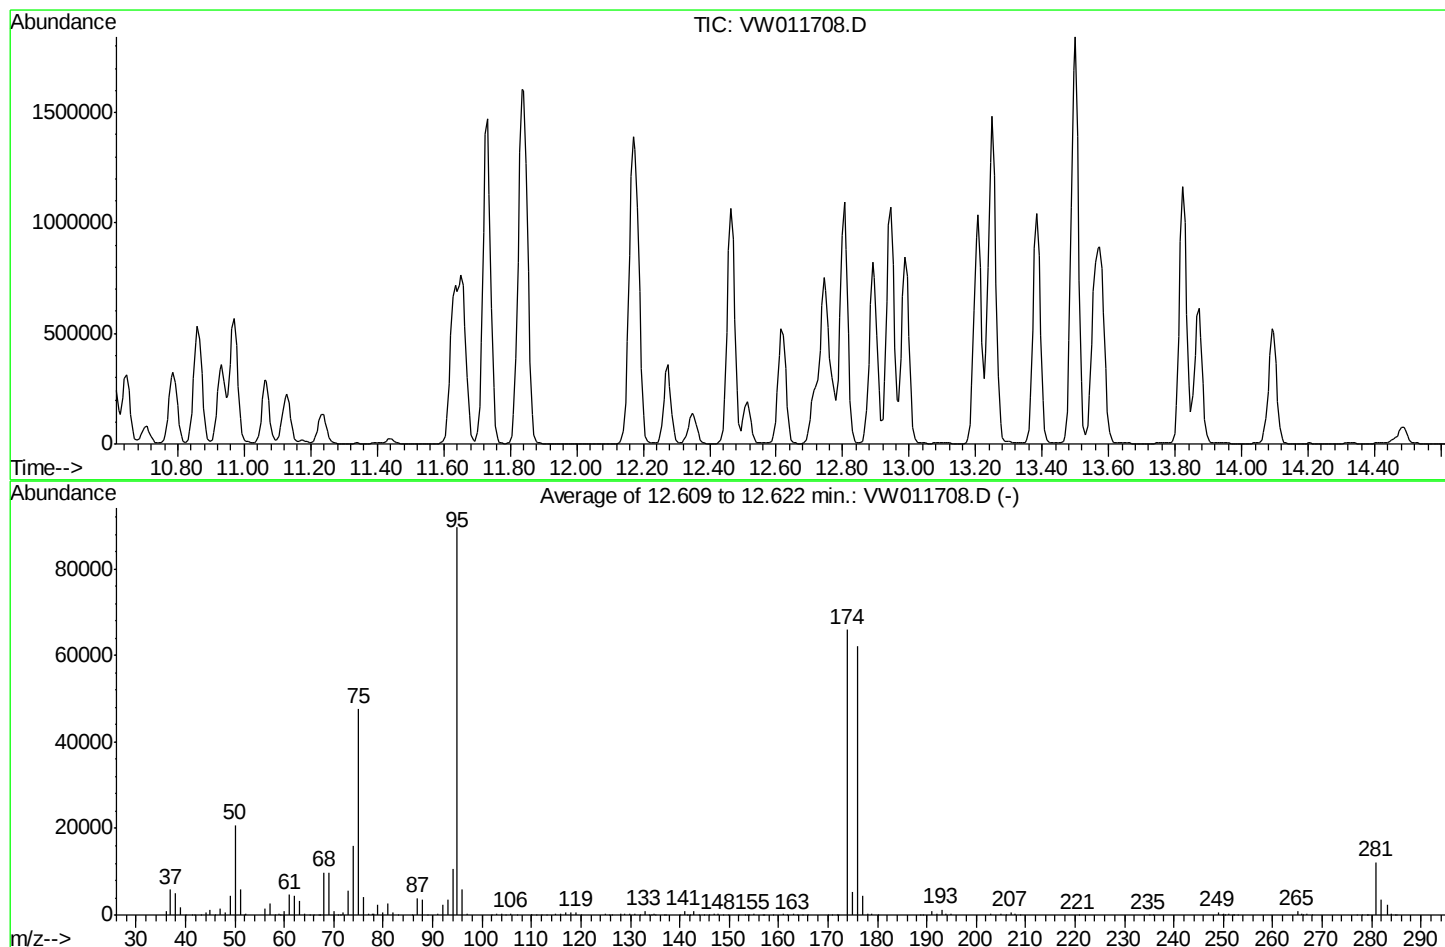

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	20780	PASS
75	95	30	60	53.3	47787	PASS
95	95	100	100	100.0	89685	PASS
96	95	5	9	6.6	5907	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.6	65997	PASS
175	174	5	9	8.1	5373	PASS
176	174	95	101	94.1	62093	FAIL *
177	176	5	9	7.4	4586	PASS