

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080620\
 Data File : VW016055.D
 Acq On : 06 Aug 2020 19:52
 Operator : SY/VA
 Sample : L3564-07
 Misc : 6.30G/10ML/MSVOA W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFSQ1

Quant Time: Aug 07 08:15:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 07 07:41:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	382269	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	347107	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	149176	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	67729	12.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.24%
7) Chloroethane-d5	2.89	69	58075	13.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.04%
10) 1,1-Dichloroethene-d2	4.01	63	112934	10.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	41.44%#
20) 2-Butanone-d5	7.09	46	38330	27.05	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.10%
24) Chloroform-d	7.65	84	183218	17.07	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	68.28%
26) 1,2-Dichloroethane-d4	8.31	65	92327	15.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	62.68%#
29) Benzene-d6	8.27	84	357678	16.93	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	67.72%
33) 1,2-Dichloropropane-d6	9.27	67	108130	17.07	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	68.28%#
37) Toluene-d8	10.32	98	315632	16.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	65.96%
38) trans-1,3-Dichloropropene-	10.58	79	39587	14.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	58.64%
39) 2-Hexanone-d5	10.93	63	31564	29.93	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.86%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	82727	16.99	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	67.96%
61) 1,2-Dichlorobenzene-d4	13.85	152	111548	19.18	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	76.72%


Target Compounds					Ovalue
47) Tetrachloroethene	10.86	164	2134	0.493 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW080620\
Data File : VW016055.D
Acq On : 06 Aug 2020 19:52
Operator : SY/VA
Sample : L3564-07
Misc : 6.30G/10ML/MSVOA W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFSQ1

Quant Time: Aug 07 08:15:17 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 07 07:41:20 2020
Response via : Initial Calibration

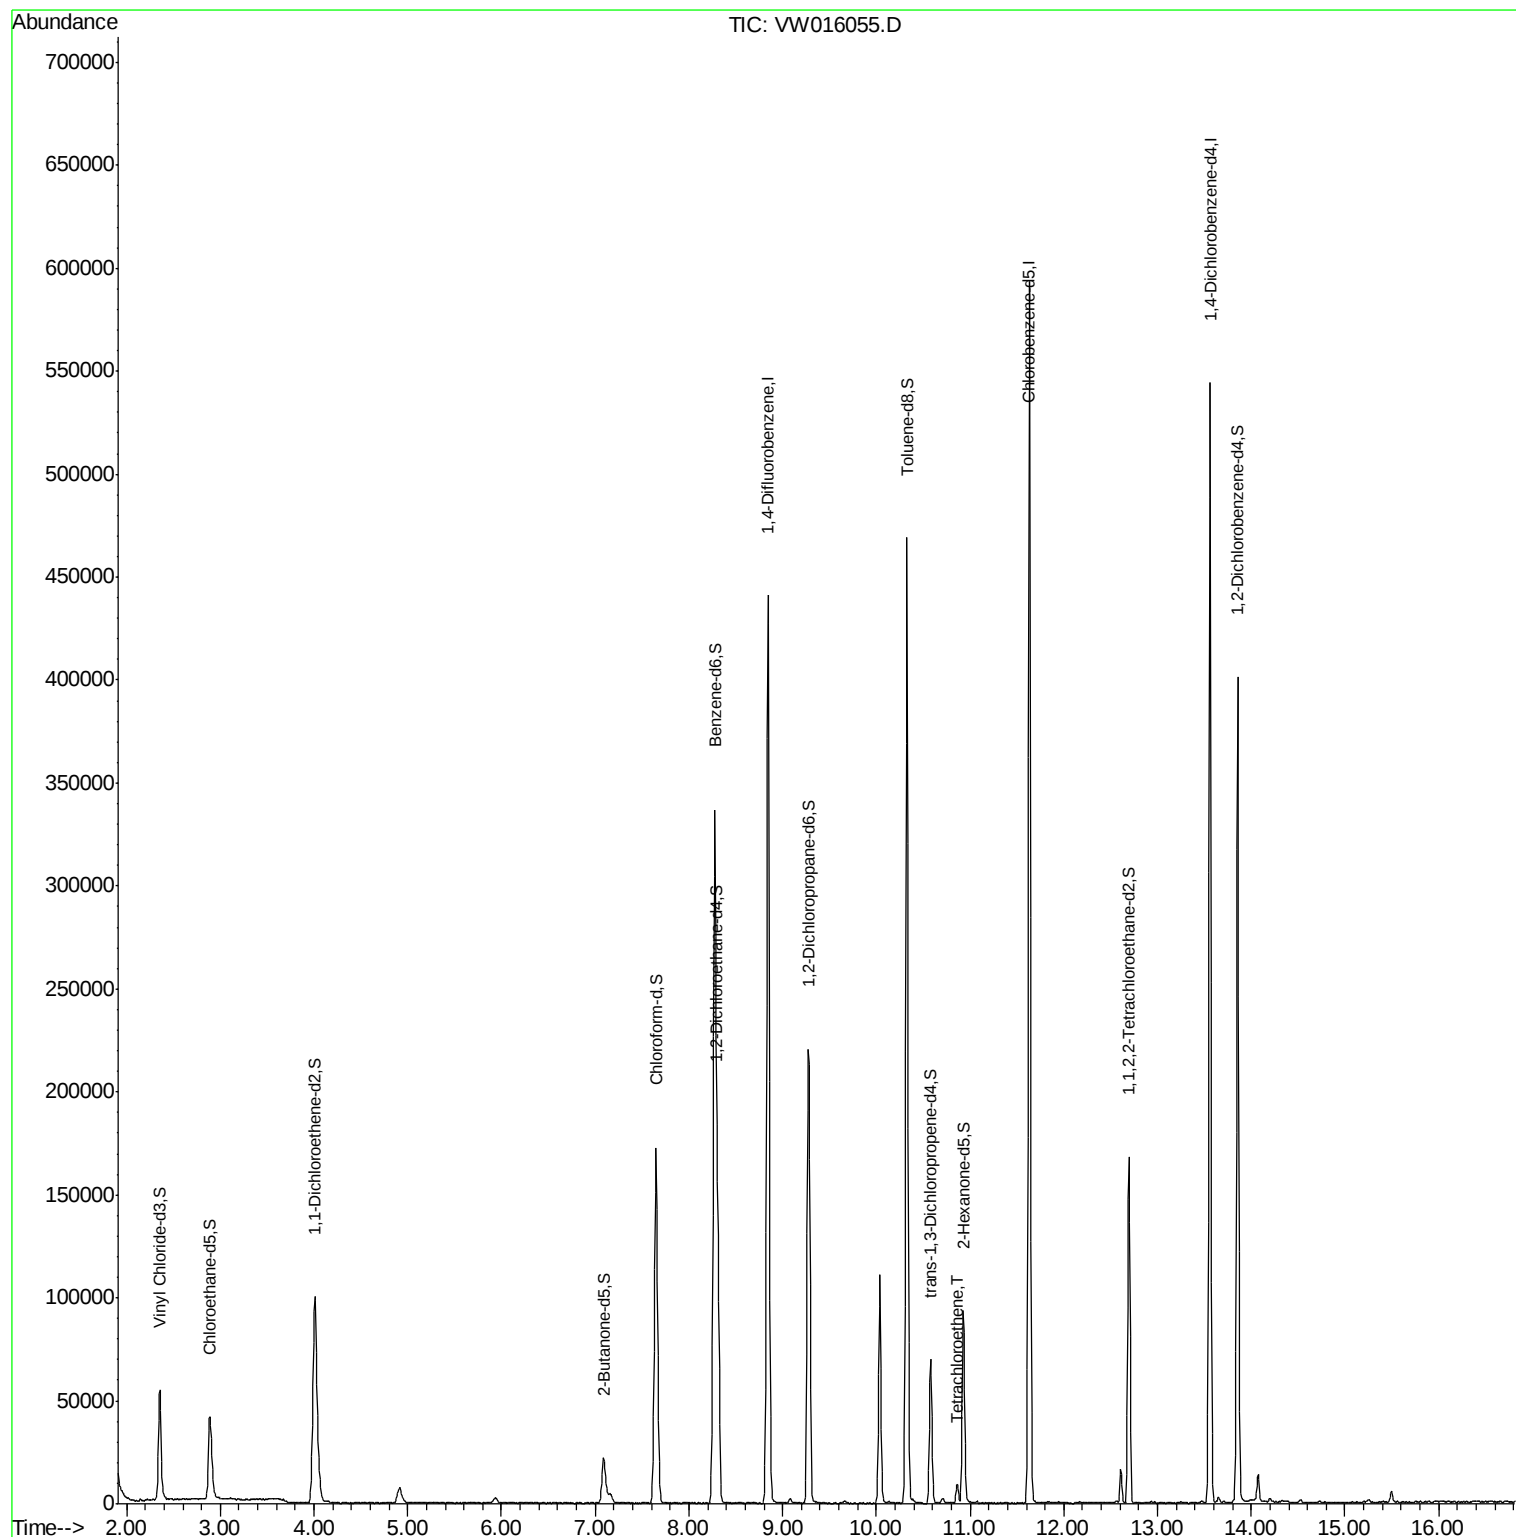

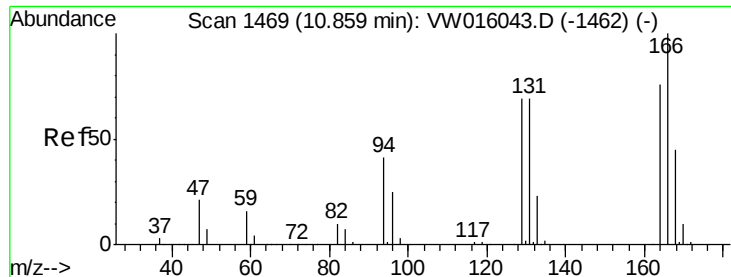

#47

Tetrachloroethene

Concen: 0.493 ug/L

RT: 10.86 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VW016055.D


Acq: 06 Aug 2020 19:52

Instrument :

MSVOA_W

ClientSampleId :

BFSQ1

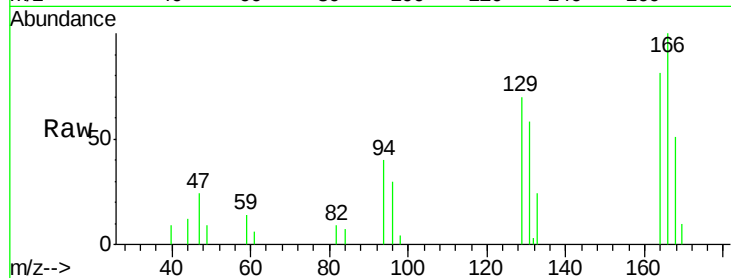

Tot Ion:164 Resp: 2134

Ion Ratio Lower Upper

164 100

129 86.9 70.0 130.0

131 72.1 67.3 124.9


166 124.1 88.5 164.3

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

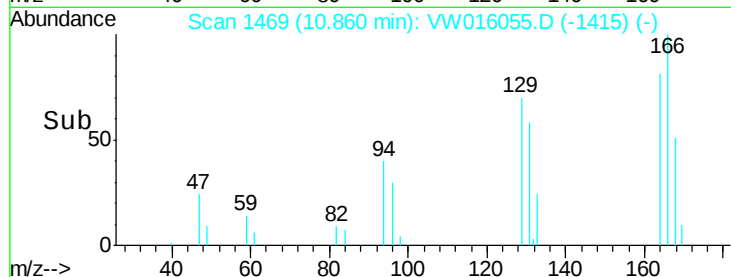

Time-->

