

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080621\
 Data File : VW019700.D
 Acq On : 06 Aug 2021 13:57
 Operator : SY/VA
 Sample : M3287-10RE
 Misc : 3.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGB11RE

Quant Time: Aug 07 01:04:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 07 01:03:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	437178	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	345026	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	107210	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	115504	18.647	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.600%
7) Chloroethane-d5	2.897	69	93401	21.145	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.560%
11) 1,1-Dichloroethene-d2	4.025	63	184714	15.455	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.800%
21) 2-Butanone-d5	7.086	46	55057	30.624	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	61.240%
24) Chloroform-d	7.653	84	253684	21.001	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.000%
26) 1,2-Dichloroethane-d4	8.311	65	149448	22.545	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.160%
32) Benzene-d6	8.281	84	505221	24.599	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.400%
36) 1,2-Dichloropropane-d6	9.274	67	152505	23.824	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.280%
41) Toluene-d8	10.323	98	422497	22.817	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.280%
43) trans-1,3-Dichloroprop...	10.579	79	53490	19.512	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.040%
47) 2-Hexanone-d5	10.927	63	43585	36.700	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.400%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	108132	20.905	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.640%
66) 1,2-Dichlorobenzene-d4	13.853	152	81515	21.550	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.200%
Target Compounds						Qvalue
16) Methylene chloride	4.928	84	87393	10.027	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080621\
Data File : VW019700.D
Acq On : 06 Aug 2021 13:57
Operator : SY/VA
Sample : M3287-10RE
Misc : 3.99g/10mL/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGB11RE

Quant Time: Aug 07 01:04:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 07 01:03:00 2021
Response via : Initial Calibration

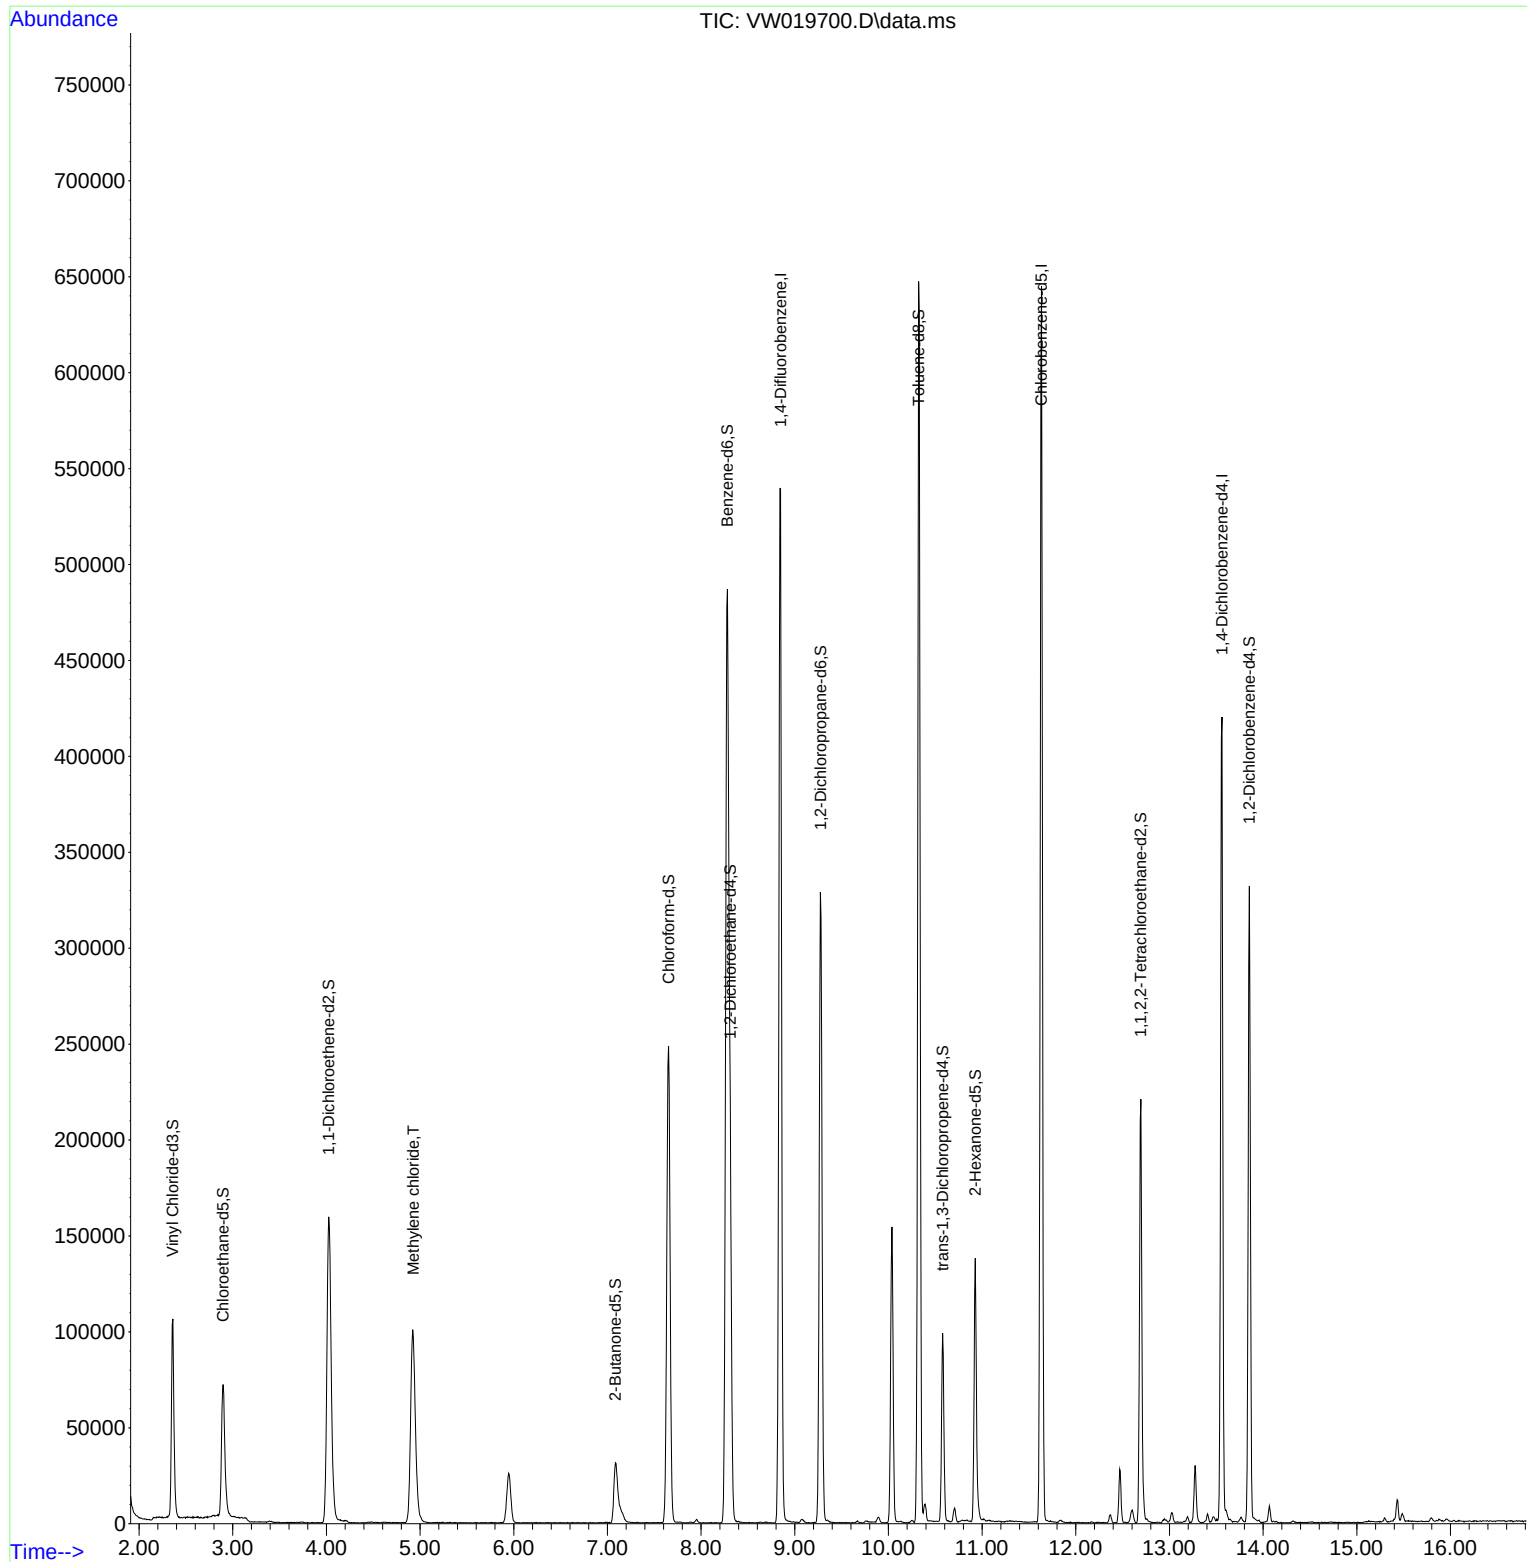

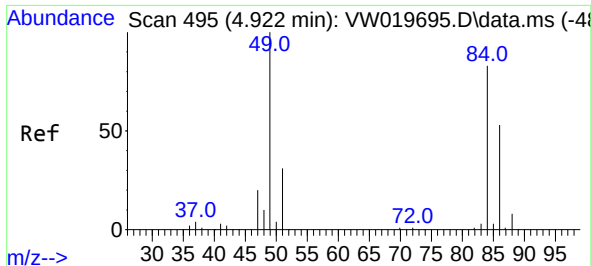

#16
Methylene chloride
Concen: 10.027 ug/L
RT: 4.928 min Scan# 496
Delta R.T. 0.006 min
Lab File: VW019700.D
Acq: 06 Aug 2021 13:57

Instrument :
MSVOA_W
ClientSampleId :
BGB11RE

Tgt Ion:	84	Resp:	87393
Ion	Ratio	Lower	Upper
84	100		
86	64.8	45.3	84.1
49	123.0	86.6	160.8

