

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080624\
 Data File : VW029837.D
 Acq On : 06 Aug 2024 13:00
 Operator : SY/MD
 Sample : VW0806SBL02
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 07 02:27:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 07 02:26:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	249093	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	246043	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	108027	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	49771	14.074	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.280%
7) Chloroethane-d5	2.893	69	44111	17.472	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.880%
11) 1,1-Dichloroethene-d2	4.021	65	26946	16.693	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.760%
21) 2-Butanone-d5	7.081	46	40944	42.243	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.480%
24) Chloroform-d	7.648	84	142109	22.039	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.160%
26) 1,2-Dichloroethane-d4	8.307	65	85905	23.390	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.560%
32) Benzene-d6	8.270	84	257287	19.353	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.400%
36) 1,2-Dichloropropane-d6	9.276	67	91776	21.620	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.480%
41) Toluene-d8	10.325	98	226218	19.138	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.560%
43) trans-1,3-Dichloroprop...	10.575	79	33083	19.260	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.040%
47) 2-Hexanone-d5	10.922	63	27124	38.751	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.500%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	71009	22.529	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.120%
66) 1,2-Dichlorobenzene-d4	13.849	152	76596	22.835	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.360%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	2608	0.388	ug/L	# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080624\
Data File : VW029837.D
Acq On : 06 Aug 2024 13:00
Operator : SY/MD
Sample : VW0806SBL02
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Aug 07 02:27:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 07 02:26:16 2024
Response via : Initial Calibration

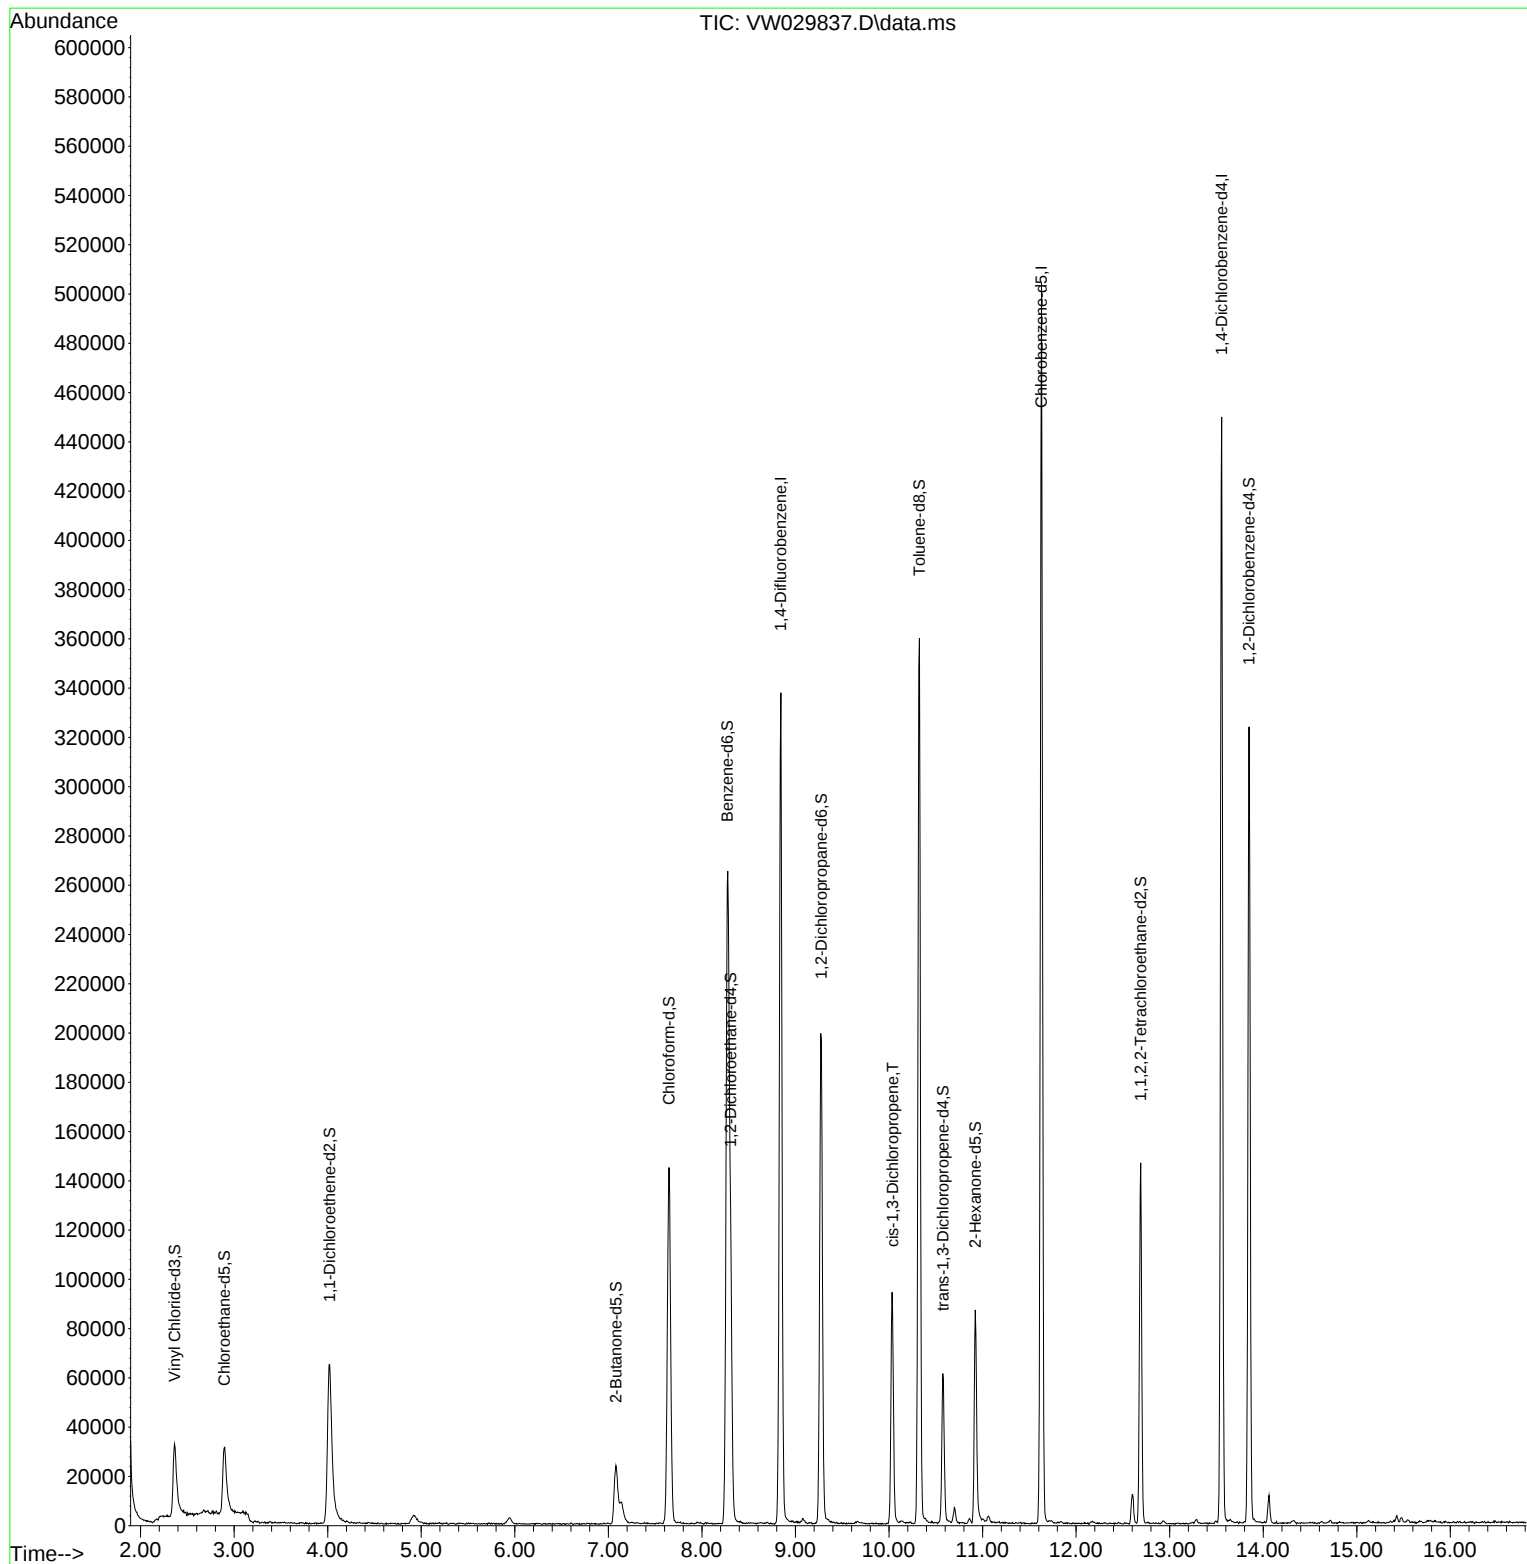

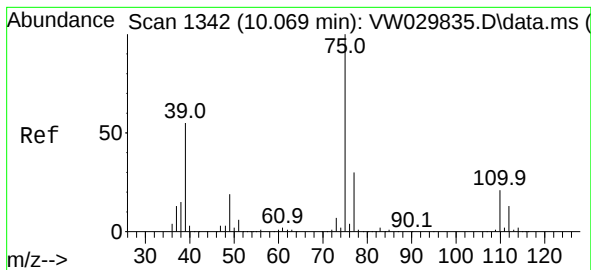

#39
 cis-1,3-Dichloropropene
 Concen: 0.388 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.031 min
 Lab File: VW029837.D
 Acq: 06 Aug 2024 13:00

Instrument :
 MSVOA_W
 ClientSampleId :

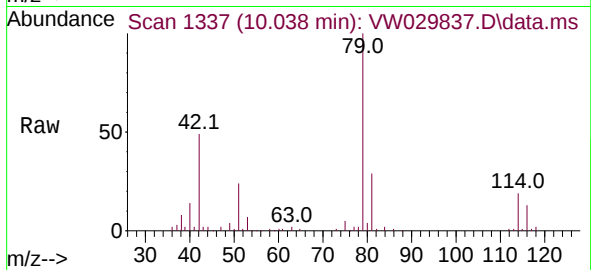

Tgt Ion: 75 Resp: 2608
 Ion Ratio Lower Upper
 75 100
 77 41.5 20.8 38.6#

