

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW080718\
 Data File : VW004488.D
 Acq On : 07 Aug 2018 10:46
 Operator : SY/AP
 Sample : J4268-09
 Misc : 4.89G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AA1

Quant Time: Aug 08 05:49:18 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 08 05:39:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	899183	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	791016	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	262482	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	217805	19.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.88%
7) Chloroethane-d5	2.89	69	192064	20.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.64%
10) 1,1-Dichloroethene-d2	4.01	63	340126	14.98	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.92%
20) 2-Butanone-d5	7.09	46	120207	24.38	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	48.76%
24) Chloroform-d	7.65	84	525707	21.60	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.40%
26) 1,2-Dichloroethane-d4	8.31	65	283827	20.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.64%
29) Benzene-d6	8.28	84	994836	23.64	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.56%
33) 1,2-Dichloropropane-d6	9.27	67	337108	24.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.04%
37) Toluene-d8	10.33	98	811666	21.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.52%
38) trans-1,3-Dichloropropene-	10.58	79	112103	19.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.28%
39) 2-Hexanone-d5	10.93	63	94001	28.08	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	56.16%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	248246	16.64	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	66.56%
61) 1,2-Dichlorobenzene-d4	13.86	152	211114	21.41	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.64%


Target Compounds					Qvalue
13) Acetone	4.15	43	9060	2.121 ug/L	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW080718\
Data File : VW004488.D
Acq On : 07 Aug 2018 10:46
Operator : SY/AP
Sample : J4268-09
Misc : 4.89G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AA1

Quant Time: Aug 08 05:49:18 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 08 05:39:03 2018
Response via : Initial Calibration

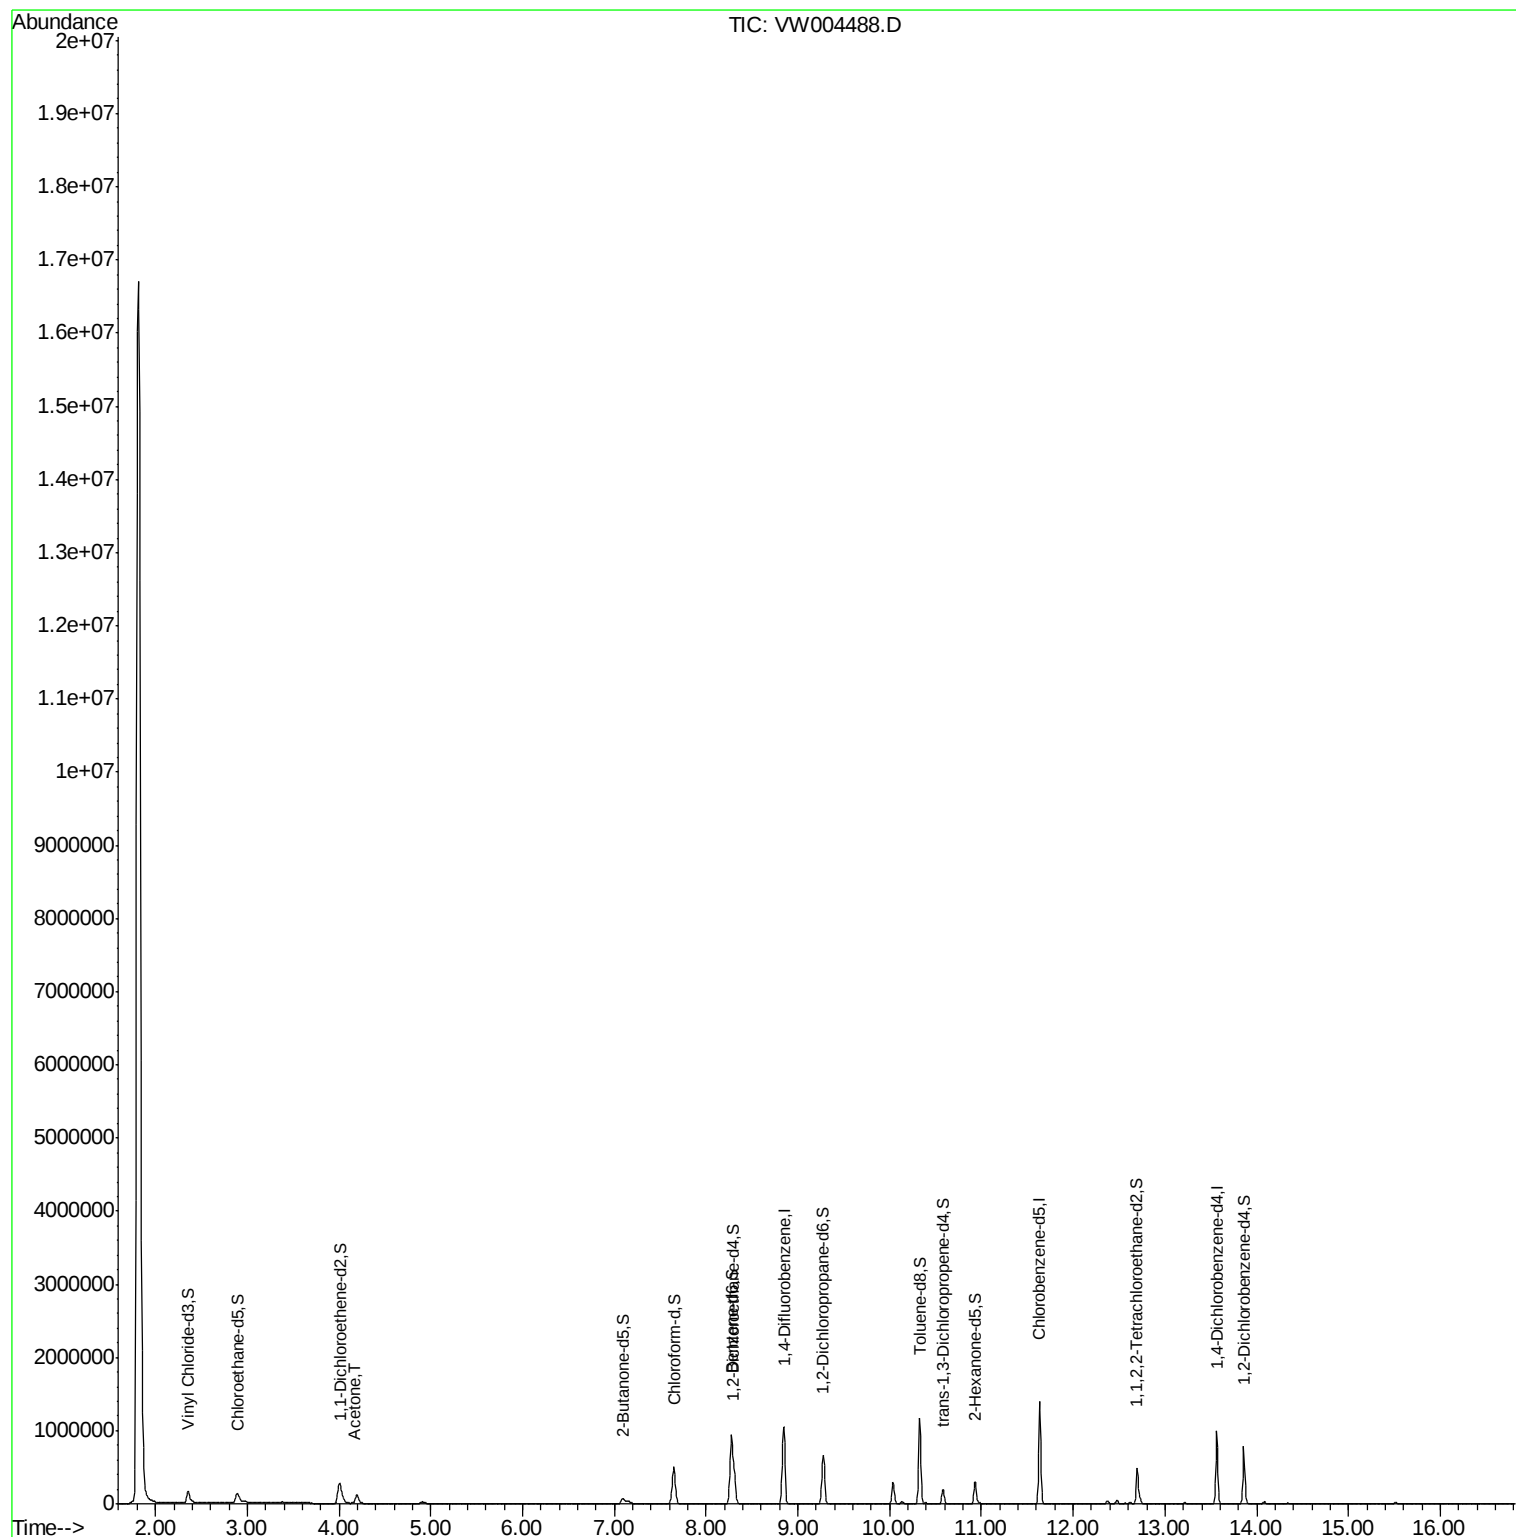

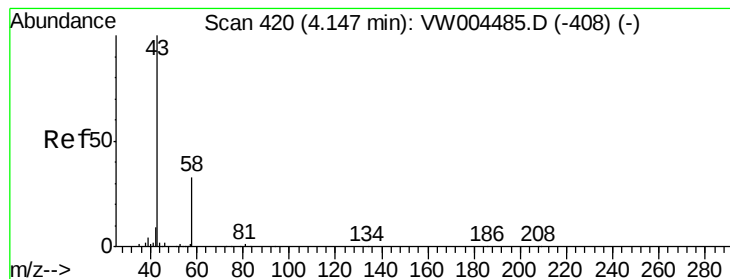

#13

Acetone

Concen: 2.121 ug/L

RT: 4.15 min Scan# 421

Delta R.T. 0.01 min

Lab File: VW004488.D

Acq: 07 Aug 2018 10:46

Instrument :

MSVOA_W

ClientSampleId :

C0AA1

Tgt Ion: 43 Resp: 9060

Ion Ratio Lower Upper

43 100

58 11.0 0.0 66.4

