

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080718\
 Data File : VW004490.D
 Acq On : 07 Aug 2018 12:21
 Operator : SY/AP
 Sample : J4301-17RE
 Misc : 5.33G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF8RE

Quant Time: Aug 08 07:52:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 08 05:39:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	827465	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	726359	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	236312	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	208667	20.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.08%
7) Chloroethane-d5	2.89	69	185218	21.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.56%
10) 1,1-Dichloroethene-d2	4.01	63	321554	15.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.52%
20) 2-Butanone-d5	7.09	46	161983	35.69	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.38%
24) Chloroform-d	7.65	84	516650	23.06	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.24%
26) 1,2-Dichloroethane-d4	8.31	65	304182	24.36	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.44%
29) Benzene-d6	8.28	84	954198	24.69	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.76%
33) 1,2-Dichloropropane-d6	9.28	67	325359	25.76	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.04%
37) Toluene-d8	10.33	98	744935	21.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.48%
38) trans-1,3-Dichloropropene-	10.58	79	106450	20.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.00%
39) 2-Hexanone-d5	10.93	63	108774	35.38	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.76%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	314589	22.97	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.88%
61) 1,2-Dichlorobenzene-d4	13.86	152	211198	23.80	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.20%


Target Compounds					Ovalue
16) Methylene chloride	4.91	84	186317	11.34 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080718\
Data File : VW004490.D
Acq On : 07 Aug 2018 12:21
Operator : SY/AP
Sample : J4301-17RE
Misc : 5.33G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AF8RE

Quant Time: Aug 08 07:52:46 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 08 05:39:03 2018
Response via : Initial Calibration

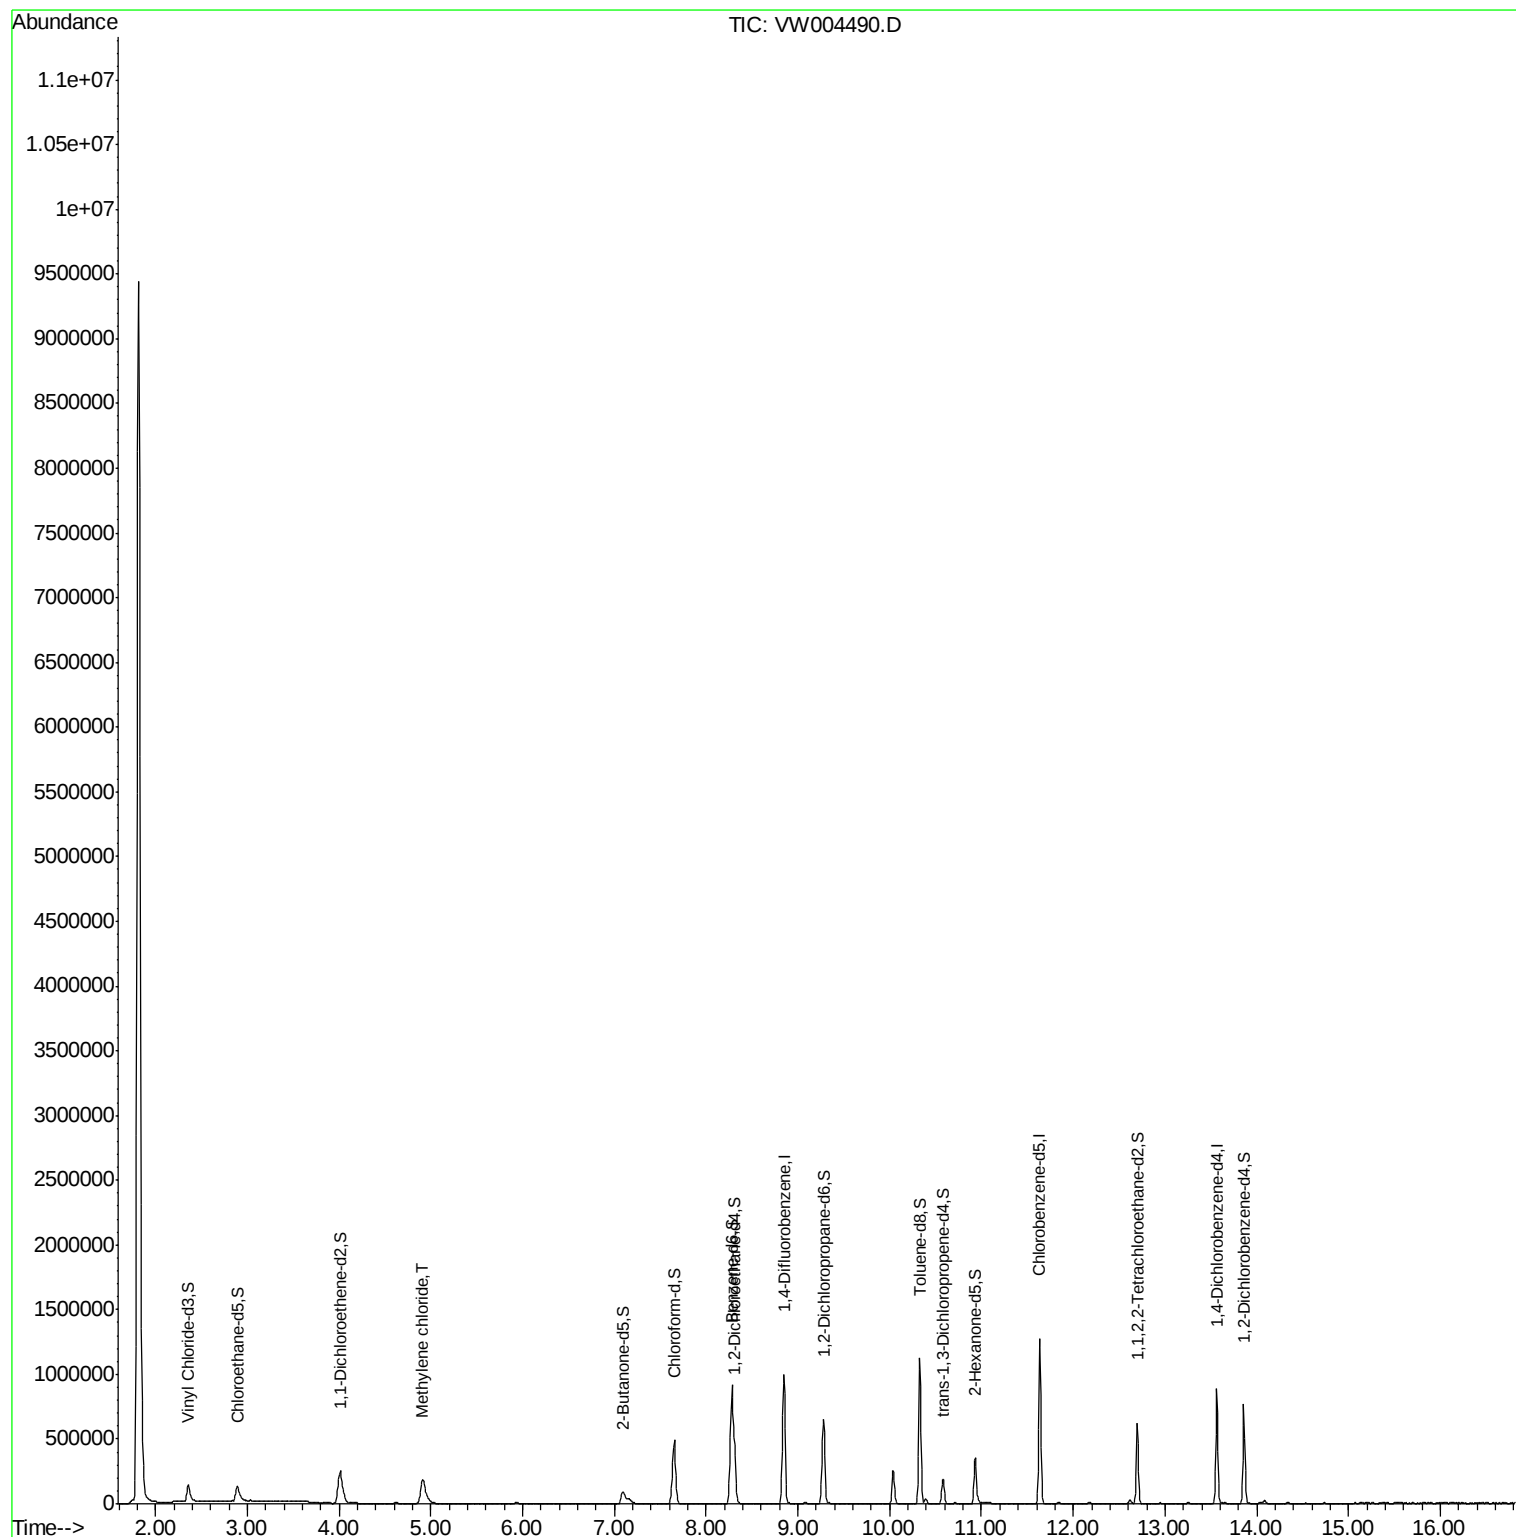

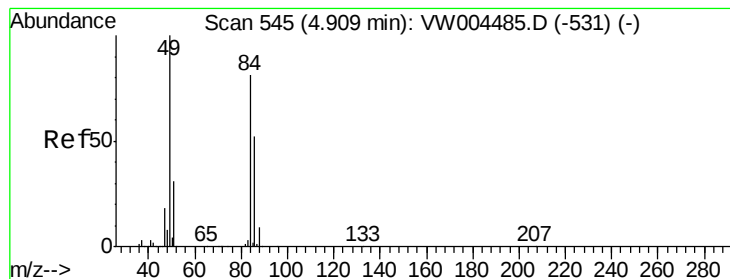

#16
 Methvlene chloride
 Concen: 11.34 ug/L
 RT: 4.91 min Scan# 545
 Delta R.T. -0.00 min
 Lab File: VW004490.D
 Acq: 07 Aug 2018 12:21

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF8RE

Tot Ion: 84 Resp: 186317
 Ion Ratio Lower Upper
 84 100
 49 122.7 86.0 159.6
 86 63.0 43.5 80.9

