

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080719\
 Data File : VW011736.D
 Acq On : 06 Aug 2019 11:14
 Operator : SY/VA
 Sample : K4116-21
 Misc : 5.06G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 06 16:39:18 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 06 16:36:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	345596	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	308796	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	144962	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	114227	23.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.88%
7) Chloroethane-d5	2.89	69	87091	24.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.40%
10) 1,1-Dichloroethene-d2	4.20	63	117	0.01	ug/L	0.18
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.04%#
20) 2-Butanone-d5	7.08	46	109622	50.03	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.06%
24) Chloroform-d	7.65	84	235968	24.86	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.44%
26) 1,2-Dichloroethane-d4	8.31	65	147654	26.29	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.16%
29) Benzene-d6	8.27	84	485538	25.00	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.00%
33) 1,2-Dichloropropane-d6	9.27	67	160611	25.62	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.48%
37) Toluene-d8	10.32	98	429450	24.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.68%
38) trans-1,3-Dichloropropene-	10.58	79	67157	24.44	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.76%
39) 2-Hexanone-d5	10.93	63	70860	48.40	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.80%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	129654	24.91	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.64%
61) 1,2-Dichlorobenzene-d4	13.85	152	144209	25.81	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.24%

Target Compounds


					Ovalue
13) Acetone	4.12	43	3197	1.362 ug/L	92
36) Methylcyclohexane	9.27	83	36613	3.674 ug/L #	15
59) 1,2,3-Trichloropropane	13.56	75	19584	4.852 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW080719\
Data File : VW011736.D
Acq On : 06 Aug 2019 11:14
Operator : SY/VA
Sample : K4116-21
Misc : 5.06G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 06 16:39:18 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 06 16:36:34 2019
Response via : Initial Calibration

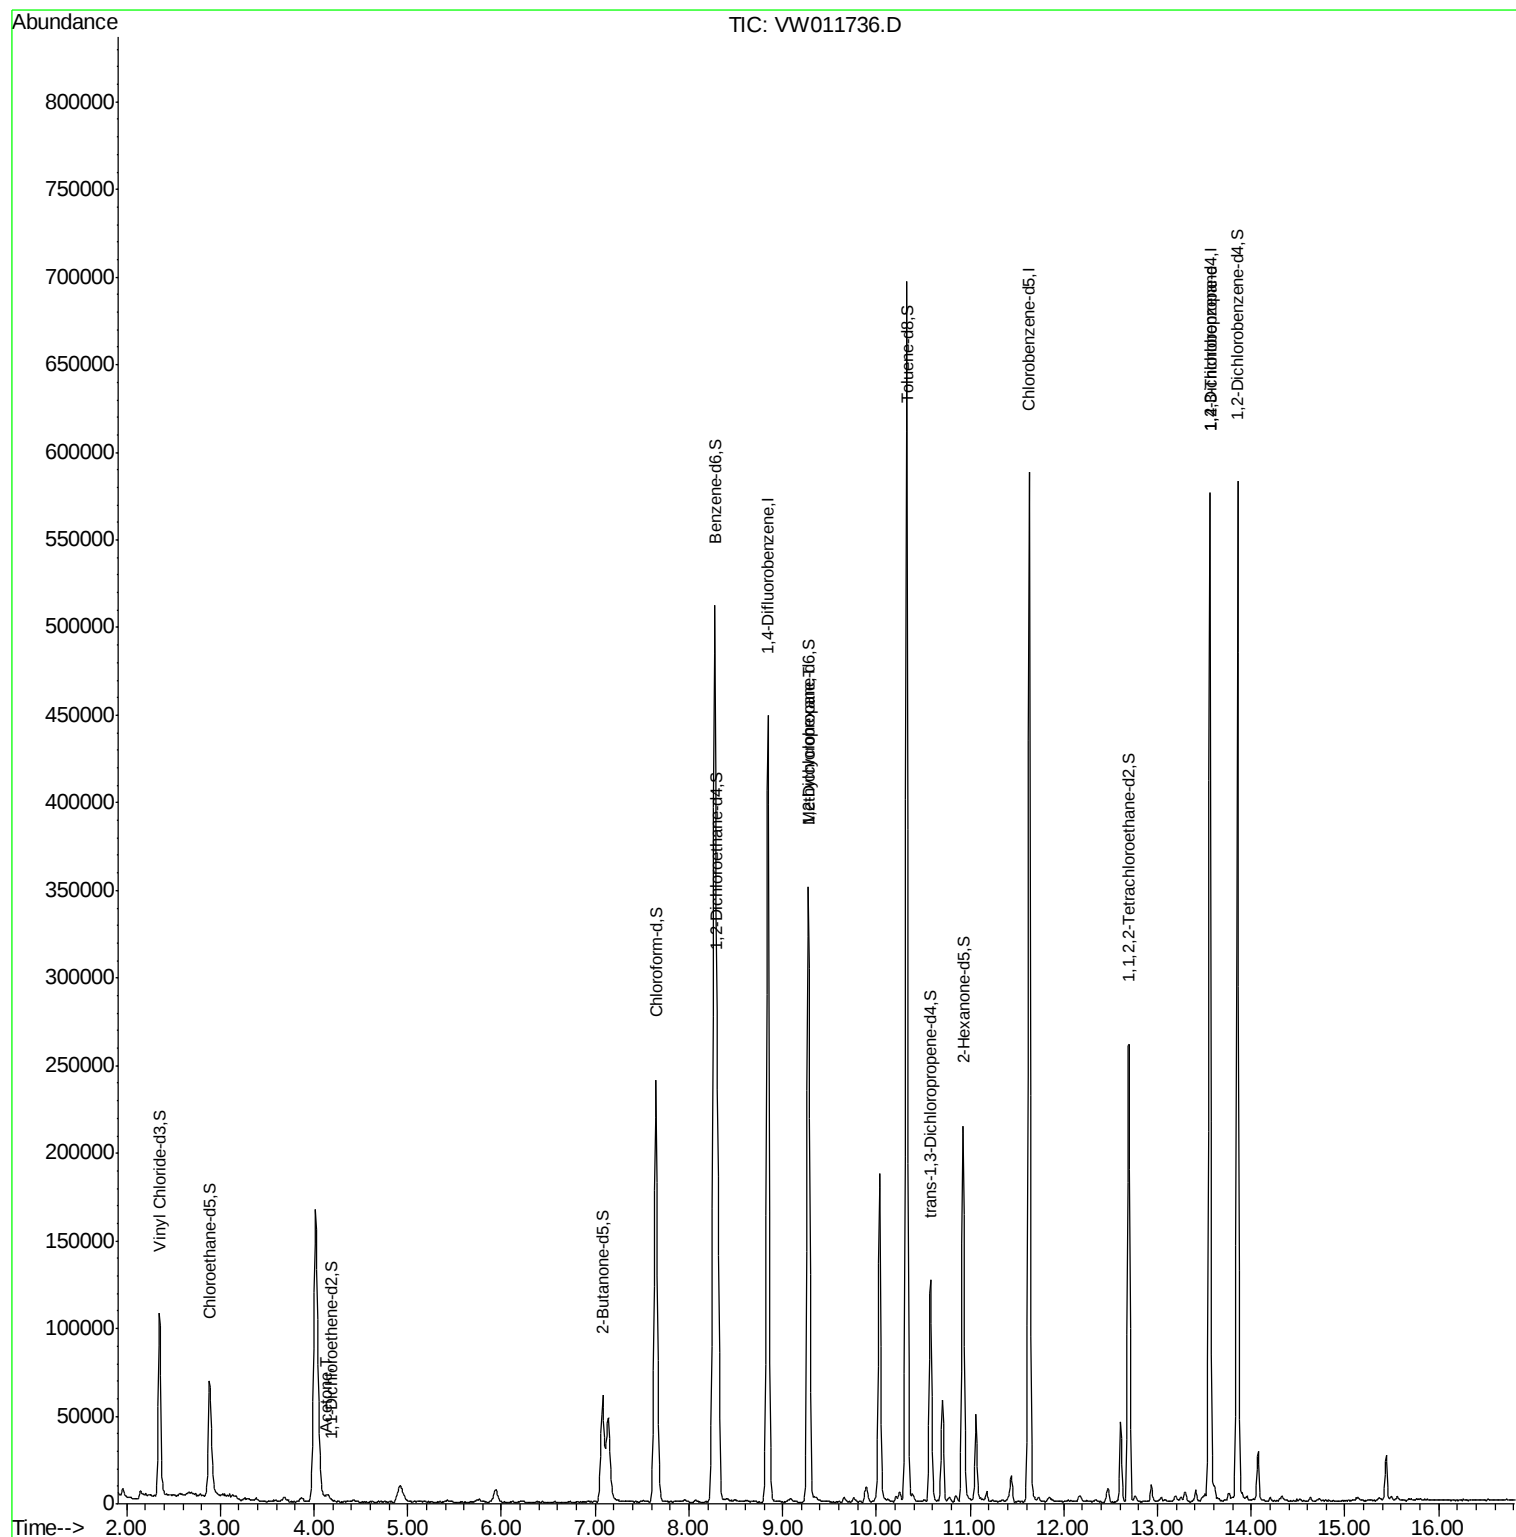

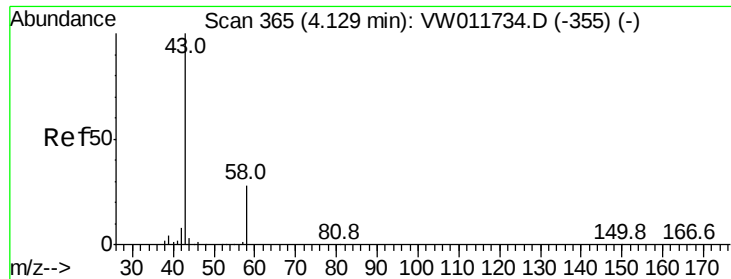

#13

Acetone

Concen: 1.362 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.00 min

Lab File: VW011736.D

Acq: 06 Aug 2019 11:14

Instrument :

MSVOA_W





ClientSampleId :

Tot Ion: 43 Resp: 3197

Ion Ratio Lower Upper

43 100

58 22.4 0.0 53.4

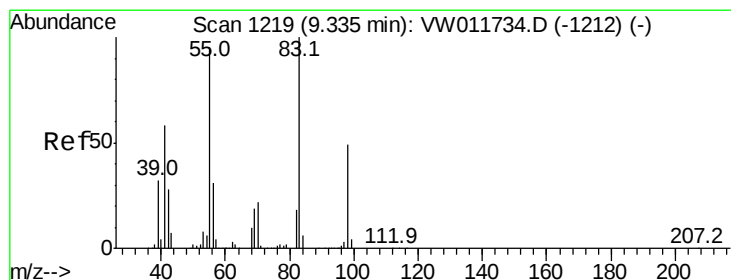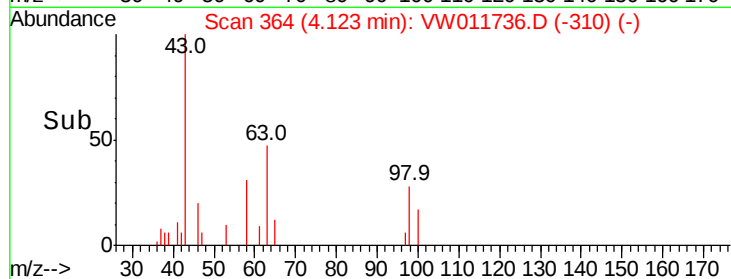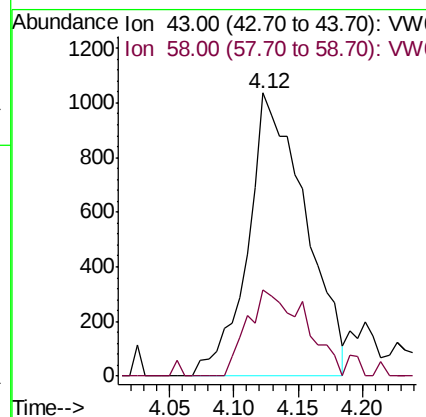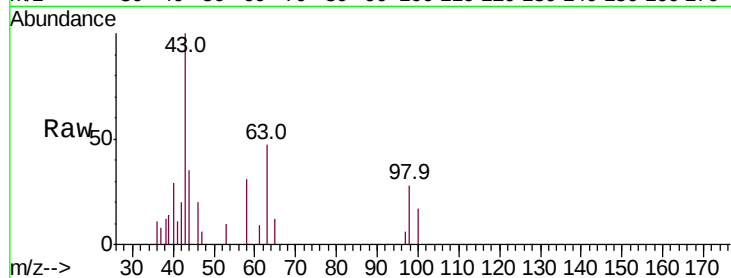

#36

Methylcyclohexane

Concen: 3.674 ug/L

RT: 9.27 min Scan# 1209

Delta R.T. -0.06 min

Lab File: VW011736.D

Acq: 06 Aug 2019 11:14




Tgt Ion: 83 Resp: 36613


Ion Ratio Lower Upper

83 100

55 1.1 72.6 108.8#

98 1.8 37.8 56.6#

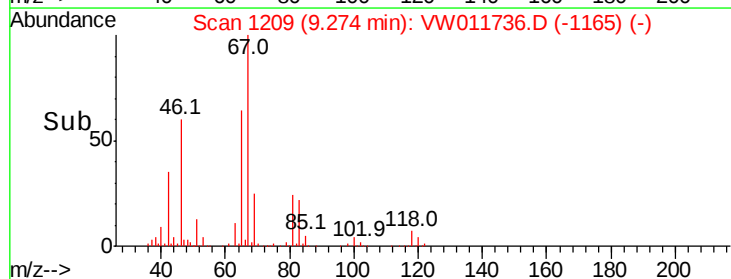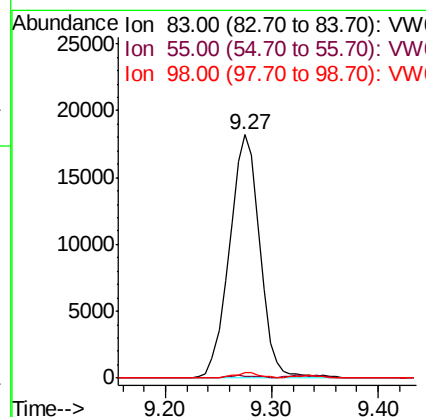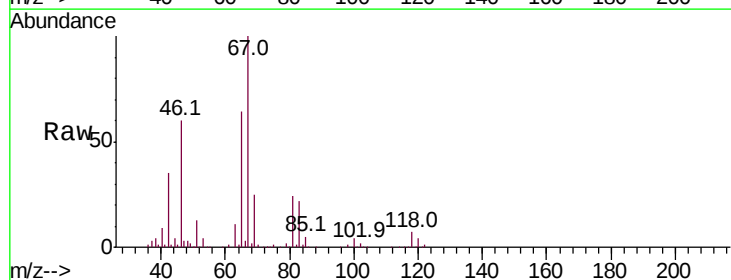

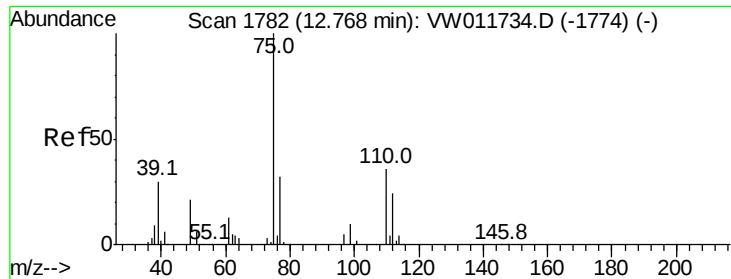

#59

1,2,3-Trichloropropane

Concen: 4.852 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW011736.D

Acq: 06 Aug 2019 11:14

Instrument :

MSVOA_W

ClientSampleId :

Tot Ion: 75 Resp: 19584

Ion Ratio Lower Upper

75 100

77 36.2 25.1 37.7

