

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080819\
 Data File : VW011750.D
 Acq On : 07 Aug 2019 14:48
 Operator : SY/VA
 Sample : K4034-02
 Misc : 5.55G/5ML/MSVOA W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 FK-PS-01-054

Quant Time: Aug 08 08:55:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 27 00:23:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	207782	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	342387	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	274996	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	97271	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	139847	58.61	ug/l	0.00
Spiked Amount	50.000		Recovery	=	117.22%	
35) Dibromofluoromethane	7.88	113	108638	56.56	ug/l	0.00
Spiked Amount	50.000		Recovery	=	113.12%	
50) Toluene-d8	10.32	98	415225	52.80	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.60%	
62) 4-Bromofluorobenzene	12.62	95	120676	43.04	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.08%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW080819\
Data File : VW011750.D
Acq On : 07 Aug 2019 14:48
Operator : SY/VA
Sample : K4034-02
Misc : 5.55G/5ML/MSVOA W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
FK-PS-01-054

Quant Time: Aug 08 08:55:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 27 00:23:30 2019
Response via : Initial Calibration

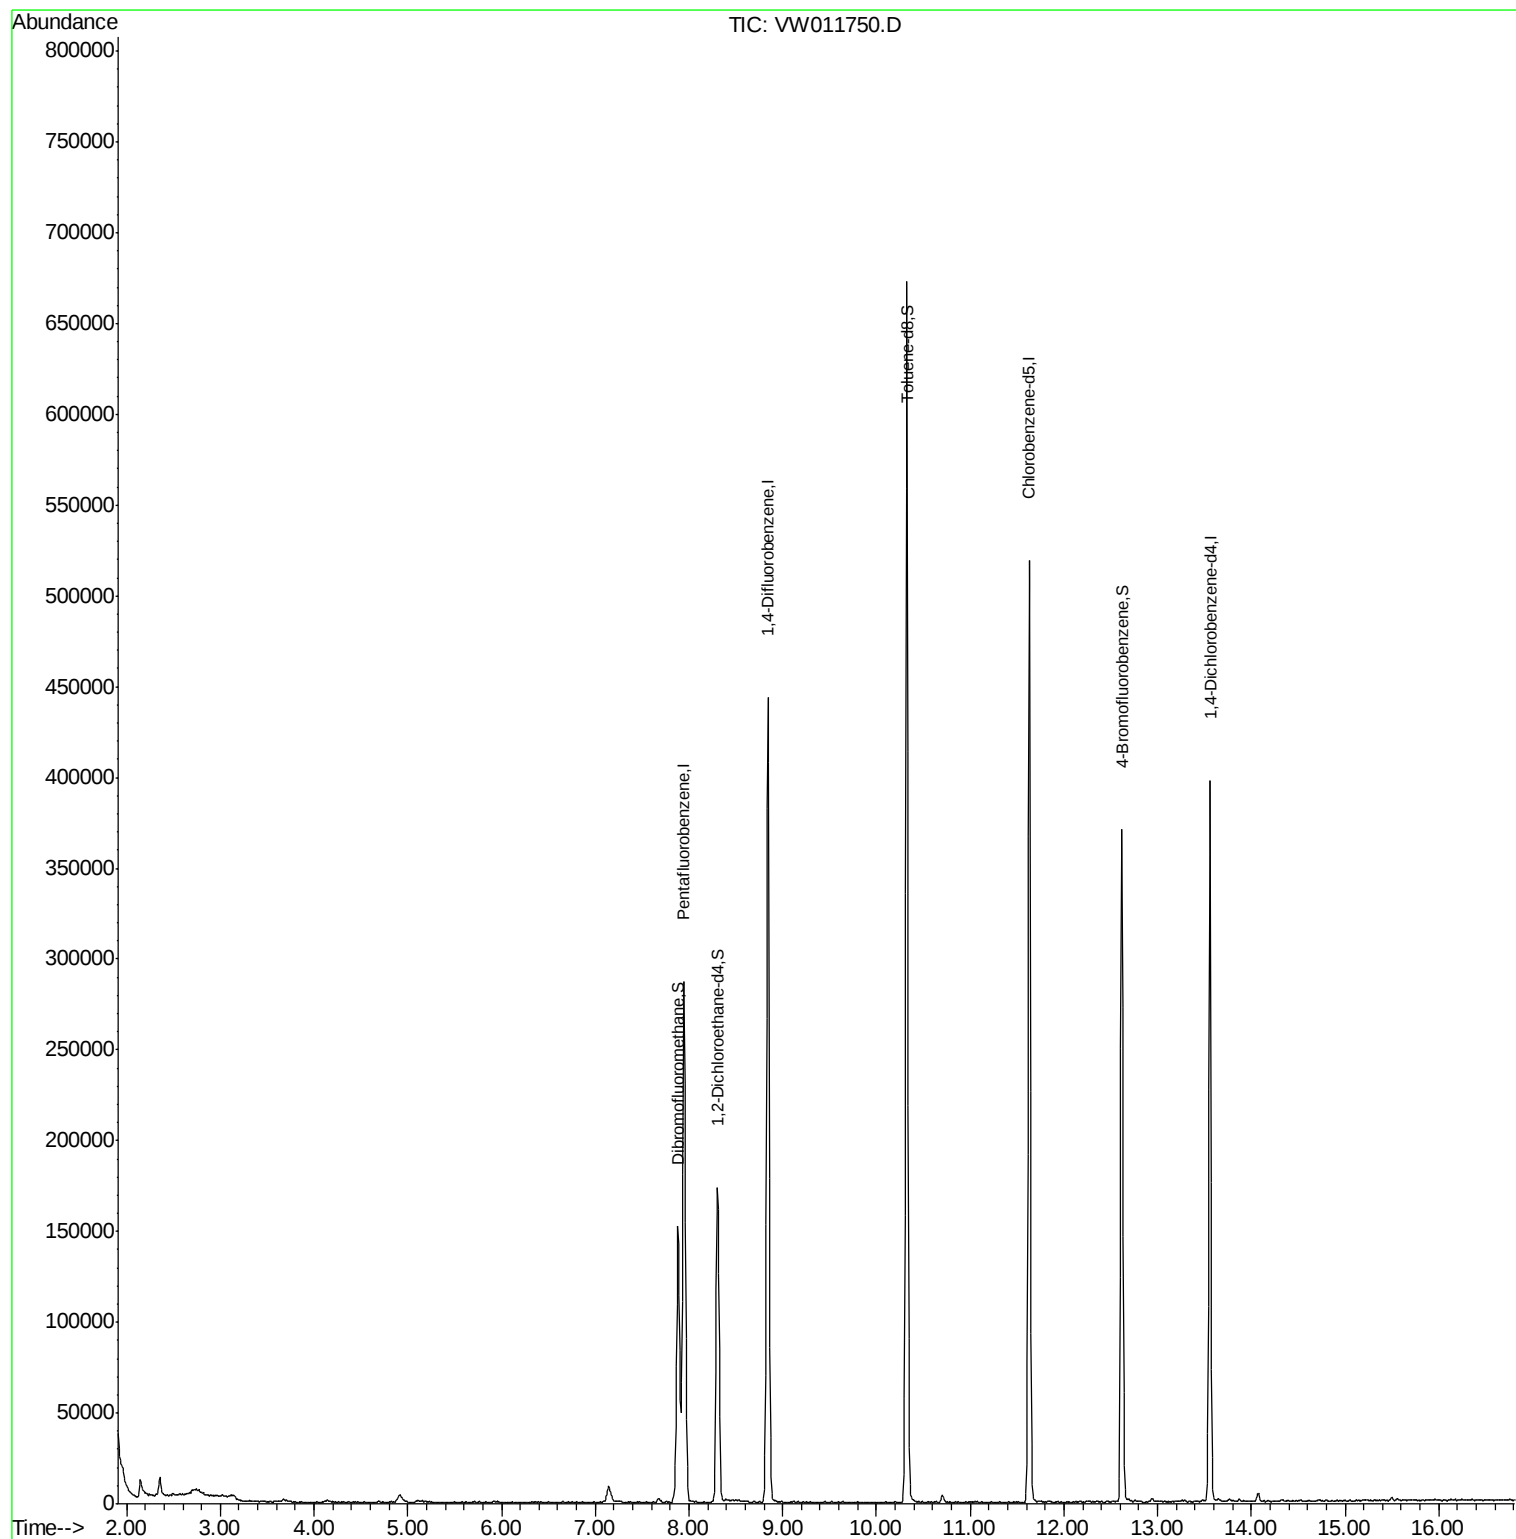

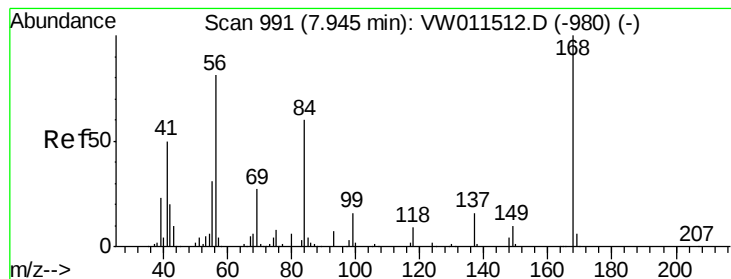

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW011750.D

Acq: 07 Aug 2019 14:48

Instrument :

MSVOA_W

ClientSampleId :


FK-PS-01-054

Tot Ion:168 Resp: 207782

Ion Ratio Lower Upper

168 100

99 61.6 48.2 72.4

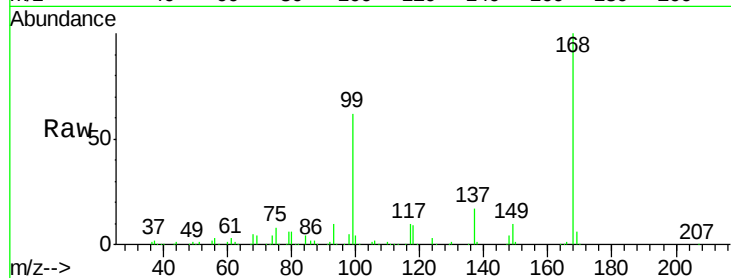

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00 8.10

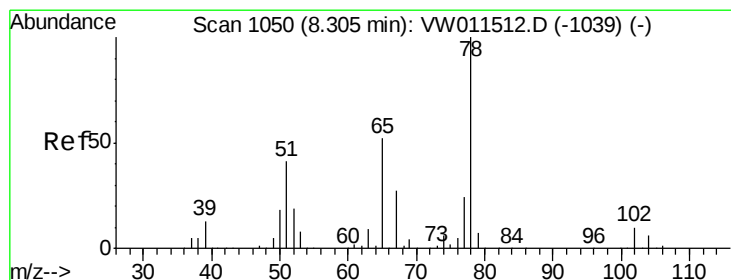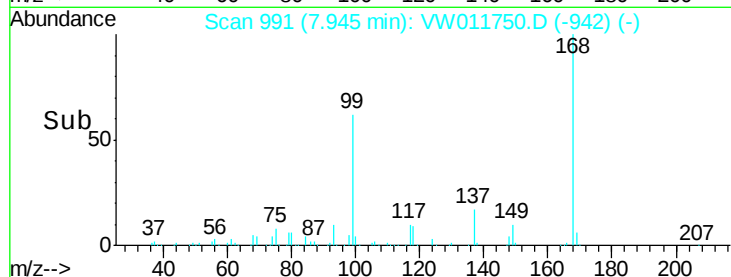

#33

1,2-Dichloroethane-d4

Concen: 58.614 ug/l

RT: 8.30 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW011750.D


Acq: 07 Aug 2019 14:48

Tgt Ion: 65 Resp: 139847

Ion Ratio Lower Upper

65 100

67 51.5 0.0 105.2

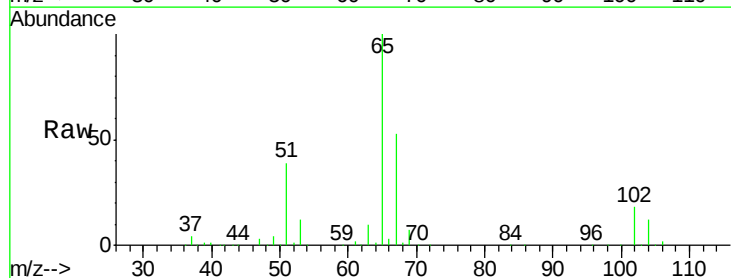

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.30


60000


40000

20000

0

Time--> 8.20 8.30 8.40




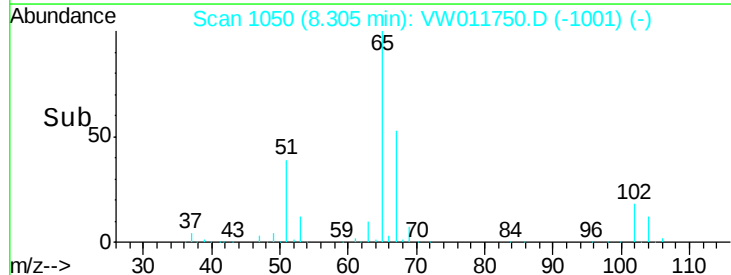


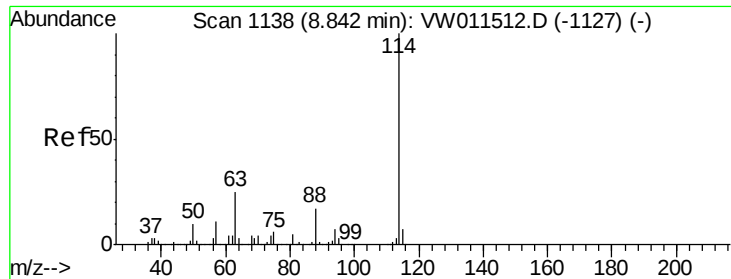

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VW011750.D
 Acq: 07 Aug 2019 14:48




Instrument :
 MSVOA_W
 ClientSampleId :
 FK-PS-01-054


Tot Ion	Ratio	Lower	Upper
114	100		
63	25.3	0.0	49.2
88	17.1	0.0	33.8

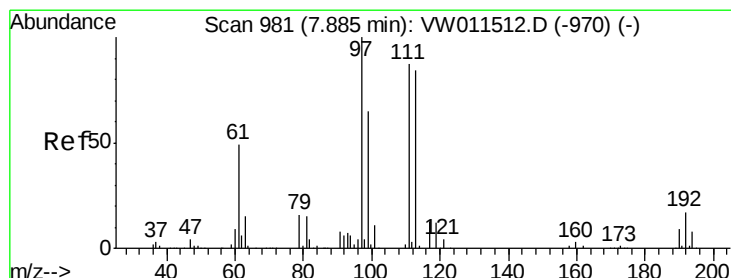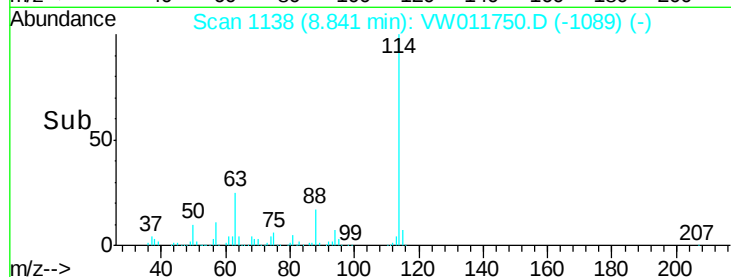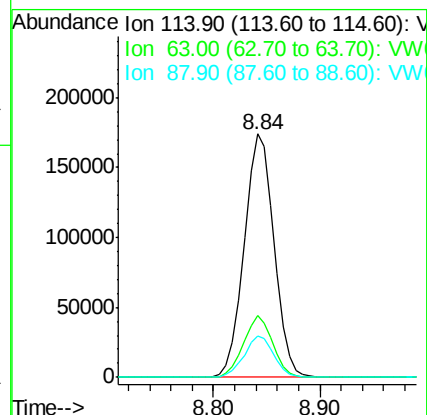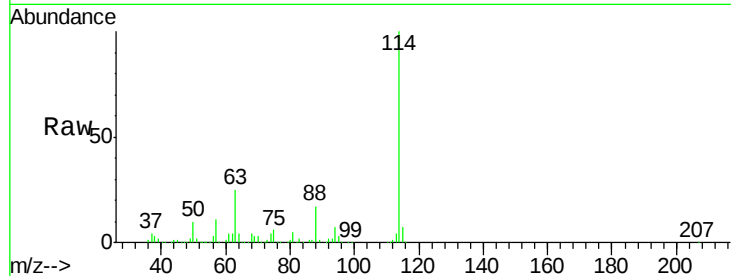

#35
 Dibromofluoromethane
 Concen: 56.557 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.00 min
 Lab File: VW011750.D
 Acq: 07 Aug 2019 14:48

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.7	82.7	124.1
192	19.6	16.1	24.1

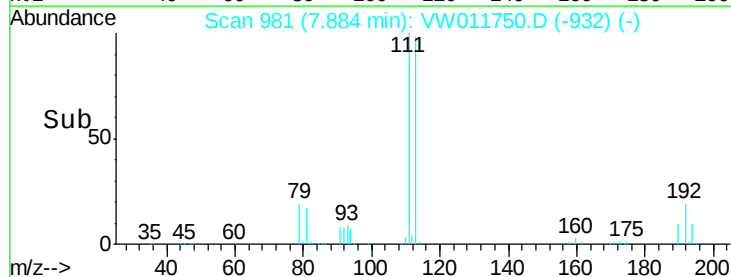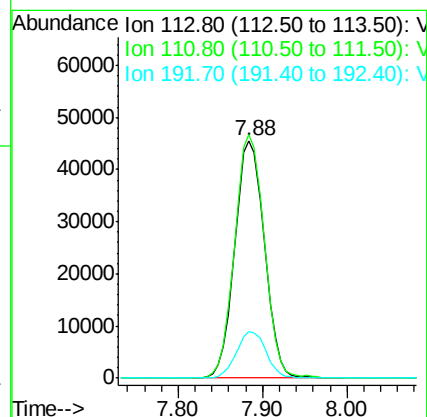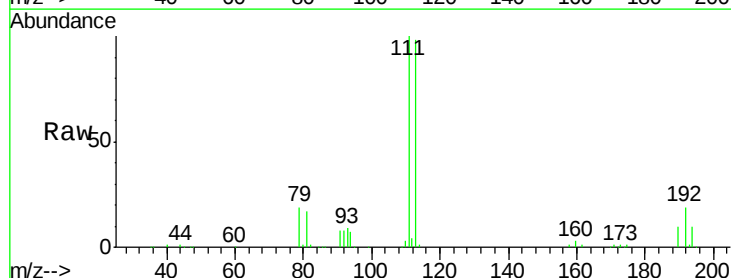

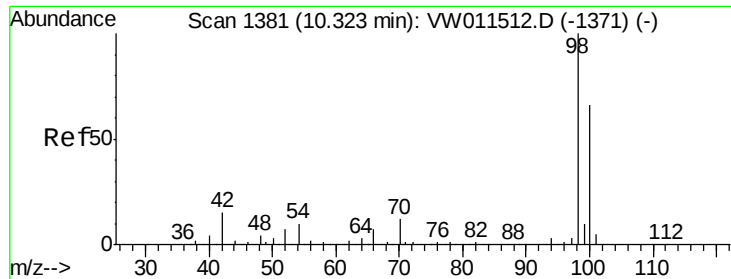

#50

Toluene-d8

Concen: 52.797 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.00 min

Lab File: VW011750.D

Acq: 07 Aug 2019 14:48

Instrument :

MSVOA_W

ClientSampleId :


FK-PS-01-054

Tot Ion: 98 Resp: 415225

Ion Ratio Lower Upper




98 100

100 64.7 52.7 79.1

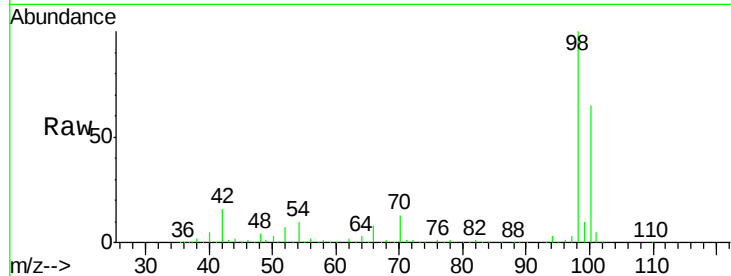

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

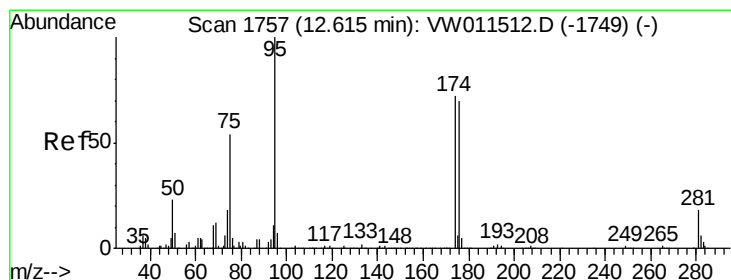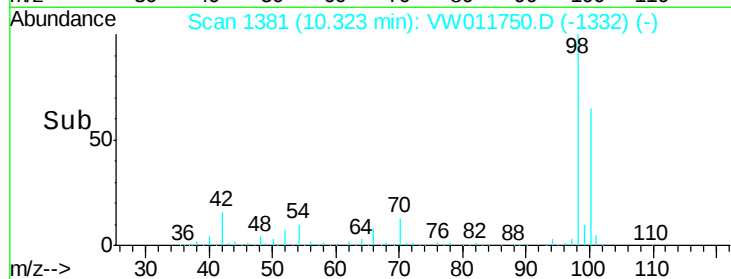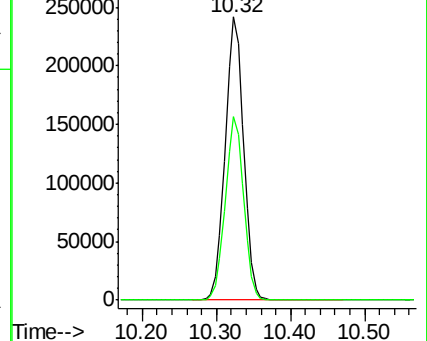

#62

4-Bromofluorobenzene

Concen: 43.039 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.01 min

Lab File: VW011750.D

Acq: 07 Aug 2019 14:48


Tgt Ion: 95 Resp: 120676

Ion Ratio Lower Upper

95 100

174 75.9 0.0 150.2



176 73.6 0.0 144.4

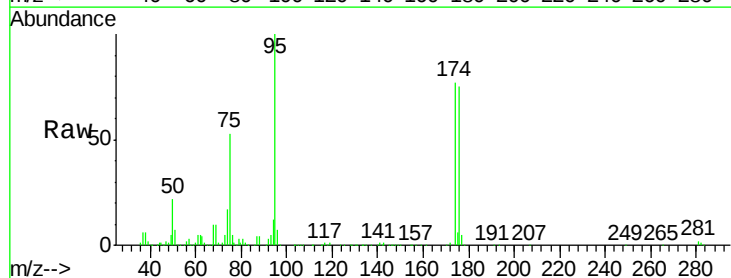


Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



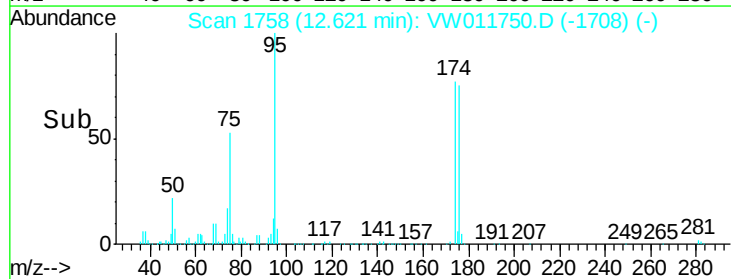
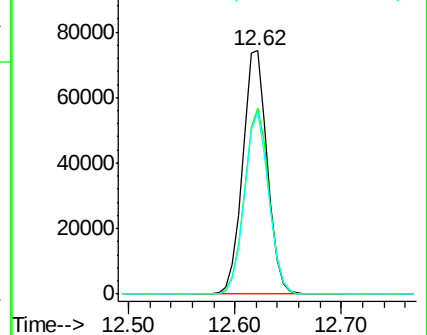


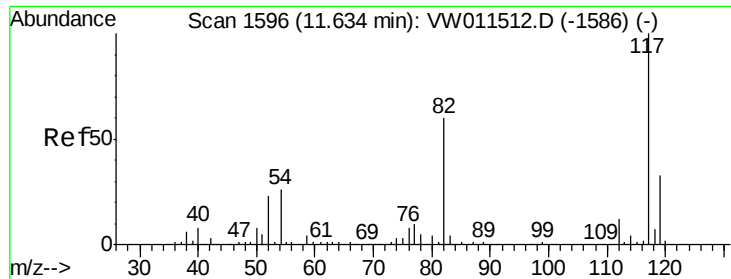

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW011750.D
Acq: 07 Aug 2019 14:48

Instrument :
MSVOA_W
ClientSampleId :
FK-PS-01-054

Tot Ion:117 Resp: 274996
Ion Ratio Lower Upper
117 100
82 58.9 47.9 71.9
119 31.8 26.2 39.2

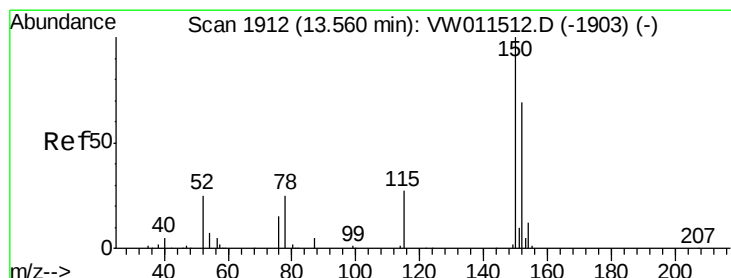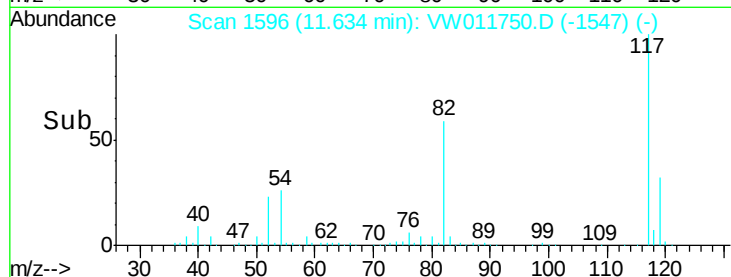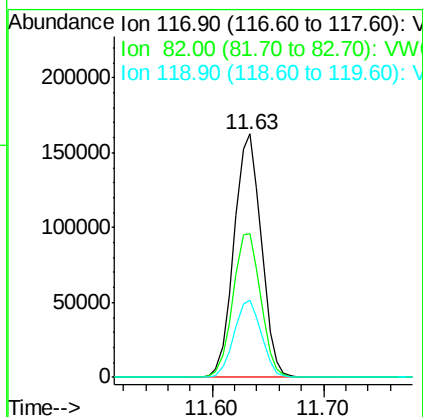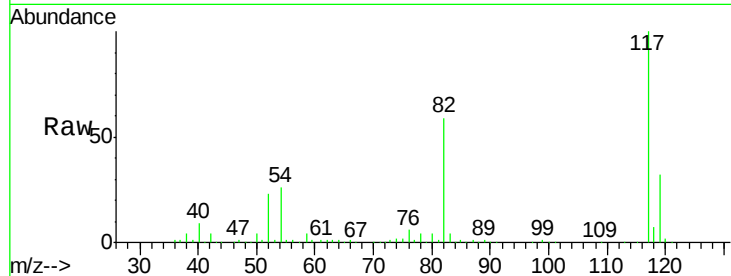

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW011750.D
Acq: 07 Aug 2019 14:48

Tgt Ion:152 Resp: 97271
Ion Ratio Lower Upper
152 100
115 59.5 30.5 91.5
150 153.5 0.0 352.6

