


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW080819\
Data File : VW011740.D
Acq On : 07 Aug 2019 10:00
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
Title : SW846 8260
Last Update : Sat Jul 27 00:23:30 2019

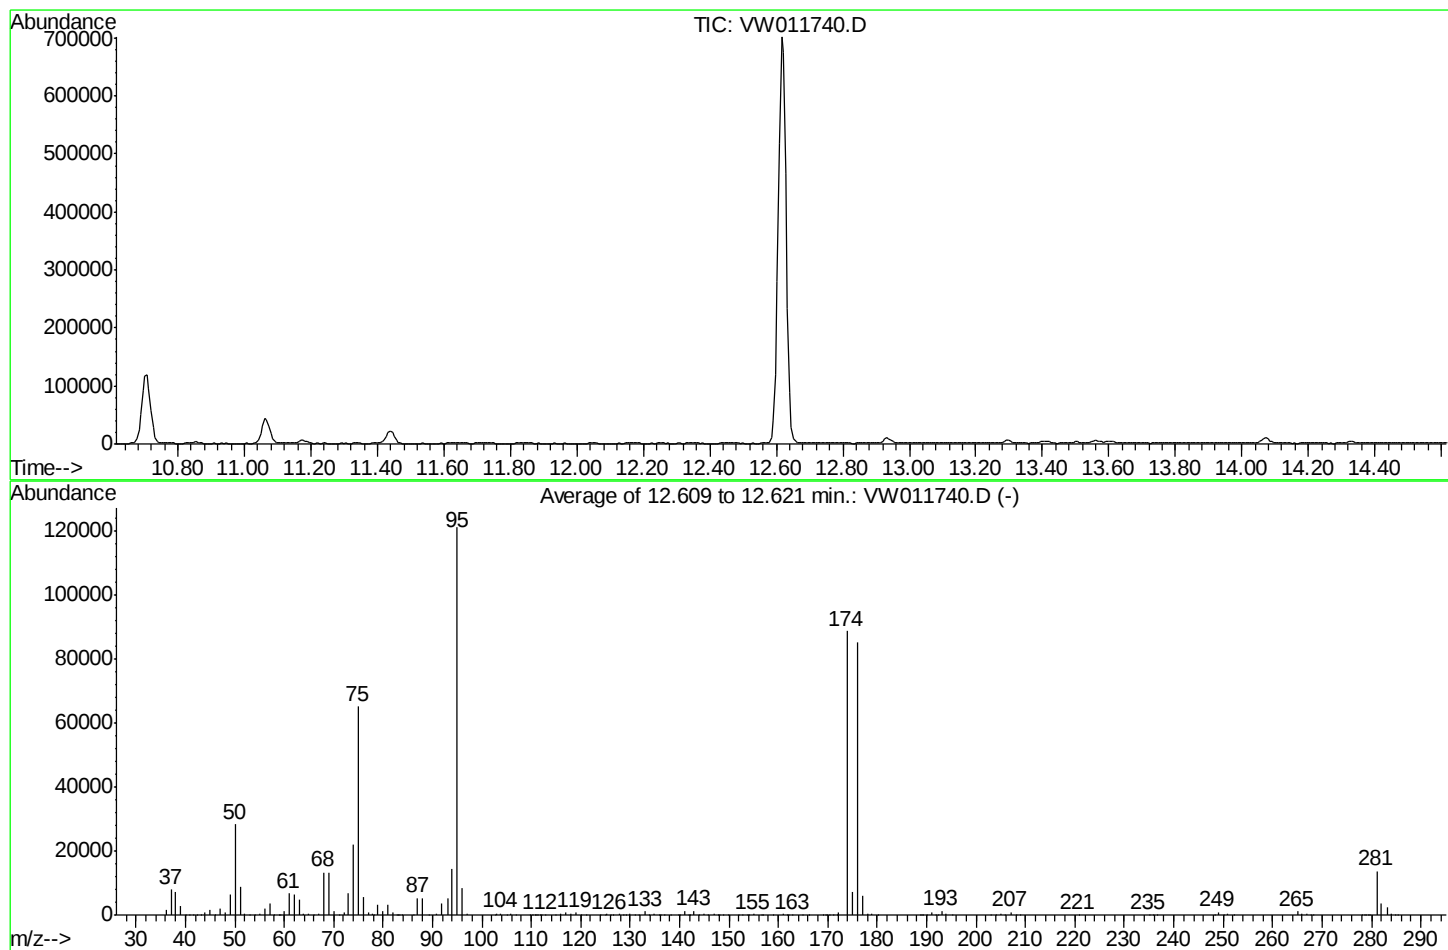

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	28365	PASS
75	95	30	60	53.8	65093	PASS
95	95	100	100	100.0	121058	PASS
96	95	5	9	6.8	8269	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.2	88669	PASS
175	174	5	9	8.0	7078	PASS
176	174	95	101	96.1	85240	PASS
177	176	5	9	7.0	6003	PASS