

Data File : VW011765.D
Acq On : 08 Aug 2019 10:36
Operator : SY/VA
Sample : VW0809SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK20

Quant Time: Aug 09 02:29:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 09 02:27:11 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	361133	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	323146	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	148937	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	106949	21.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.12%
7) Chloroethane-d5	2.89	69	82159	22.43	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.72%
10) 1,1-Dichloroethene-d2	4.01	63	197572	16.95	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.80%
20) 2-Butanone-d5	7.09	46	106272	46.41	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.82%
24) Chloroform-d	7.65	84	231718	23.36	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.44%
26) 1,2-Dichloroethane-d4	8.31	65	142069	24.20	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.80%
29) Benzene-d6	8.27	84	476024	23.43	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.72%
33) 1,2-Dichloropropane-d6	9.27	67	154707	23.58	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.32%
37) Toluene-d8	10.32	98	412515	22.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.48%
38) trans-1,3-Dichloropropene-	10.58	79	64564	22.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.84%
39) 2-Hexanone-d5	10.93	63	70092	45.75	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.50%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	128720	23.63	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.52%
61) 1,2-Dichlorobenzene-d4	13.85	152	139697	24.34	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.36%


Target Compounds						Qvalue
59) 1,2,3-Trichloropropane	13.56	75	20284	4.802	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011765.D
Acq On : 08 Aug 2019 10:36
Operator : SY/VA
Sample : VW0809SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK20

Quant Time: Aug 09 02:29:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 09 02:27:11 2019
Response via : Initial Calibration

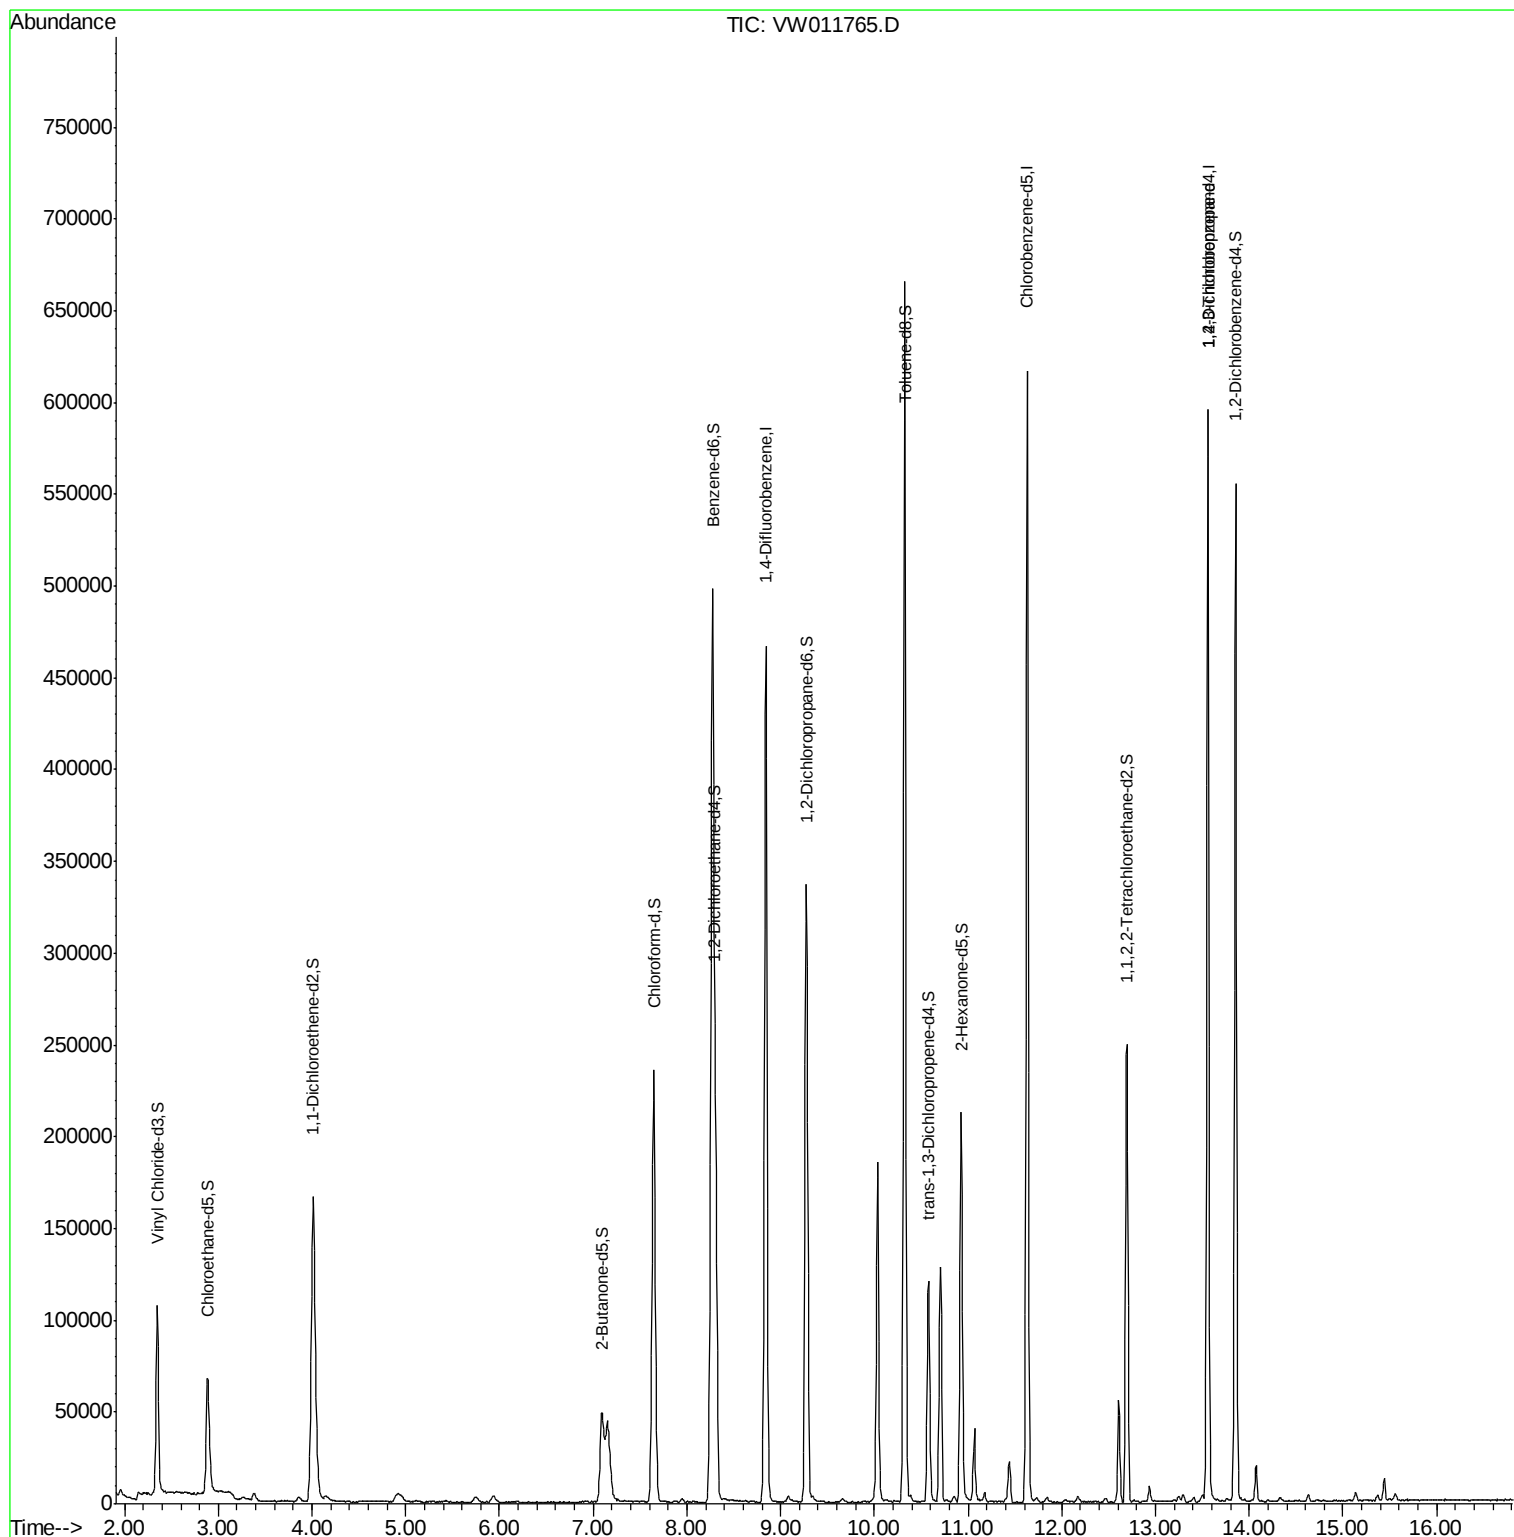

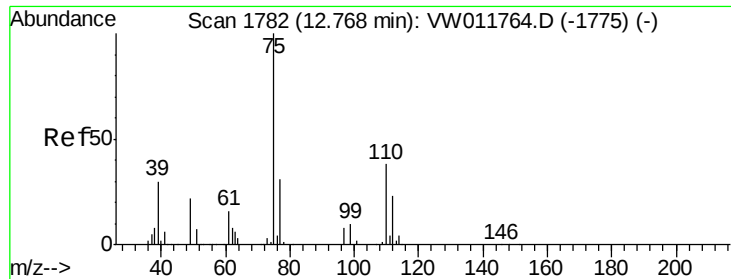

#59

1,2,3-Trichloropropane

Concen: 4.802 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW011765.D

Acq: 08 Aug 2019 10:36

Instrument :

MSVOA_W

ClientSampleId :

VBLK20

Tgt Ion: 75 Resp: 20284

Ion Ratio Lower Upper

75 100

77 37.1 25.1 37.7

