


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080919\
 Data File : VW011763.D
 Acq On : 08 Aug 2019 08:47
 Operator : SY/VA
 Sample : BFB10
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB10

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
 Title : VOC Analysis
 Last Update : Mon Aug 12 18:40:27 2019

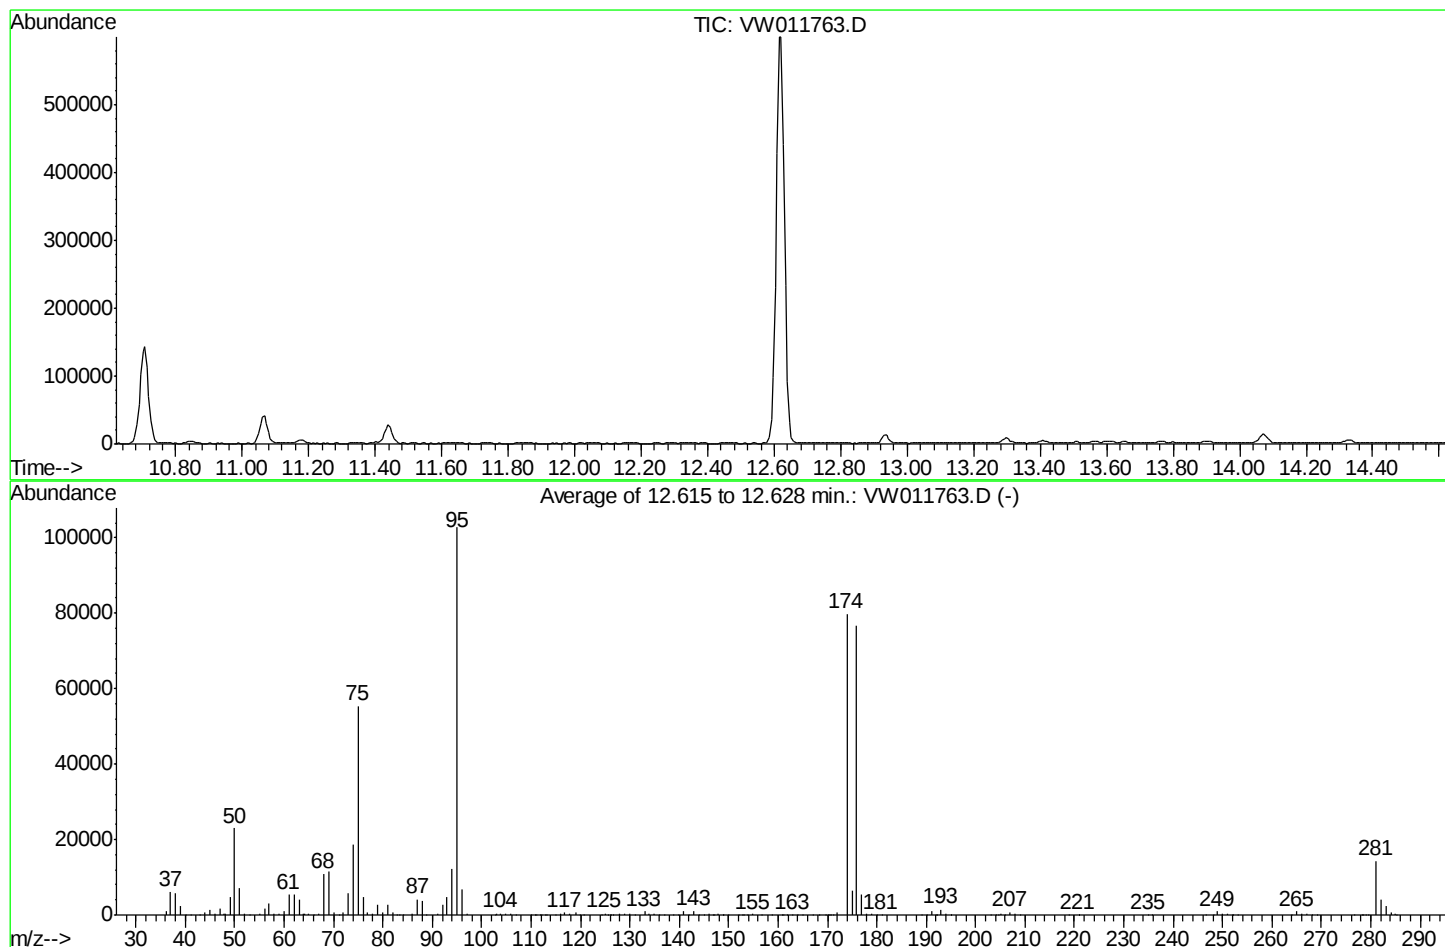

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	22949	PASS
75	95	30	80	53.9	55346	PASS
95	95	100	100	100.0	102776	PASS
96	95	5	9	6.6	6742	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.6	79794	PASS
175	174	5	9	8.0	6411	PASS
176	174	95	101	95.9	76544	PASS
177	176	5	9	7.1	5469	PASS

m/z	Abundance
36.00	1215.0
37.00	7146.0
38.10	6257.0
39.00	2944.0
40.00	428.0
41.00	71.0
43.00	218.0
44.00	1016.0
45.00	1509.0
46.10	205.0
47.00	2294.0
47.90	762.0
49.00	5056.0
50.00	25840.0
51.00	7903.0
52.00	399.0
53.00	120.0
55.00	450.0
56.00	1922.0
57.00	3458.0
58.00	289.0
58.90	272.0
60.00	1164.0
61.00	6094.0
62.00	6129.0
63.00	4526.0
63.90	576.0
65.00	515.0
65.90	108.0
67.10	374.0
68.00	12301.0
69.00	13072.0
70.00	985.0
71.10	77.0
72.00	708.0
73.00	6968.0
74.00	20512.0
75.00	61968.0
76.00	5235.0
76.90	770.0
78.00	505.0
78.90	3021.0
79.90	942.0
80.90	3047.0
81.90	627.0
82.80	152.0
84.20	62.0
86.00	237.0
86.90	4374.0
87.90	4550.0
91.10	368.0
92.00	3257.0
93.00	4853.0
94.00	13087.0
95.00	111496.0
96.00	7782.0
97.00	271.0
102.70	348.0
103.10	330.0
103.80	588.0
104.90	230.0
105.80	422.0
106.90	58.0
110.00	186.0
110.70	285.0
112.00	158.0
112.80	186.0
114.90	175.0
116.00	438.0
116.90	748.0
117.90	468.0
119.00	746.0
119.80	104.0
124.20	67.0
124.90	621.0
126.00	255.0
126.60	91.0
127.90	308.0
128.90	101.0
129.80	417.0
130.90	232.0
133.00	1630.0
133.80	493.0
134.80	465.0
135.90	60.0
136.90	119.0
138.80	53.0
139.80	104.0
141.00	929.0
141.90	181.0
143.00	1092.0
144.00	106.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

144.90	280.0
145.90	268.0
146.90	273.0
147.80	288.0
148.70	143.0
149.80	125.0
153.20	98.0
153.80	89.0
154.90	307.0
156.70	141.0
158.80	117.0
160.80	300.0
161.90	59.0
162.90	282.0
163.80	53.0
164.80	219.0
167.10	53.0
168.40	56.0
170.20	85.0
170.80	128.0
171.90	675.0
173.90	77408.0
175.00	6636.0
175.90	74480.0
176.90	5673.0
178.00	347.0
179.00	478.0
179.90	97.0
181.00	55.0
188.90	225.0
190.00	165.0
191.00	1478.0
191.90	385.0
192.90	2168.0
194.10	405.0
194.90	273.0
203.00	301.0
204.10	85.0
205.00	400.0
207.00	1303.0
207.90	383.0
208.90	106.0
220.80	109.0
235.00	211.0
235.80	101.0
248.10	51.0
249.00	1367.0
249.90	415.0
251.00	751.0
252.00	165.0
253.00	90.0
264.10	67.0
265.00	1484.0
266.10	483.0
267.00	371.0
268.00	59.0
269.00	53.0
276.70	52.0
278.10	84.0
279.00	251.0
281.10	21744.0
282.10	6172.0
283.10	3806.0
284.10	811.0
285.00	370.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

m/z	Abundance
36.00	1353.0
37.00	6722.0
38.00	6333.0
39.00	2577.0
40.00	326.0
41.00	101.0
42.80	125.0
44.00	895.0
45.00	1294.0
46.00	224.0
47.00	1755.0
48.10	720.0
49.00	5100.0
50.00	25592.0
51.00	7852.0
52.10	438.0
53.00	64.0
54.90	422.0
56.00	1876.0
57.00	3499.0
58.00	176.0
58.90	196.0
60.10	1070.0
61.00	6053.0
62.00	5717.0
63.00	4511.0
64.10	578.0
65.00	538.0
66.90	413.0
68.00	12171.0
69.00	12705.0
70.00	930.0
71.10	101.0
72.00	778.0
73.00	6305.0
74.00	20216.0
75.00	61000.0
76.00	5064.0
77.00	797.0
78.00	748.0
78.90	3124.0
79.90	774.0
81.00	3096.0
82.00	706.0
82.80	73.0
83.20	70.0
86.00	203.0
87.00	4720.0
87.90	4326.0
88.80	166.0
91.00	490.0
92.00	3191.0
93.00	5361.0
94.00	13500.0
95.00	113568.0
96.00	7356.0
96.90	192.0
103.10	273.0
103.90	561.0
104.90	242.0
105.90	478.0
107.00	119.0
109.80	124.0
111.10	126.0
111.70	105.0
112.10	115.0
113.00	82.0
114.90	216.0
115.80	452.0
116.80	648.0
118.00	567.0
119.00	802.0
119.90	70.0
120.70	63.0
125.00	466.0
125.60	201.0
126.20	68.0
127.90	362.0
128.90	330.0
129.80	338.0
131.00	145.0
133.10	887.0
134.90	280.0
136.00	102.0
137.00	240.0
139.90	79.0
140.90	1112.0
141.90	214.0
143.00	1032.0
143.90	155.0
145.00	121.0
145.90	180.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

147.10	223.0
147.90	263.0
149.00	259.0
149.90	128.0
151.90	95.0
152.80	58.0
153.20	67.0
153.80	76.0
154.80	195.0
156.80	179.0
158.90	176.0
161.10	165.0
163.00	186.0
164.90	110.0
170.60	142.0
171.10	206.0
172.00	774.0
173.90	88312.0
175.00	7043.0
175.90	84688.0
177.00	6137.0
178.00	266.0
179.00	280.0
179.80	89.0
181.00	83.0
189.00	149.0
191.00	945.0
192.10	222.0
193.00	1350.0
193.90	318.0
195.10	193.0
203.00	113.0
205.10	285.0
206.00	117.0
207.00	841.0
208.00	185.0
208.90	77.0
218.90	87.0
221.00	61.0
234.80	77.0
235.80	51.0
246.70	52.0
248.90	1023.0
250.00	223.0
251.00	308.0
251.80	118.0
253.10	128.0
263.90	59.0
265.00	1004.0
266.10	239.0
266.90	350.0
268.10	60.0
278.40	82.0
279.40	173.0
281.00	14146.0
282.10	3692.0
283.00	2475.0
284.00	528.0
284.90	230.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

m/z	Abundance
36.10	922.0
37.10	4699.0
38.00	4376.0
39.00	1519.0
40.00	406.0
43.00	140.0
44.10	869.0
45.10	867.0
46.00	139.0
47.00	1230.0
47.90	489.0
49.00	3667.0
50.00	17416.0
51.00	5566.0
52.10	339.0
55.10	272.0
56.00	1276.0
57.00	2508.0
58.00	145.0
58.90	130.0
59.90	710.0
61.00	4099.0
62.00	4151.0
63.00	3172.0
64.00	331.0
64.90	259.0
67.00	240.0
68.00	8258.0
69.00	9169.0
70.10	639.0
71.10	86.0
72.00	484.0
73.00	4286.0
74.00	14908.0
75.00	43072.0
76.00	3849.0
77.00	671.0
78.10	237.0
78.90	2025.0
80.00	694.0
80.90	2268.0
81.90	542.0
82.80	105.0
85.90	145.0
87.00	3303.0
88.00	2858.0
91.00	413.0
92.00	2235.0
93.00	3822.0
94.00	10083.0
95.00	83264.0
96.00	5089.0
97.00	169.0
102.80	100.0
103.90	310.0
104.90	138.0
105.90	361.0
107.10	64.0
109.80	83.0
110.90	52.0
111.80	80.0
113.10	72.0
114.70	91.0
115.80	345.0
116.90	529.0
117.80	399.0
118.90	352.0
124.80	191.0
126.20	68.0
127.90	266.0
128.90	192.0
129.90	351.0
130.80	129.0
133.00	372.0
133.80	156.0
134.90	143.0
136.00	58.0
137.10	180.0
140.00	118.0
140.90	1018.0
141.90	94.0
142.90	995.0
143.90	118.0
144.90	143.0
145.90	189.0
147.10	107.0
147.90	282.0
148.80	103.0
150.00	118.0
151.90	98.0
153.10	83.0
154.90	248.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

156.80	142.0
158.90	167.0
161.00	222.0
163.00	83.0
164.90	63.0
169.50	53.0
170.40	62.0
171.00	121.0
171.90	617.0
173.90	73664.0
175.00	5554.0
175.90	70464.0
177.00	4598.0
177.80	153.0
178.90	81.0
188.90	97.0
190.90	335.0
191.70	109.0
193.10	609.0
193.90	96.0
195.00	83.0
203.10	70.0
204.50	78.0
205.10	87.0
206.00	64.0
207.00	420.0
207.90	86.0
248.90	531.0
250.10	138.0
251.00	139.0
252.10	61.0
265.00	430.0
265.90	148.0
267.00	170.0
268.20	67.0
278.30	55.0
281.00	7297.0
282.00	2167.0
283.10	878.0
284.00	258.0
284.90	111.0
285.30	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

Scan 1749 (12.567 min): VW011763.D
BFB10

m/z	Abundance
39.30	66.0
40.00	290.0
41.20	55.0
42.10	74.0
43.00	99.0
44.00	369.0
55.30	52.0
207.00	58.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10