
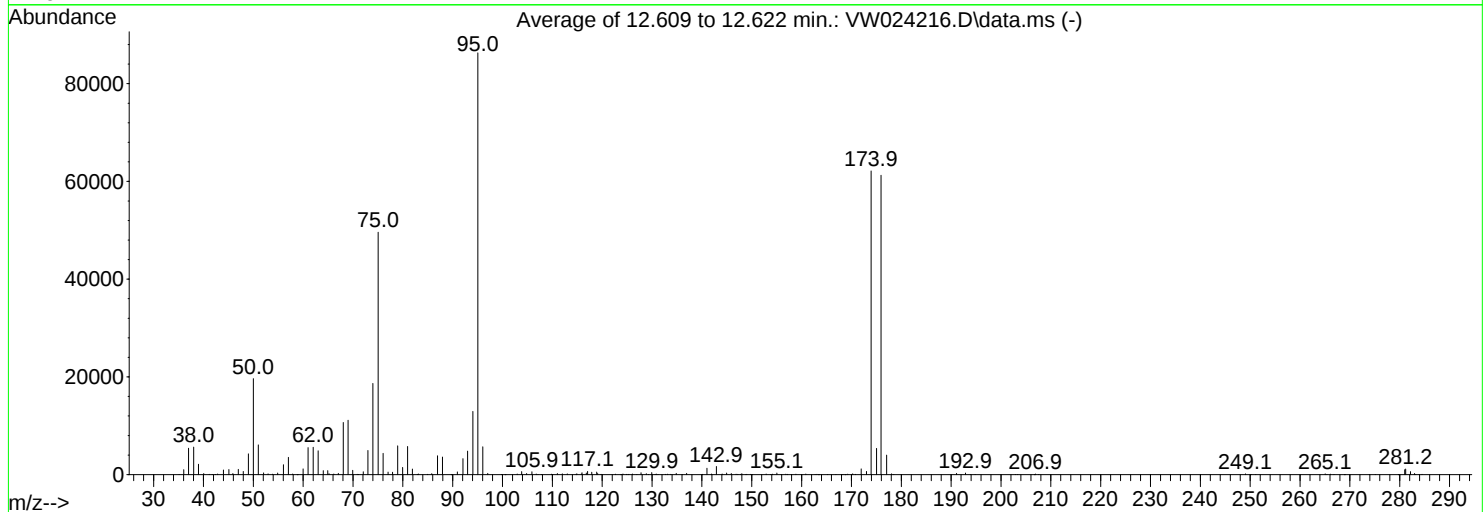


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081022\
Data File : VW024216.D
Acq On : 10 Aug 2022 08:06
Operator : SY/VA
Sample : BFB406
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB406

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Title : SFAM01.0
Last Update : Wed Aug 10 01:09:21 2022

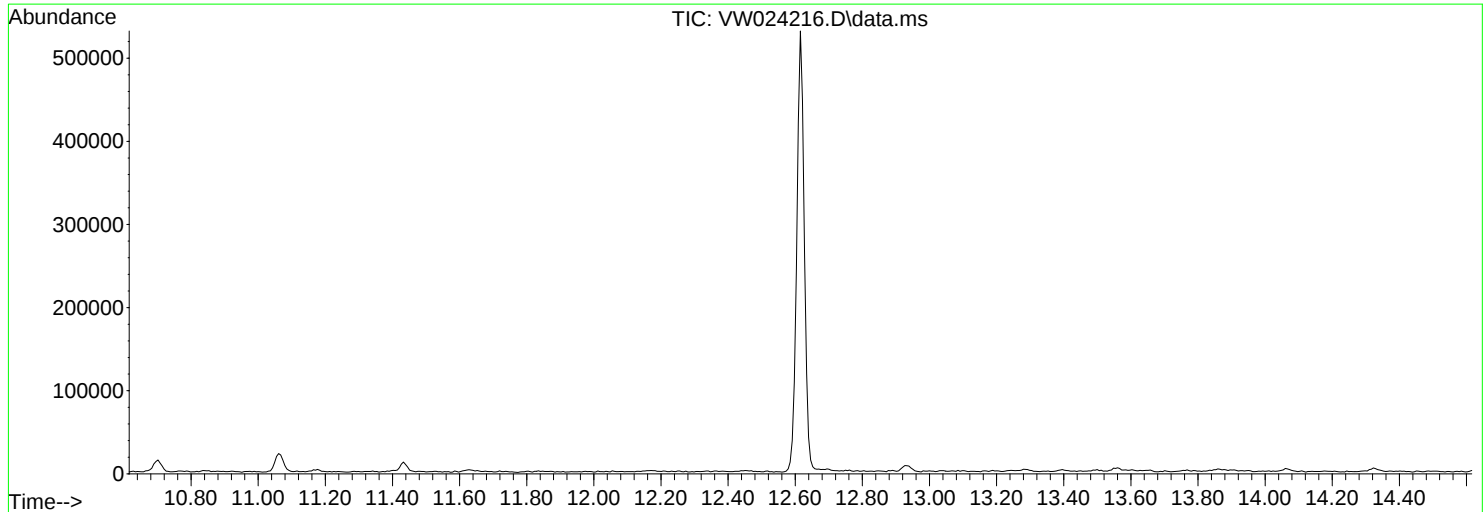

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	19656	PASS
75	95	30	80	57.5	49584	PASS
95	95	100	100	100.0	86307	PASS
96	95	5	9	6.6	5686	PASS
173	174	0.00	2	1.1	658	PASS
174	95	50	120	72.0	62152	PASS
175	174	5	9	8.6	5358	PASS
176	174	95	105	98.6	61264	PASS
177	176	5	10	6.5	3993	PASS

m/z	Abundance
36.10	202.0
36.70	116.0
37.60	116.0
37.80	115.0
39.00	113.0
39.90	186.0
40.80	99.0
42.10	127.0
43.00	76.0
44.00	203.0
44.60	76.0
46.50	59.0
47.30	57.0
50.40	66.0
51.70	67.0
52.90	99.0
56.30	54.0
57.80	76.0
68.80	64.0
103.00	59.0
139.10	55.0
158.30	52.0
199.80	84.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

m/z	Abundance
35.10	102.0
36.10	1336.0
37.00	5938.0
38.10	5706.0
39.00	2395.0
39.90	305.0
41.10	154.0
41.70	84.0
42.40	64.0
42.90	145.0
44.00	1085.0
45.10	994.0
45.90	223.0
47.00	1135.0
48.10	544.0
49.00	4076.0
50.00	19584.0
51.00	5932.0
52.10	404.0
53.00	242.0
53.80	185.0
55.00	326.0
56.00	2132.0
57.00	3336.0
58.00	223.0
60.00	1280.0
61.00	4847.0
62.00	5247.0
63.00	4356.0
64.00	977.0
65.00	1025.0
66.30	85.0
67.00	188.0
68.00	9389.0
69.00	10374.0
70.00	880.0
70.90	113.0
72.10	556.0
73.00	4654.0
74.00	18144.0
75.00	47000.0
76.00	4071.0
77.20	460.0
78.00	344.0
79.00	5484.0
79.90	1351.0
80.90	5400.0
81.90	1006.0
83.20	116.0
85.80	308.0
87.00	3563.0
88.00	3248.0
90.90	486.0
92.10	2993.0
93.00	4191.0
94.10	12082.0
95.00	76688.0
96.00	5088.0
97.10	353.0
102.90	207.0
103.90	508.0
104.90	320.0
106.00	553.0
106.80	227.0
109.80	144.0
111.10	220.0
112.00	150.0
113.00	184.0
114.80	91.0
115.00	93.0
115.80	449.0
117.00	901.0
118.00	515.0
118.90	726.0
119.80	81.0
122.70	55.0
125.20	128.0
126.10	228.0
127.80	208.0
128.80	112.0
129.30	152.0
130.00	406.0
130.60	120.0
131.20	65.0
133.10	327.0
133.80	97.0
134.90	336.0
137.00	177.0
141.00	1109.0
142.90	1368.0
144.10	65.0
145.10	317.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

145.90	212.0
146.80	108.0
147.80	172.0
148.80	108.0
149.80	96.0
152.90	191.0
153.80	83.0
155.10	242.0
156.80	100.0
157.30	65.0
158.90	111.0
160.90	81.0
162.70	100.0
163.10	126.0
165.20	124.0
166.90	64.0
168.30	76.0
169.20	122.0
170.20	125.0
170.80	214.0
172.10	1039.0
173.90	50440.0
175.00	4633.0
176.00	49896.0
177.00	3597.0
178.00	146.0
178.50	113.0
191.10	385.0
192.90	489.0
193.90	124.0
194.80	55.0
202.90	83.0
206.90	185.0
207.60	56.0
249.00	288.0
251.10	70.0
265.10	279.0
266.10	190.0
266.80	70.0
268.90	53.0
273.90	70.0
279.70	56.0
281.00	3104.0
282.20	741.0
282.90	390.0
283.90	108.0
284.50	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

m/z	Abundance
36.00	1180.0
37.00	5713.0
38.00	6423.0
39.00	2702.0
40.10	394.0
40.80	62.0
41.20	56.0
41.80	65.0
42.40	61.0
42.90	126.0
44.00	1391.0
45.10	1180.0
45.80	197.0
46.90	1314.0
48.00	728.0
49.00	5131.0
50.00	22376.0
51.00	6735.0
52.00	411.0
53.00	400.0
53.90	120.0
54.80	480.0
56.10	2357.0
57.10	4150.0
58.00	174.0
60.00	1394.0
61.00	6567.0
62.00	6403.0
63.00	5913.0
64.10	919.0
64.90	590.0
65.20	582.0
66.10	127.0
67.00	337.0
68.00	13217.0
69.00	13667.0
70.00	1090.0
71.10	138.0
72.00	694.0
73.00	5774.0
74.00	21440.0
75.10	57488.0
76.10	4876.0
77.00	564.0
77.90	651.0
79.00	6913.0
80.00	1803.0
80.90	6636.0
81.90	1273.0
83.10	323.0
85.00	77.0
85.70	125.0
86.90	4278.0
88.00	4328.0
89.70	58.0
91.00	743.0
92.00	3687.0
93.00	5057.0
94.00	15125.0
95.00	100960.0
96.10	7020.0
97.00	236.0
99.80	68.0
103.00	162.0
103.90	658.0
104.80	214.0
105.90	548.0
107.10	87.0
107.80	61.0
110.10	148.0
110.90	261.0
112.00	210.0
113.00	146.0
114.80	177.0
116.00	617.0
117.10	1079.0
117.80	580.0
119.10	713.0
119.80	67.0
122.70	126.0
123.70	57.0
124.20	147.0
124.90	82.0
125.40	114.0
126.10	90.0
126.90	55.0
127.80	541.0
128.90	237.0
130.00	536.0
130.80	182.0
132.70	186.0
133.70	151.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

134.80	272.0
136.10	76.0
136.90	380.0
140.10	156.0
141.00	1658.0
141.90	214.0
142.90	2013.0
144.00	193.0
144.90	397.0
145.80	234.0
147.20	223.0
148.00	351.0
149.00	180.0
149.80	120.0
152.80	73.0
154.10	127.0
155.00	300.0
157.10	126.0
158.00	70.0
158.90	142.0
160.80	178.0
162.90	75.0
169.20	97.0
170.30	174.0
171.90	1407.0
174.00	67744.0
175.10	5894.0
175.90	67240.0
177.00	4593.0
178.10	145.0
191.10	196.0
192.90	374.0
194.80	66.0
203.40	62.0
207.00	236.0
207.60	72.0
249.10	141.0
250.00	54.0
264.90	127.0
265.40	82.0
266.10	74.0
281.20	1998.0
282.10	676.0
283.00	328.0
284.50	81.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

m/z	Abundance
36.10	1157.0
37.00	4561.0
38.10	4745.0
39.00	1590.0
40.00	293.0
40.80	118.0
42.10	83.0
42.70	165.0
43.00	147.0
44.00	1020.0
45.10	995.0
46.00	240.0
47.10	830.0
47.90	714.0
49.00	3555.0
50.00	17008.0
51.00	5644.0
52.10	253.0
53.00	137.0
55.00	236.0
56.00	1608.0
57.10	3151.0
58.00	208.0
58.80	52.0
60.00	910.0
61.00	5203.0
62.00	5119.0
63.00	4355.0
64.10	545.0
65.00	889.0
66.10	135.0
67.10	312.0
68.10	9451.0
69.00	9382.0
69.90	740.0
70.80	83.0
72.10	517.0
73.00	4451.0
74.00	16363.0
75.00	44264.0
76.00	4072.0
77.00	541.0
78.00	469.0
78.90	5329.0
79.90	1257.0
81.00	5282.0
81.90	1205.0
82.90	191.0
84.90	114.0
85.90	211.0
87.00	3791.0
87.90	3245.0
90.90	434.0
92.00	3182.0
93.00	5233.0
94.00	11621.0
95.10	81272.0
96.00	4950.0
97.10	162.0
100.50	58.0
102.90	176.0
103.80	692.0
104.80	116.0
105.80	699.0
106.70	138.0
107.90	80.0
109.90	124.0
111.00	223.0
112.00	145.0
113.00	179.0
114.90	372.0
115.90	607.0
116.80	969.0
117.90	434.0
118.90	812.0
119.70	51.0
122.50	73.0
124.10	217.0
124.80	118.0
125.30	86.0
126.00	126.0
127.00	63.0
127.80	484.0
128.90	253.0
129.80	310.0
130.90	238.0
134.90	203.0
136.00	54.0
137.00	221.0
141.00	1206.0
141.90	186.0
142.90	1630.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

144.00	150.0
144.80	280.0
146.00	275.0
146.90	173.0
148.00	200.0
150.10	100.0
153.00	123.0
154.20	132.0
155.00	454.0
155.90	65.0
156.90	189.0
157.90	54.0
158.70	91.0
160.90	179.0
163.40	54.0
168.00	70.0
168.70	53.0
169.30	84.0
170.30	210.0
171.90	1045.0
173.00	1974.0
174.00	68272.0
175.00	5548.0
176.00	66656.0
177.10	3789.0
178.00	213.0
191.20	171.0
193.00	161.0
203.30	68.0
206.70	50.0
249.00	81.0
264.90	70.0
265.40	66.0
275.10	60.0
281.20	1450.0
282.10	498.0
283.20	207.0
284.30	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406