
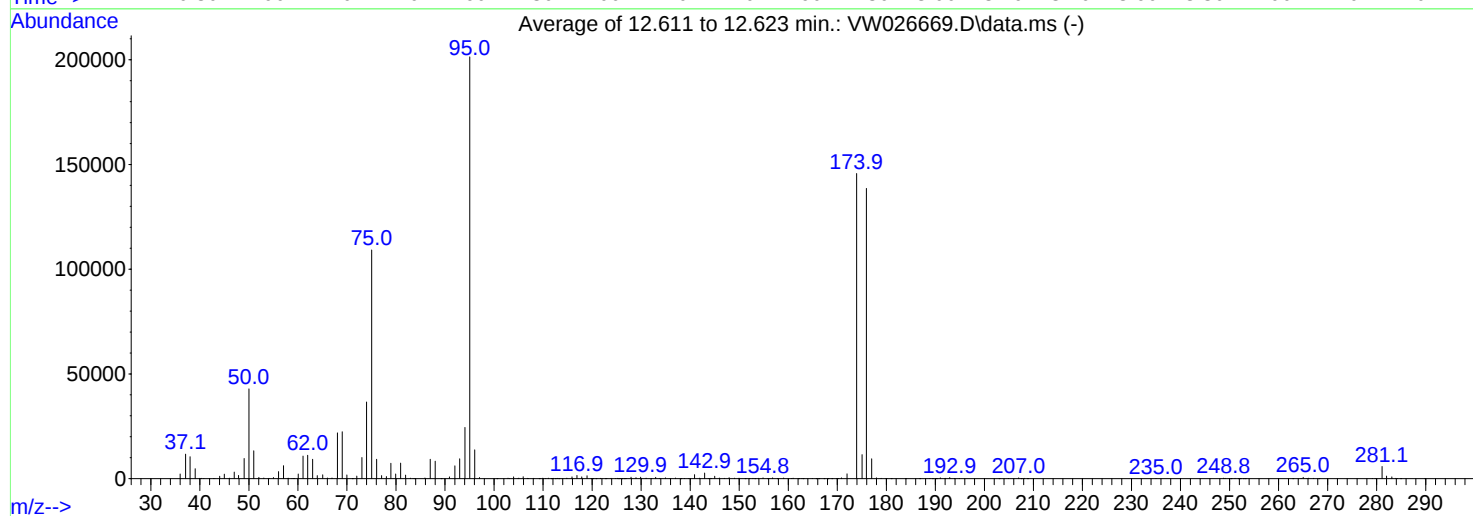


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081023\
Data File : VW026669.D
Acq On : 10 Aug 2023 09:26
Operator : SY/MD
Sample : BFB559
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Title : SFAM01.0
Last Update : Mon Aug 14 23:23:26 2023

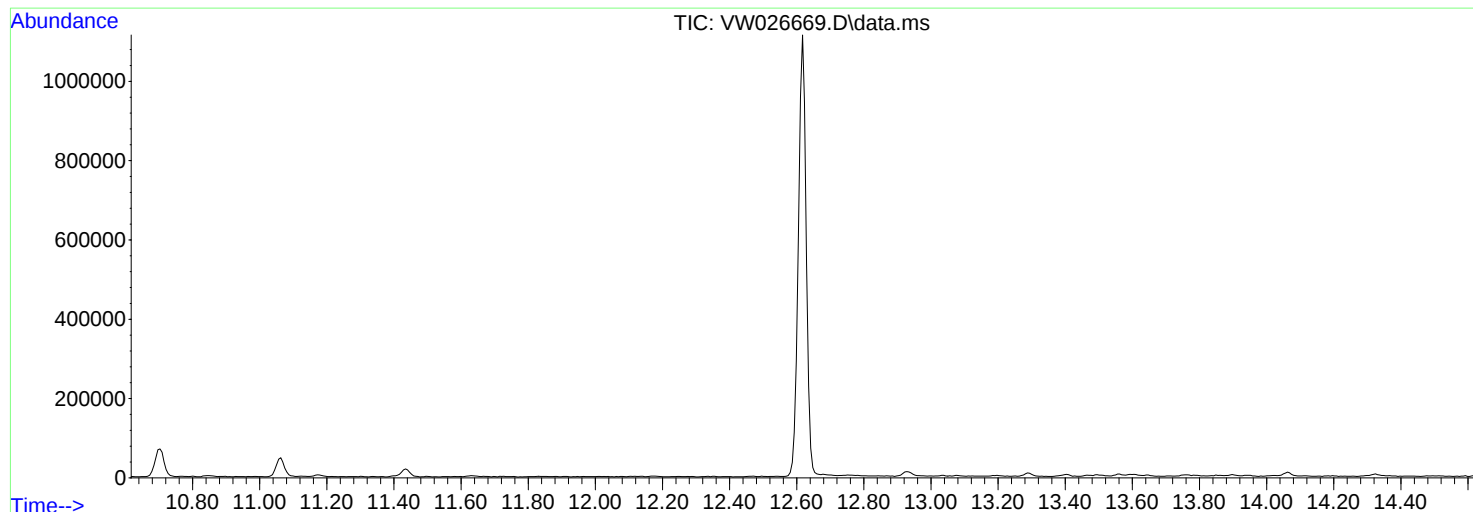

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	42847	PASS
75	95	30	80	54.2	109176	PASS
95	95	100	100	100.0	201387	PASS
96	95	5	9	6.8	13764	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	145712	PASS
175	174	5	9	7.9	11451	PASS
176	174	95	105	95.1	138608	PASS
177	176	5	10	6.9	9501	PASS