

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081119\
 Data File : VW011809.D
 Acq On : 09 Aug 2019 13:29
 Operator : SY/VA
 Sample : K4215-13
 Misc : 4.32G/10ML/MSVOA W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETOC4

Manual Integrations
 APPROVED

MMDadoda
 8/12/2019 1:09:50 PM

Quant Time: Aug 10 04:58:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 10 03:43:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	125476	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	68784	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	13873	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	64104	36.28	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	145.12%
7) Chloroethane-d5	2.89	69	51579	40.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	162.12%#
10) 1,1-Dichloroethene-d2	4.02	63	89778	22.16	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	88.64%
20) 2-Butanone-d5	7.08	46	68401	85.98	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	171.96%#
24) Chloroform-d	7.65	84	113790	33.02	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	132.08%
26) 1,2-Dichloroethane-d4	8.31	65	81211	39.82	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	159.28%#
29) Benzene-d6	8.27	84	195677	45.24	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	180.96%#
33) 1,2-Dichloropropane-d6	9.27	67	70486	50.48	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	201.92%#
37) Toluene-d8	10.32	98	104084	27.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.44%
38) trans-1,3-Dichloropropene-	10.58	79	21847	35.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	142.80%#
39) 2-Hexanone-d5	10.93	63	33556	102.89	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	205.78%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	46014	39.68	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	158.72%#
61) 1,2-Dichlorobenzene-d4	13.85	152	13494	25.24	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.96%

Target Compounds					Ovalue
13) Acetone	4.14	43	5251	6.163 ug/L	97
16) Methylene chloride	4.92	84	7044m	3.597 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081119\
Data File : VW011809.D
Acq On : 09 Aug 2019 13:29
Operator : SY/VA
Sample : K4215-13
Misc : 4.32G/10ML/MSVOA W/SOIL
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
ETOC4

Manual Integrations
APPROVED

MMDadoda
8/12/2019 1:09:50 PM

Quant Time: Aug 10 04:58:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 10 03:43:50 2019
Response via : Initial Calibration

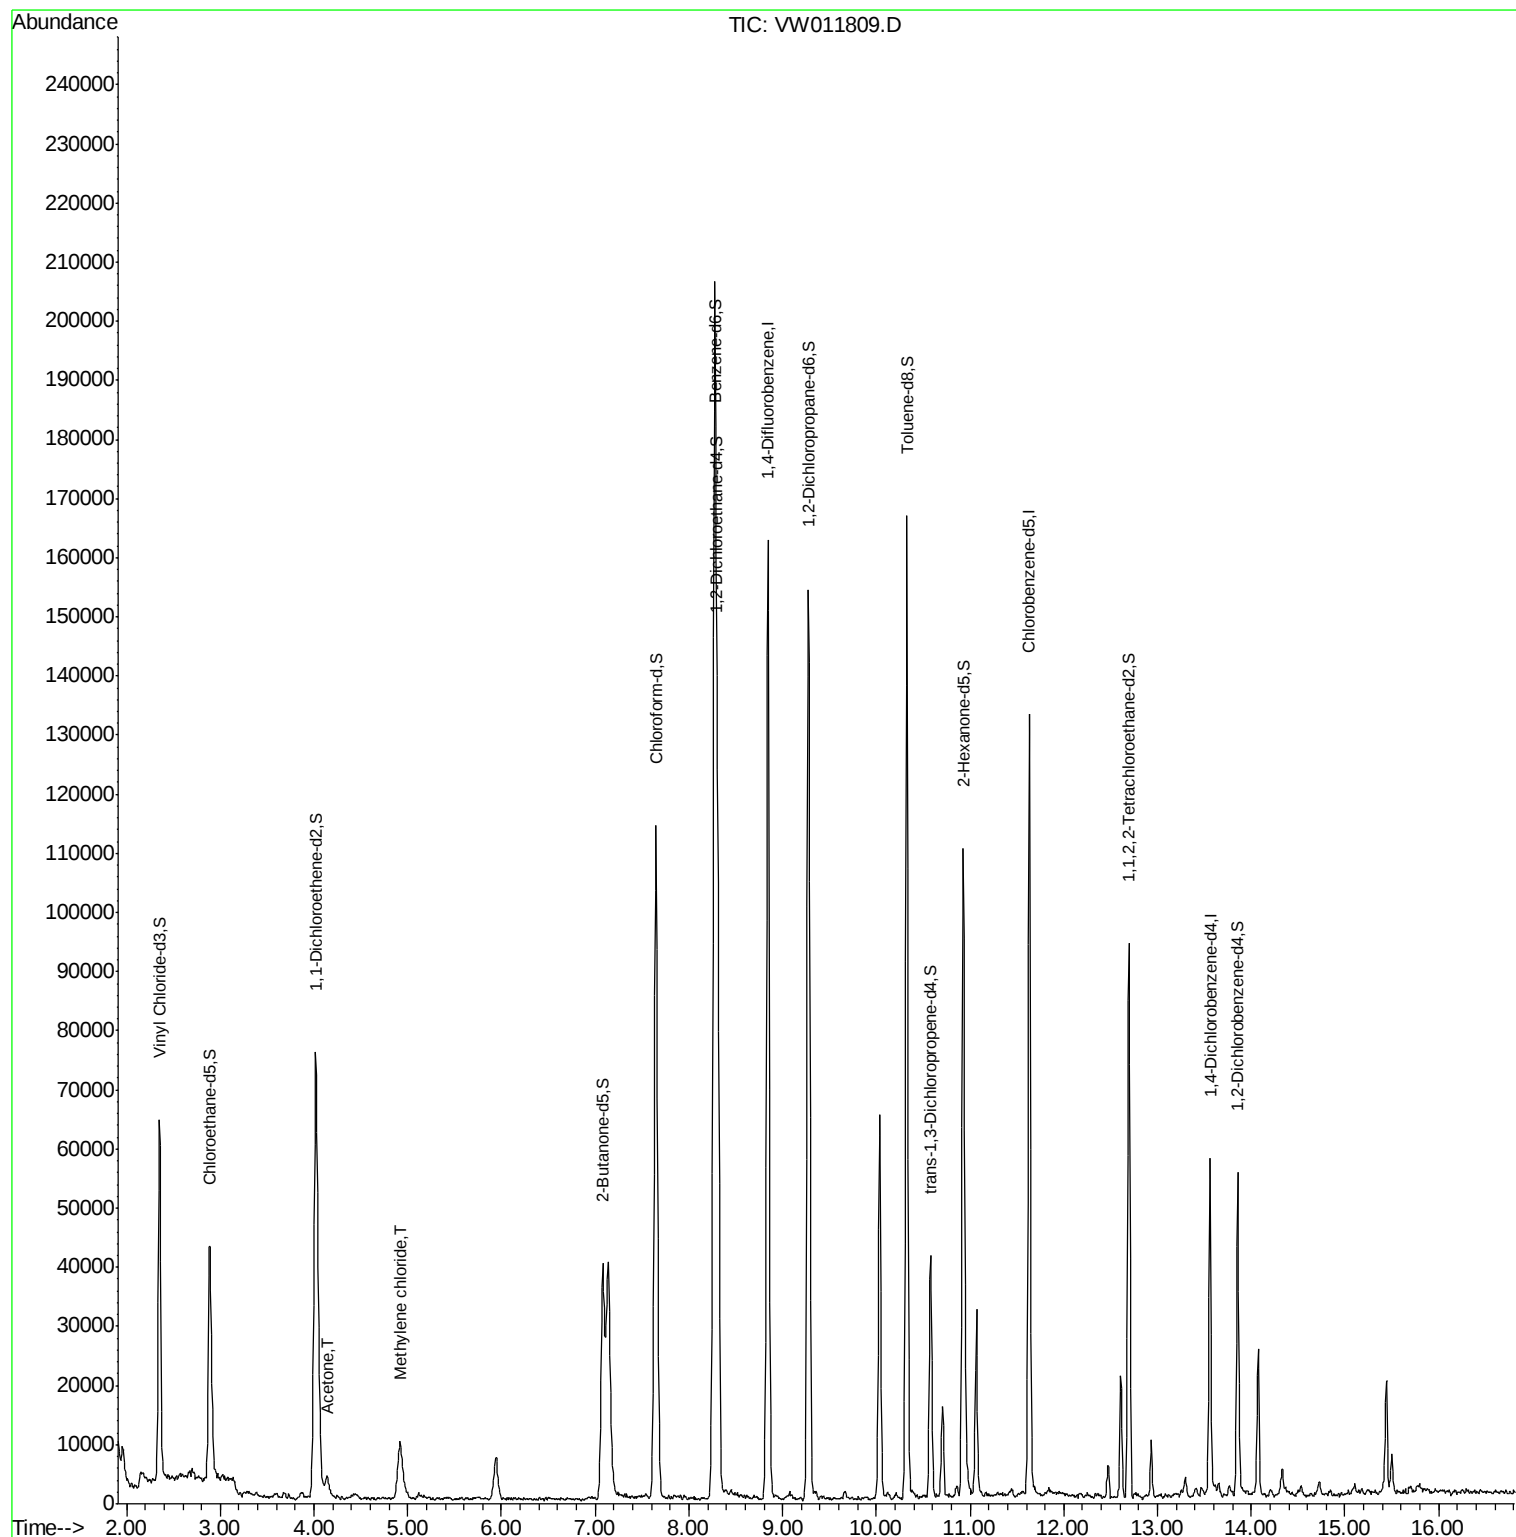

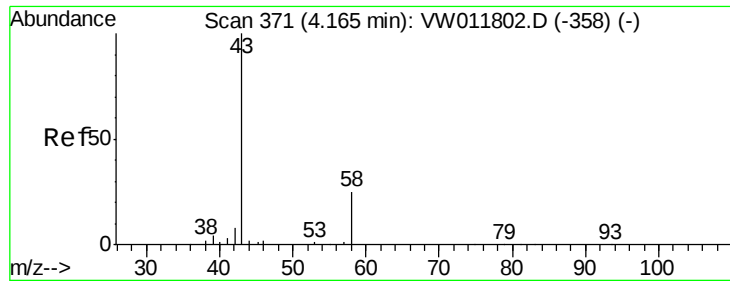

#13

Acetone

Concen: 6.163 ug/L

RT: 4.14 min Scan# 367

Delta R.T. -0.02 min

Lab File: VW011809.D

Acq: 09 Aug 2019 13:29

Instrument :

MSVOA_W

ClientSampleId :

ETOC4

Tot Ion: 43 Resp: 5251

Ion Ratio Lower Upper

43 100


58 28.4 0.0 53.4

Manual Integrations

APPROVED

MMDadoda

8/12/2019 1:09:50 PM

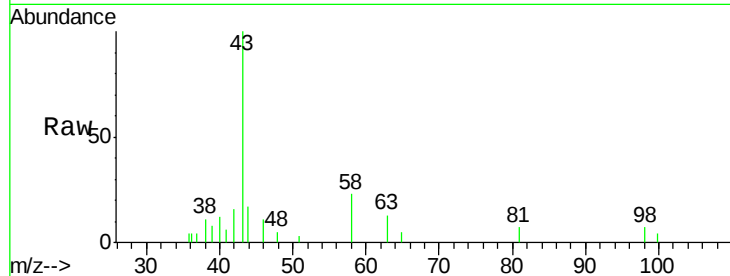

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.14



1500

1000

500

0

Time-->

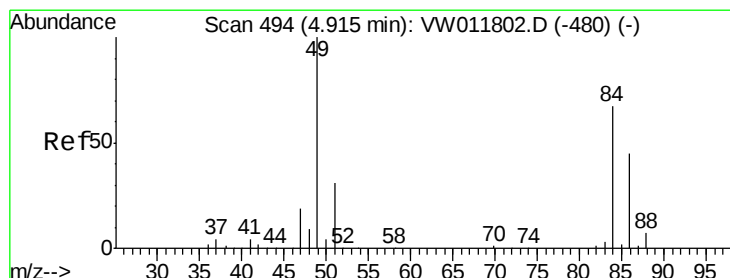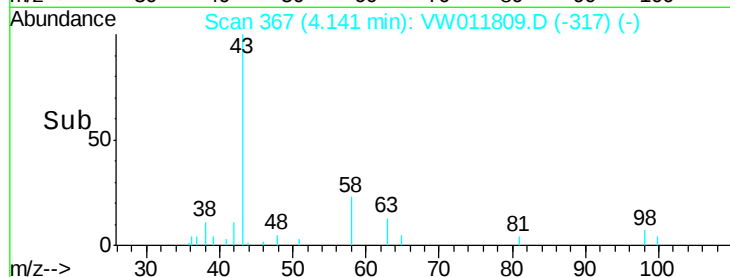

#16

Methylene chloride

Concen: 3.597 ug/L m

RT: 4.92 min Scan# 494

Delta R.T. 0.00 min

Lab File: VW011809.D

Acq: 09 Aug 2019 13:29


Tgt Ion: 84 Resp: 7044

Ion Ratio Lower Upper

84 100

49 161.0 106.8 198.4

86 56.0 42.8 79.4

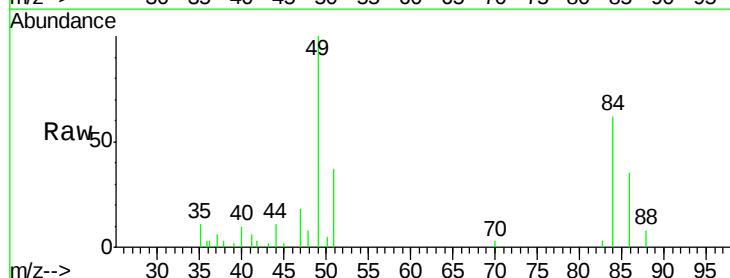

Abundance Ion 84.00 (83.70 to 84.70): VW

Ion 49.00 (48.70 to 49.70): VW

Ion 86.00 (85.70 to 86.70): VW

4.92

4000

3000

2000

1000

0

Time-->

