


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081119\
 Data File : VW011801.D
 Acq On : 09 Aug 2019 09:21
 Operator : SY/VA
 Sample : BFB11
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB11

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
 Title : VOC Analysis
 Last Update : Mon Aug 12 16:40:43 2019

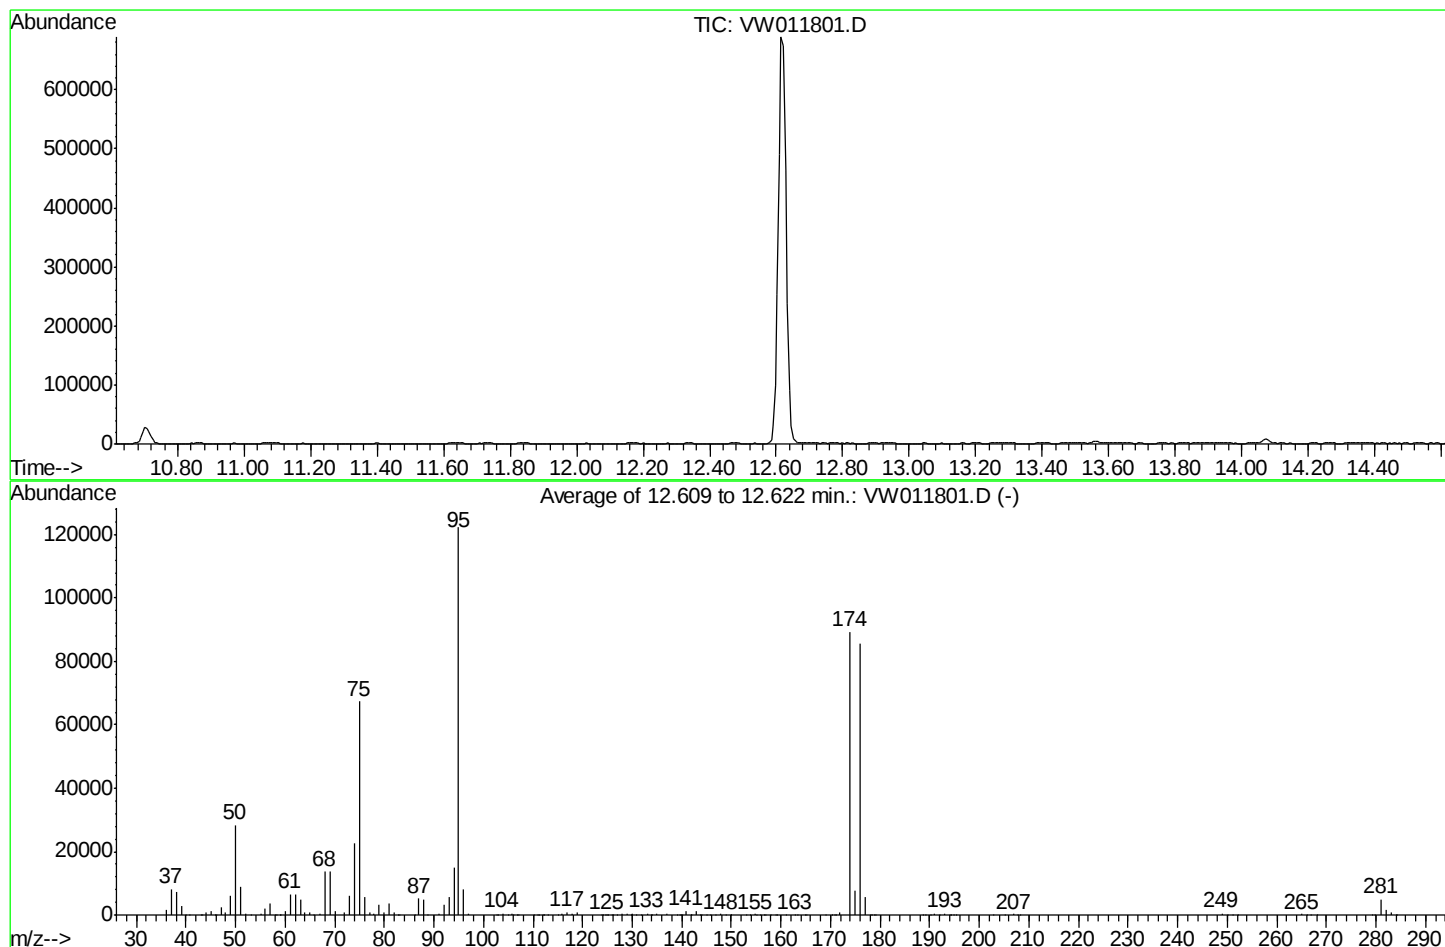

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	28408	PASS
75	95	30	80	55.0	67296	PASS
95	95	100	100	100.0	122301	PASS
96	95	5	9	6.7	8174	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.0	89317	PASS
175	174	5	9	8.4	7488	PASS
176	174	95	101	95.9	85650	PASS
177	176	5	9	6.8	5787	PASS

m/z	Abundance
36.00	1435.0
37.10	6890.0
38.00	5933.0
39.10	2576.0
40.10	265.0
41.00	84.0
43.00	197.0
44.00	1038.0
45.00	1166.0
45.80	103.0
46.20	123.0
47.10	1731.0
47.90	858.0
49.10	4972.0
50.00	24400.0
51.00	7867.0
52.10	332.0
53.00	103.0
55.00	368.0
56.00	1775.0
57.00	3049.0
58.10	189.0
58.90	133.0
59.90	896.0
61.00	5528.0
62.00	5815.0
63.00	4180.0
64.00	773.0
65.00	701.0
65.90	104.0
67.10	391.0
68.00	11155.0
69.00	11313.0
70.00	784.0
72.00	628.0
73.00	5245.0
74.00	18176.0
75.00	55696.0
76.10	4787.0
76.90	605.0
77.90	411.0
78.90	2764.0
79.90	990.0
80.90	2845.0
81.90	710.0
83.10	102.0
86.00	156.0
87.00	4156.0
88.00	3925.0
91.00	352.0
92.00	2773.0
93.00	4410.0
94.00	11745.0
95.00	97528.0
96.00	6741.0
97.00	203.0
103.00	226.0
103.90	490.0
105.00	176.0
105.80	440.0
107.00	110.0
110.00	63.0
110.80	120.0
111.90	83.0
112.80	81.0
114.90	147.0
115.90	398.0
116.90	593.0
118.00	366.0
118.80	529.0
124.90	238.0
126.20	82.0
127.00	57.0
127.90	278.0
128.90	175.0
129.70	255.0
130.90	115.0
133.00	609.0
133.70	136.0
134.10	112.0
134.80	284.0
136.90	218.0
139.60	91.0
140.10	116.0
140.90	913.0
142.00	128.0
142.90	979.0
143.80	61.0
145.00	184.0
145.70	163.0
146.90	141.0
147.90	313.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

149.80	89.0
153.00	96.0
153.80	72.0
154.80	314.0
156.70	164.0
158.90	160.0
161.00	108.0
162.80	120.0
163.30	57.0
164.90	80.0
168.90	105.0
170.30	119.0
171.10	224.0
171.90	649.0
173.90	62264.0
175.00	5448.0
175.90	61456.0
176.90	4071.0
177.90	201.0
178.80	125.0
189.00	119.0
190.10	77.0
190.90	450.0
191.80	199.0
193.00	761.0
193.90	101.0
194.10	104.0
194.70	52.0
205.10	154.0
206.90	418.0
207.80	95.0
208.30	80.0
249.00	548.0
250.10	145.0
251.00	117.0
265.10	348.0
266.00	166.0
267.00	127.0
268.00	69.0
279.30	95.0
281.00	5749.0
282.10	1773.0
283.00	1119.0
283.90	193.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

m/z	Abundance
36.00	1611.0
37.10	9125.0
38.10	7990.0
39.10	3338.0
40.00	403.0
40.70	93.0
43.00	152.0
44.00	1259.0
45.00	1365.0
46.10	229.0
47.10	2666.0
48.00	1211.0
49.00	7325.0
50.00	31896.0
51.00	9938.0
52.00	395.0
53.00	148.0
55.00	371.0
56.00	2185.0
57.00	4455.0
58.20	177.0
59.10	116.0
59.90	1577.0
61.00	6950.0
62.00	7365.0
63.00	5572.0
63.90	582.0
65.10	692.0
65.90	147.0
67.00	383.0
68.00	15256.0
69.00	15692.0
70.00	1225.0
72.10	726.0
73.00	7498.0
74.00	25264.0
75.00	74472.0
76.00	6211.0
77.00	799.0
77.90	593.0
78.90	3744.0
79.90	1062.0
80.90	4163.0
81.90	933.0
82.80	124.0
86.00	154.0
86.90	6030.0
88.00	5841.0
91.00	589.0
92.00	3500.0
93.00	6473.0
94.00	17144.0
95.00	135744.0
96.00	9287.0
97.00	232.0
103.00	145.0
103.80	583.0
105.00	235.0
106.00	612.0
106.80	153.0
110.10	93.0
111.00	157.0
111.80	100.0
112.90	135.0
114.90	109.0
115.80	554.0
116.90	949.0
117.90	588.0
118.90	790.0
124.00	114.0
124.60	115.0
125.10	141.0
125.80	93.0
127.90	380.0
128.90	233.0
129.90	488.0
130.90	217.0
133.10	422.0
133.90	130.0
134.70	209.0
136.90	274.0
139.00	82.0
139.80	98.0
141.00	1340.0
141.70	177.0
142.90	1383.0
144.00	119.0
144.80	236.0
145.80	220.0
146.90	174.0
147.90	257.0
148.90	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

150.00	141.0
152.90	87.0
153.90	109.0
155.10	297.0
155.90	83.0
156.90	269.0
157.80	52.0
158.70	198.0
161.00	272.0
162.90	91.0
165.20	71.0
168.80	72.0
170.80	210.0
171.90	925.0
173.90	99560.0
175.00	8248.0
175.90	95032.0
177.00	6704.0
178.00	222.0
178.90	169.0
188.70	56.0
191.00	400.0
191.90	103.0
193.00	635.0
194.20	59.0
195.20	97.0
202.80	72.0
205.10	104.0
207.00	396.0
248.90	424.0
250.00	132.0
250.90	180.0
252.00	63.0
265.00	493.0
265.90	129.0
266.80	130.0
279.20	89.0
279.80	100.0
281.00	5459.0
282.00	1612.0
283.10	945.0
284.00	249.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

m/z	Abundance
36.00	1616.0
37.00	8647.0
38.00	7372.0
39.10	2590.0
40.00	349.0
41.00	65.0
43.20	174.0
44.00	1165.0
45.00	1359.0
45.90	216.0
47.00	2335.0
48.00	996.0
49.00	6494.0
50.00	28928.0
51.10	9308.0
52.10	425.0
53.10	84.0
55.10	458.0
56.00	2054.0
57.00	4007.0
57.90	191.0
59.20	109.0
60.00	1401.0
61.00	6916.0
62.00	6401.0
63.10	5266.0
64.00	528.0
65.10	484.0
65.80	99.0
67.00	565.0
68.00	14262.0
69.00	14435.0
70.00	1127.0
72.00	808.0
73.00	6068.0
74.00	24344.0
75.00	71720.0
76.00	5771.0
77.10	753.0
78.00	670.0
79.00	3691.0
80.00	1002.0
80.90	3519.0
81.90	851.0
83.00	144.0
86.10	187.0
87.00	5389.0
88.00	5375.0
88.80	215.0
91.00	409.0
92.00	3506.0
93.00	6481.0
94.00	15680.0
95.00	133632.0
96.00	8496.0
97.10	318.0
102.70	84.0
103.90	700.0
104.90	177.0
105.80	476.0
107.10	139.0
111.10	88.0
112.10	167.0
112.80	80.0
115.00	194.0
115.90	483.0
116.90	1015.0
117.80	520.0
118.90	759.0
123.70	84.0
125.00	84.0
125.80	75.0
127.90	529.0
128.80	242.0
129.90	436.0
130.90	178.0
131.90	59.0
133.00	300.0
133.80	106.0
134.90	223.0
136.80	188.0
139.90	124.0
140.90	1474.0
141.80	202.0
143.00	1207.0
144.00	121.0
144.90	198.0
145.90	254.0
146.70	176.0
147.90	365.0
148.90	115.0
149.80	233.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

152.90	118.0
153.90	99.0
154.90	378.0
155.90	95.0
156.80	205.0
157.80	62.0
159.10	170.0
160.80	177.0
162.90	79.0
168.80	76.0
170.20	113.0
171.20	244.0
171.90	790.0
173.90	106128.0
175.00	8769.0
175.90	100464.0
177.00	6588.0
177.80	162.0
178.20	125.0
179.10	60.0
191.00	308.0
192.90	379.0
205.10	91.0
207.00	180.0
249.00	254.0
249.90	94.0
250.90	156.0
265.00	342.0
266.10	90.0
267.00	54.0
279.20	56.0
281.10	3970.0
282.00	1164.0
283.00	557.0
284.20	161.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

Scan 1748 (12.561 min): VW011801.D
BFB11

m/z	Abundance
37.00	61.0
40.00	294.0
40.90	89.0
44.00	260.0
56.80	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11