


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081120\
Data File : VW016122.D
Acq On : 11 Aug 2020 07:07
Operator : SY/VA
Sample : BFB07
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB07

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
Title : VOC Analysis
Last Update : Tue Aug 11 01:19:31 2020

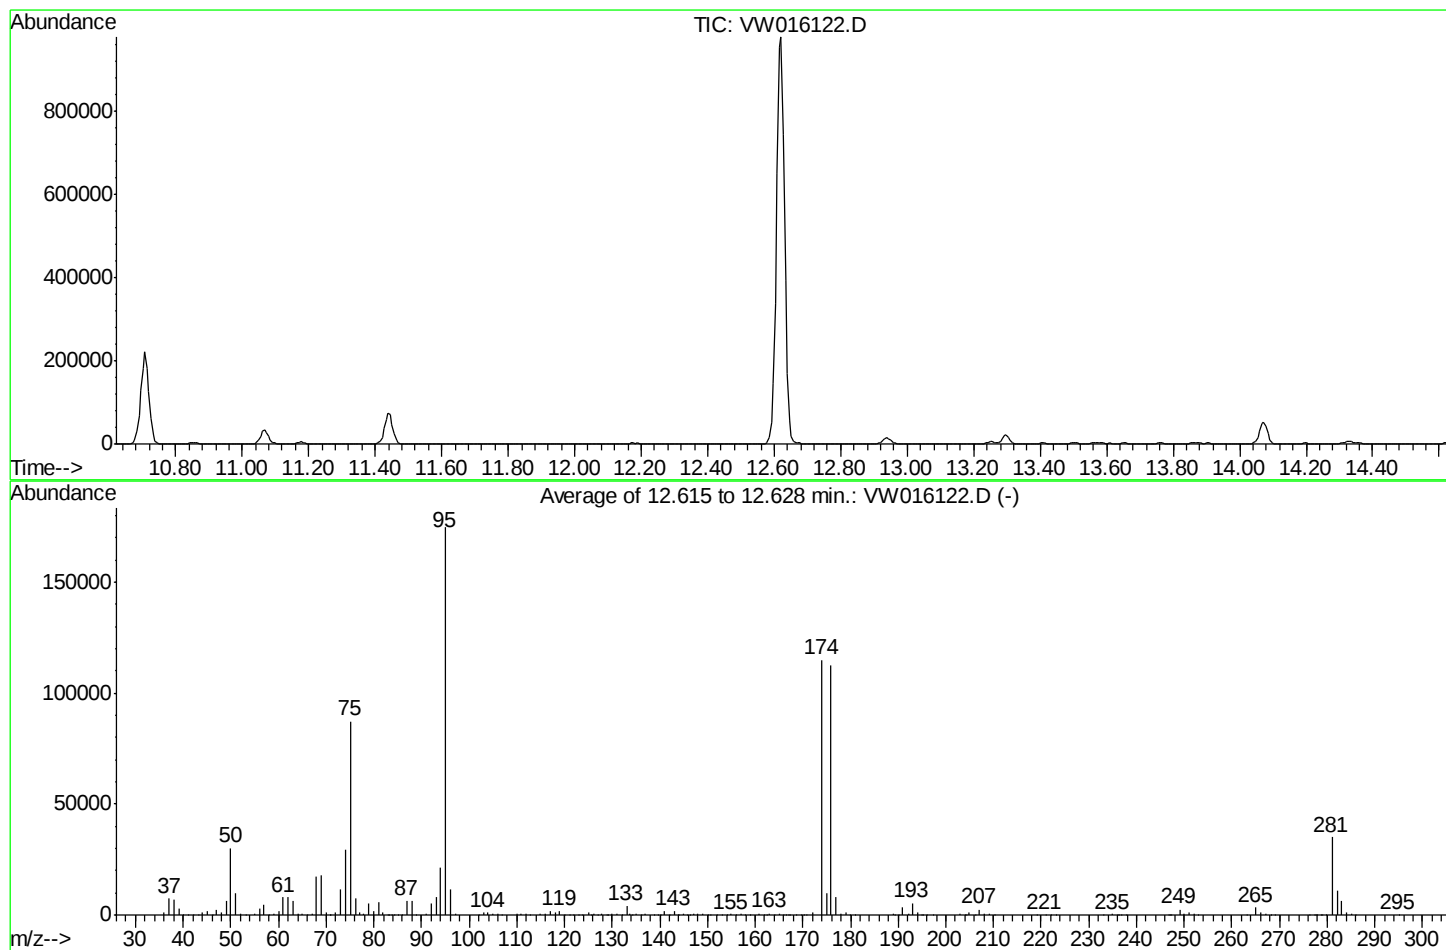

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	30234	PASS
75	95	30	80	50.0	87354	PASS
95	95	100	100	100.0	174677	PASS
96	95	5	9	6.5	11358	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	65.8	114882	PASS
175	174	5	9	8.4	9642	PASS
176	174	95	101	97.7	112226	PASS
177	176	5	9	7.3	8223	PASS