


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW081120\
 Data File : VW016122.D
 Acq On : 11 Aug 2020 07:07
 Operator : SY/VA
 Sample : BFB07
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB07

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
 Title : VOC Analysis
 Last Update : Thu Aug 13 01:23:48 2020

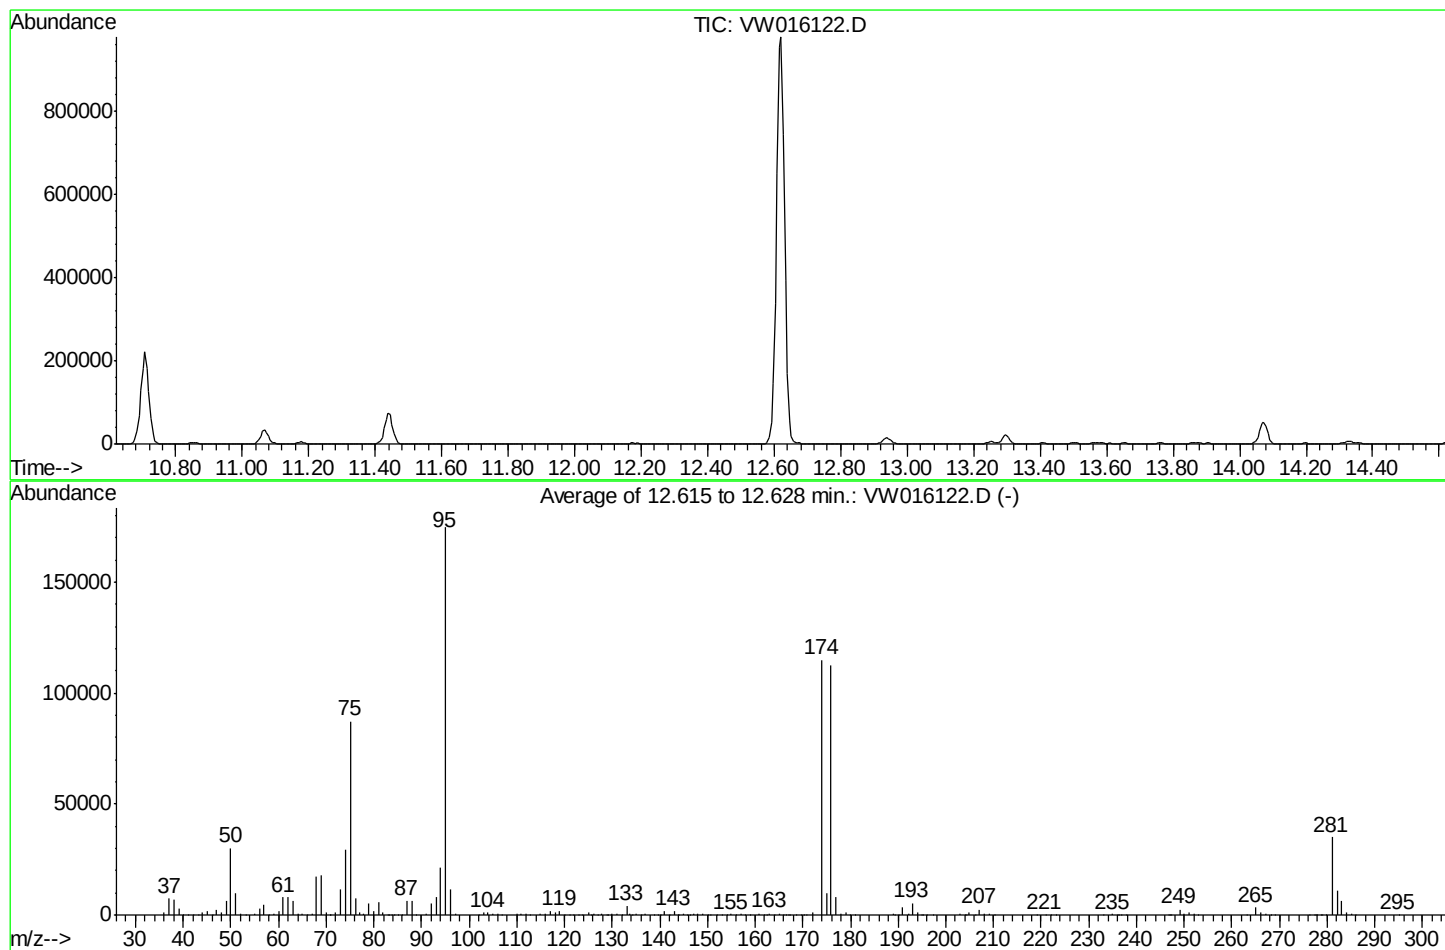

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	30234	PASS
75	95	30	80	50.0	87354	PASS
95	95	100	100	100.0	174677	PASS
96	95	5	9	6.5	11358	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	65.8	114882	PASS
175	174	5	9	8.4	9642	PASS
176	174	95	101	97.7	112226	PASS
177	176	5	9	7.3	8223	PASS

m/z	Abundance
36.00	1397.0
37.00	8399.0
38.10	7500.0
39.10	3097.0
40.00	228.0
43.10	285.0
44.00	1345.0
45.00	2485.0
46.20	210.0
47.00	2388.0
48.00	1185.0
49.00	7221.0
50.00	32928.0
51.00	10776.0
52.00	470.0
53.00	107.0
55.00	462.0
56.00	2698.0
57.00	4947.0
58.10	241.0
59.10	1110.0
60.10	1852.0
61.00	9066.0
62.00	8530.0
63.10	6808.0
64.00	979.0
65.00	863.0
66.00	158.0
67.10	440.0
68.00	18632.0
69.00	18760.0
70.00	1375.0
70.80	131.0
72.00	1175.0
73.00	14751.0
74.00	30984.0
75.00	92152.0
76.10	8525.0
76.90	1197.0
77.90	627.0
78.90	5496.0
80.00	1602.0
80.90	6144.0
81.90	1335.0
82.90	210.0
83.80	215.0
85.10	165.0
86.00	337.0
86.90	6783.0
87.90	6027.0
88.80	454.0
91.00	743.0
92.00	4845.0
93.00	7725.0
94.10	21912.0
95.00	178368.0
96.00	12431.0
97.10	501.0
102.00	123.0
103.10	1498.0
104.00	1348.0
105.00	594.0
106.00	665.0
107.00	265.0
110.00	421.0
111.00	692.0
112.00	563.0
112.80	236.0
114.90	737.0
116.00	747.0
117.00	1646.0
118.00	1539.0
118.90	2502.0
119.90	160.0
121.00	332.0
121.90	142.0
123.00	64.0
123.80	69.0
125.00	2055.0
126.00	590.0
127.00	88.0
127.80	639.0
128.80	222.0
129.10	234.0
129.90	611.0
131.00	414.0
132.00	263.0
133.10	6885.0
135.00	914.0
135.90	124.0
136.90	247.0
139.00	62.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

141.00	1747.0
142.00	332.0
143.00	1848.0
143.80	303.0
145.00	415.0
146.20	266.0
147.00	742.0
148.00	513.0
149.00	375.0
149.90	258.0
150.70	121.0
151.90	161.0
153.00	164.0
154.10	80.0
155.00	264.0
155.90	92.0
157.00	341.0
157.90	65.0
158.80	395.0
160.90	689.0
161.80	158.0
162.90	1196.0
164.00	295.0
165.10	898.0
165.80	148.0
166.30	90.0
166.90	131.0
168.80	106.0
170.20	139.0
170.70	164.0
172.10	1368.0
174.00	103976.0
175.00	8977.0
176.00	105232.0
177.00	8746.0
178.00	649.0
179.10	1530.0
180.00	271.0
181.10	338.0
189.00	760.0
191.00	5743.0
192.10	1197.0
193.00	9164.0
194.00	1353.0
194.90	899.0
195.90	192.0
197.20	75.0
203.00	576.0
204.20	114.0
205.00	1370.0
206.10	403.0
207.00	3501.0
208.10	765.0
209.00	526.0
210.10	111.0
219.10	52.0
220.90	214.0
221.90	89.0
223.10	92.0
233.00	60.0
235.00	644.0
236.00	153.0
236.90	72.0
237.80	74.0
247.10	210.0
249.10	3547.0
250.10	1053.0
251.10	1574.0
252.10	479.0
252.90	207.0
263.10	90.0
265.00	4997.0
266.10	1592.0
267.00	1085.0
268.10	287.0
269.00	137.0
276.30	133.0
277.50	166.0
278.00	175.0
279.00	582.0
281.10	51384.0
282.10	14496.0
283.00	9123.0
284.10	1501.0
285.00	690.0
286.00	119.0
295.00	88.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

m/z	Abundance
36.00	1165.0
37.00	8041.0
38.00	7615.0
39.10	3463.0
40.00	283.0
43.00	283.0
44.00	1281.0
45.10	2042.0
46.00	197.0
47.00	2176.0
48.00	1242.0
49.00	7288.0
50.00	33968.0
51.00	10586.0
52.00	392.0
55.00	493.0
56.00	3330.0
57.00	4912.0
58.10	250.0
59.00	594.0
60.00	1573.0
61.00	8415.0
62.10	9026.0
63.10	6340.0
64.00	800.0
65.00	646.0
65.90	138.0
66.90	676.0
68.00	18864.0
69.00	19648.0
70.00	1305.0
71.00	178.0
72.10	1210.0
73.00	11703.0
74.10	32616.0
75.00	98288.0
76.10	8161.0
77.00	1115.0
78.00	740.0
78.90	5845.0
79.90	1854.0
81.00	5963.0
82.00	1178.0
83.10	196.0
85.10	133.0
86.00	157.0
87.00	7620.0
87.90	7710.0
90.90	633.0
92.00	6111.0
93.00	8894.0
94.00	23168.0
95.00	195648.0
96.10	12130.0
97.10	376.0
102.90	920.0
103.90	1081.0
105.00	428.0
105.90	778.0
107.00	282.0
109.90	351.0
110.90	362.0
112.10	347.0
112.80	189.0
114.90	461.0
116.00	760.0
116.90	1621.0
118.00	1076.0
119.00	1702.0
119.90	218.0
120.90	140.0
122.00	58.0
122.90	68.0
123.90	227.0
125.00	1353.0
125.70	574.0
126.10	569.0
127.00	108.0
127.90	663.0
128.90	238.0
129.90	548.0
131.00	468.0
133.00	4223.0
133.80	956.0
134.90	612.0
136.00	74.0
137.00	385.0
138.80	67.0
140.00	150.0
141.00	1943.0
142.90	2106.0
144.00	155.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

144.90	358.0
145.80	356.0
147.00	669.0
147.90	648.0
149.00	392.0
150.00	241.0
151.90	162.0
153.00	116.0
154.10	145.0
155.00	462.0
156.00	138.0
157.00	413.0
158.00	80.0
158.90	297.0
160.90	532.0
162.30	190.0
163.00	879.0
164.10	146.0
165.00	783.0
165.80	119.0
167.20	60.0
168.60	77.0
169.60	94.0
170.20	168.0
171.90	1202.0
174.00	123952.0
175.00	10862.0
175.90	127968.0
177.00	8781.0
178.00	793.0
179.00	811.0
179.90	187.0
180.90	161.0
188.90	543.0
190.10	167.0
191.00	3424.0
192.10	667.0
193.00	5008.0
194.00	1008.0
195.10	536.0
195.90	68.0
203.00	351.0
203.90	125.0
204.90	921.0
207.10	2664.0
208.00	533.0
209.10	292.0
210.10	82.0
220.90	128.0
223.10	84.0
235.00	392.0
236.30	129.0
246.80	80.0
247.30	63.0
249.10	2525.0
250.00	740.0
251.10	1234.0
252.10	424.0
252.90	114.0
263.10	103.0
265.10	2921.0
266.10	812.0
267.10	959.0
268.10	203.0
277.20	138.0
277.60	110.0
281.00	33320.0
282.00	11973.0
283.10	6964.0
284.00	1217.0
285.00	380.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

m/z	Abundance
36.00	1102.0
37.10	5678.0
38.10	5374.0
39.00	2005.0
39.90	216.0
41.10	67.0
42.10	55.0
43.10	90.0
44.00	949.0
45.00	1336.0
46.10	171.0
47.00	1682.0
48.00	898.0
49.10	5218.0
50.00	23808.0
51.00	7985.0
52.10	324.0
55.00	295.0
56.00	2300.0
57.00	3726.0
58.00	201.0
59.00	215.0
60.00	1455.0
61.00	6647.0
62.00	6222.0
63.00	5302.0
64.00	655.0
65.00	470.0
65.80	89.0
66.80	380.0
68.00	14186.0
69.00	15224.0
70.00	1034.0
70.90	104.0
71.90	785.0
73.00	8547.0
74.10	24080.0
75.00	71624.0
76.10	6527.0
77.00	809.0
78.00	570.0
79.00	4653.0
79.90	1328.0
80.90	4648.0
82.00	1026.0
83.10	133.0
84.20	99.0
85.20	96.0
85.90	169.0
87.00	5365.0
88.00	5726.0
90.90	618.0
92.00	4153.0
93.00	6953.0
94.00	18528.0
95.00	150016.0
96.00	9514.0
97.00	456.0
103.00	433.0
104.00	842.0
104.90	296.0
106.00	593.0
106.80	87.0
110.00	331.0
110.90	266.0
112.00	230.0
112.90	237.0
115.00	262.0
116.00	680.0
116.90	1140.0
118.00	657.0
119.00	1030.0
120.00	53.0
122.80	56.0
123.80	103.0
124.90	524.0
126.00	208.0
127.90	594.0
128.90	327.0
129.90	653.0
130.90	248.0
132.00	120.0
133.10	1896.0
134.30	250.0
135.00	470.0
136.10	122.0
136.90	307.0
138.80	95.0
139.70	65.0
140.10	58.0
140.90	1384.0
142.00	218.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

143.00	1762.0
145.00	312.0
145.90	208.0
146.90	437.0
147.90	334.0
148.80	265.0
149.90	188.0
151.80	73.0
152.80	82.0
154.00	124.0
154.90	233.0
155.90	80.0
157.00	222.0
157.90	62.0
158.80	208.0
161.00	292.0
162.90	477.0
164.10	100.0
165.00	335.0
168.70	97.0
170.00	109.0
171.90	787.0
174.00	116720.0
175.00	9089.0
176.00	103480.0
177.00	7143.0
178.00	401.0
178.90	538.0
180.10	53.0
180.90	137.0
189.20	227.0
191.00	1287.0
192.10	262.0
193.00	2332.0
194.00	456.0
195.10	358.0
202.90	154.0
203.90	98.0
205.10	441.0
206.00	169.0
207.00	1191.0
208.10	307.0
209.00	243.0
221.00	126.0
235.00	221.0
236.10	98.0
249.00	1312.0
250.00	344.0
251.00	597.0
252.00	130.0
265.00	1841.0
266.10	318.0
267.00	242.0
268.00	137.0
278.70	142.0
279.10	161.0
279.80	344.0
281.10	20152.0
282.10	5836.0
283.10	2745.0
284.10	770.0
285.10	195.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

Scan 1749 (12.567 min): VW016122.D
BFB07

m/z	Abundance
40.20	108.0
43.90	275.0
68.90	80.0
73.10	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07