




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081122\
 Data File : VW024225.D
 Acq On : 11 Aug 2022 10:12
 Operator : SY/VA
 Sample : VW0811SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK574

Manual IntegrationsAPPROVED

Reviewed By :Mahesh
 Dadoda
 08/12/2022
 Supervised By :Semsettin
 Yesilyurt
 08/12/2022

Quant Time: Aug 12 03:13:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 12 03:13:23 2022
 Response via : Initial Calibration

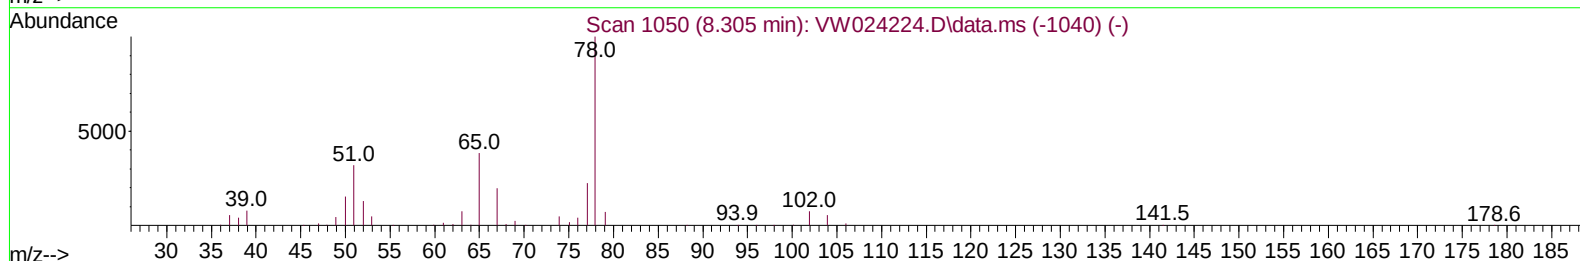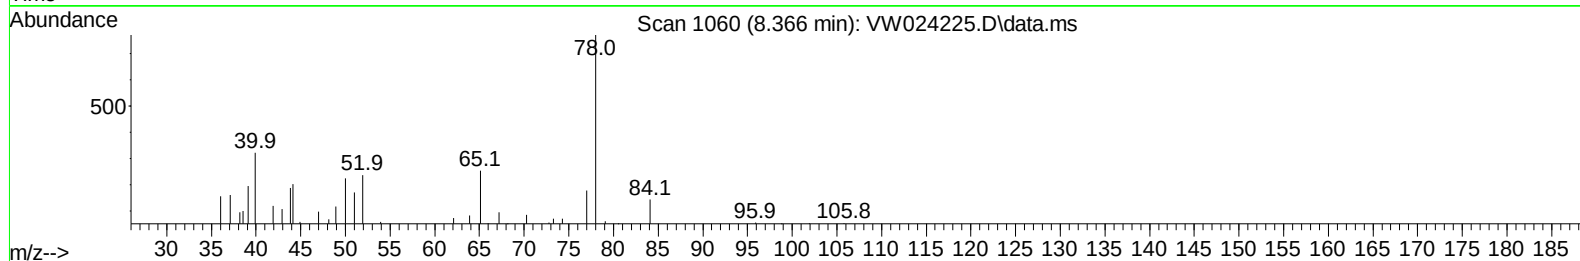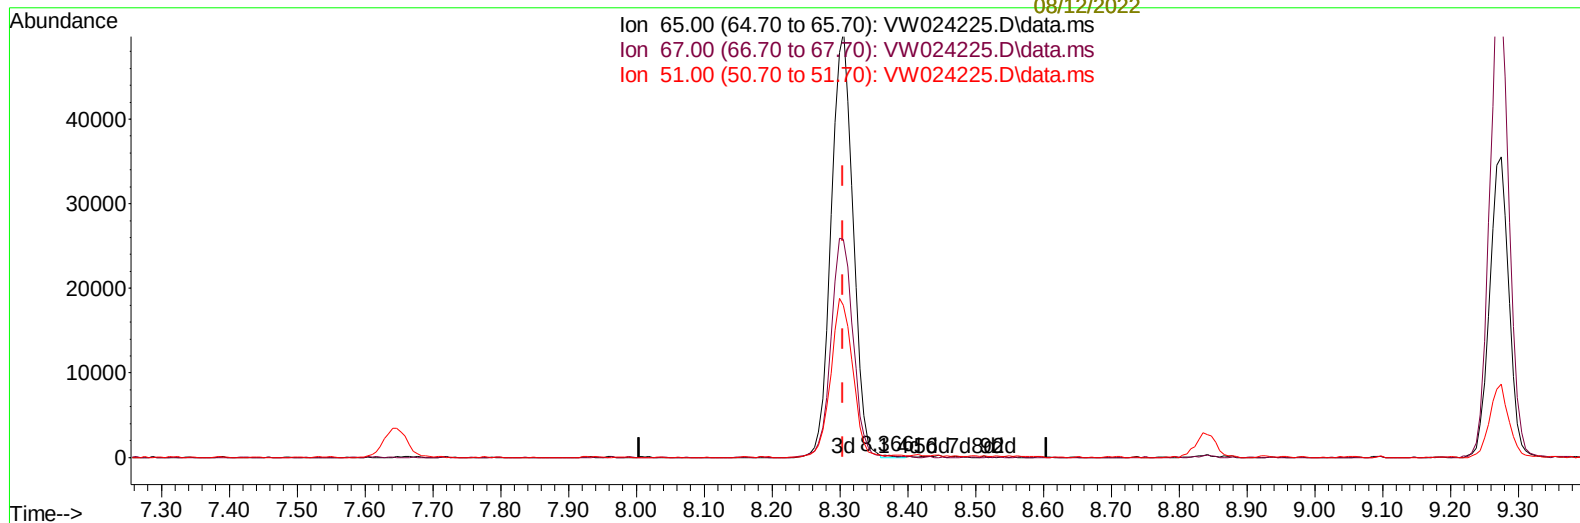

TIC: VW024225.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.366min (+ 0.061) 0.07 ug/L

response 333

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	52.85
51.00	95.20	72.97
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081122\
 Data File : VW024225.D
 Acq On : 11 Aug 2022 10:12
 Operator : SY/VA
 Sample : VW0811SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK574

Manual IntegrationsAPPROVED

Reviewed By :Mahesh
 Dadoda
 08/12/2022
 Supervised By :Semsettin
 Yesilyurt
 08/12/2022

Quant Time: Aug 12 03:13:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 12 03:13:23 2022
 Response via : Initial Calibration

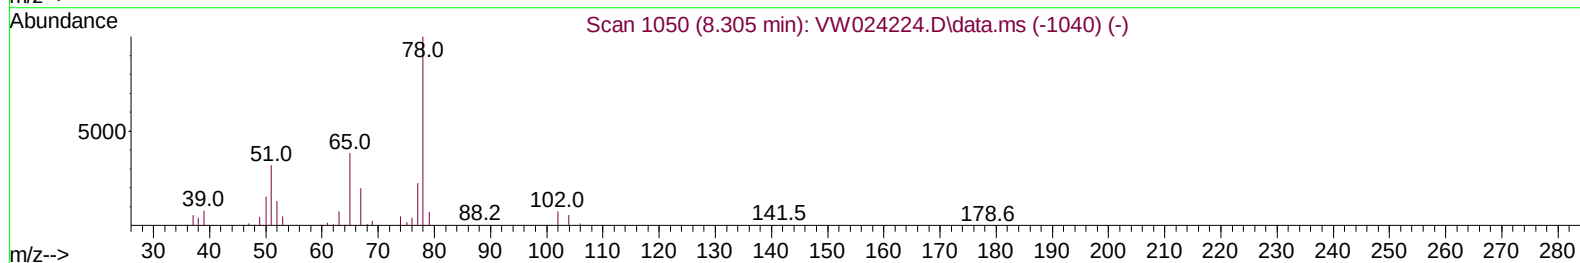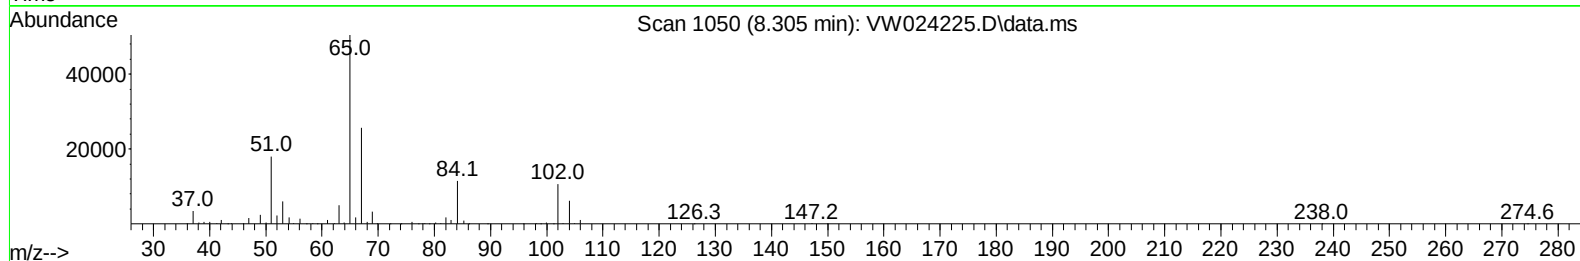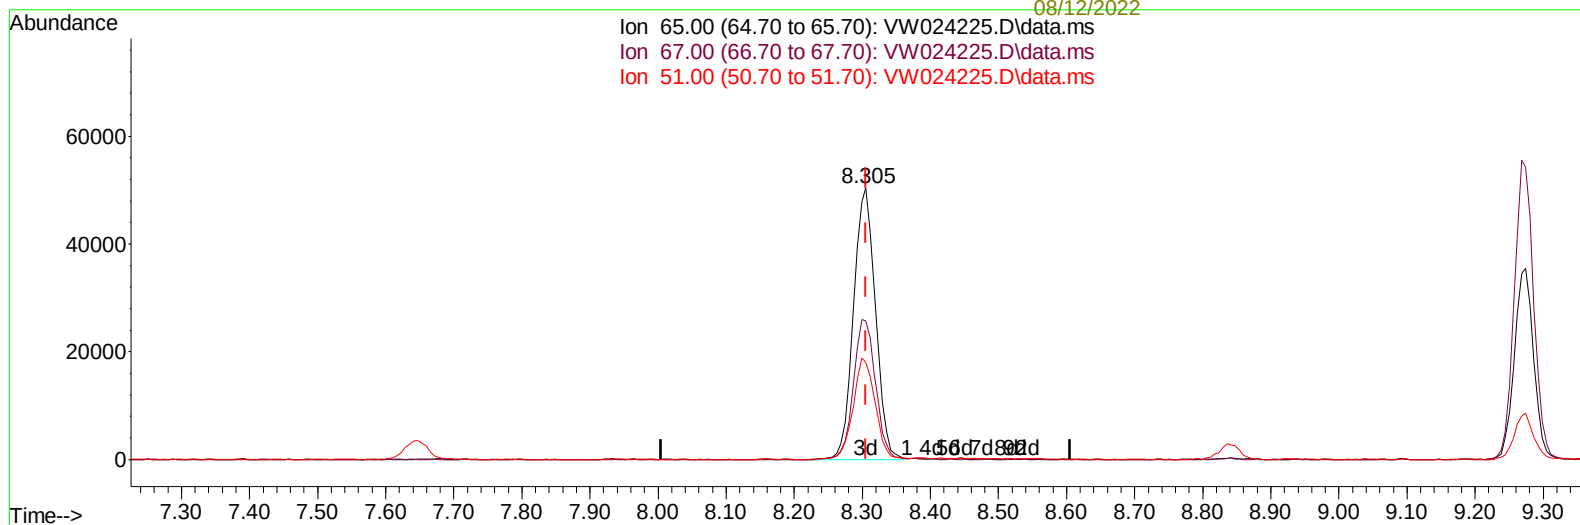

TIC: VW024225.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 23.32 ug/L m

response 112300

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	0.16#
51.00	95.20	0.22#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081122\
 Data File : VW024225.D
 Acq On : 11 Aug 2022 10:12
 Operator : SY/VA
 Sample : VW0811SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK574

Manual IntegrationsAPPROVED

Quant Time: Aug 12 03:13:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 12 03:13:23 2022
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda
 08/12/2022
 Supervised By :Semsettin
 Yesilyurt
 08/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	286652	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	288561	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	135832	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	123116	20.548	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	82.200%	
7) Chloroethane-d5	2.873	69	74166	19.870	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	79.480%	
11) 1,1-Dichloroethene-d2	4.001	63	93267	13.658	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	54.640%	
21) 2-Butanone-d5	7.074	46	58127	52.144	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	104.280%	
24) Chloroform-d	7.647	84	197418	22.761	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.040%	
26) 1,2-Dichloroethane-d4	8.305	65	112300m	23.321	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	93.280%	
32) Benzene-d6	8.269	84	351587	20.659	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	82.640%	
36) 1,2-Dichloropropane-d6	9.268	67	110214	21.935	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	87.720%	
41) Toluene-d8	10.323	98	321019	20.181	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	80.720%	
43) trans-1,3-Dichloroprop...	10.573	79	47241	21.465	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	85.880%	
47) 2-Hexanone-d5	10.927	63	47084	50.732	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	101.460%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	115473	23.687	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	94.760%	
66) 1,2-Dichlorobenzene-d4	13.853	152	128425	25.837	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	103.360%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081122\
Data File : VW024225.D
Acq On : 11 Aug 2022 10:12
Operator : SY/VA
Sample : VW0811SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK574

Manual IntegrationsAPPROVED

Reviewed By :Mahesh

Dadoda

08/12/2022

Supervised By :Semsettin

Yesilyurt

08/12/2022

Quant Time: Aug 12 03:13:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 12 03:13:23 2022
Response via : Initial Calibration

