

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081123\
 Data File : VW026716.D
 Acq On : 11 Aug 2023 17:35
 Operator : SY/MD
 Sample : 03967-21
 Misc : 5.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A48M9

Quant Time: Aug 12 00:45:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 12 00:39:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	674794	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	562819	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	175211	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	223251	20.126	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.520%
7) Chloroethane-d5	2.893	69	175256	21.247	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.000%
11) 1,1-Dichloroethene-d2	4.027	65	109398	20.052	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.200%
21) 2-Butanone-d5	7.075	46	161863	50.768	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.540%
24) Chloroform-d	7.648	84	515679	22.769	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.080%
26) 1,2-Dichloroethane-d4	8.307	65	321522	25.725	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.920%
32) Benzene-d6	8.276	84	1039097	26.788	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.160%
36) 1,2-Dichloropropane-d6	9.276	67	342419	28.340	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	113.360%
41) Toluene-d8	10.325	98	840101	25.231	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.920%
43) trans-1,3-Dichloroprop...	10.575	79	127799	25.618	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	102.480%
47) 2-Hexanone-d5	10.922	63	74307	58.529	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.060%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	265617	27.837	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	111.360%
66) 1,2-Dichlorobenzene-d4	13.854	152	157983	25.192	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.760%
Target Compounds					Qvalue	
13) Acetone	4.124	43	18896	5.961	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081123\
Data File : VW026716.D
Acq On : 11 Aug 2023 17:35
Operator : SY/MD
Sample : 03967-21
Misc : 5.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A48M9

Quant Time: Aug 12 00:45:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 12 00:39:51 2023
Response via : Initial Calibration

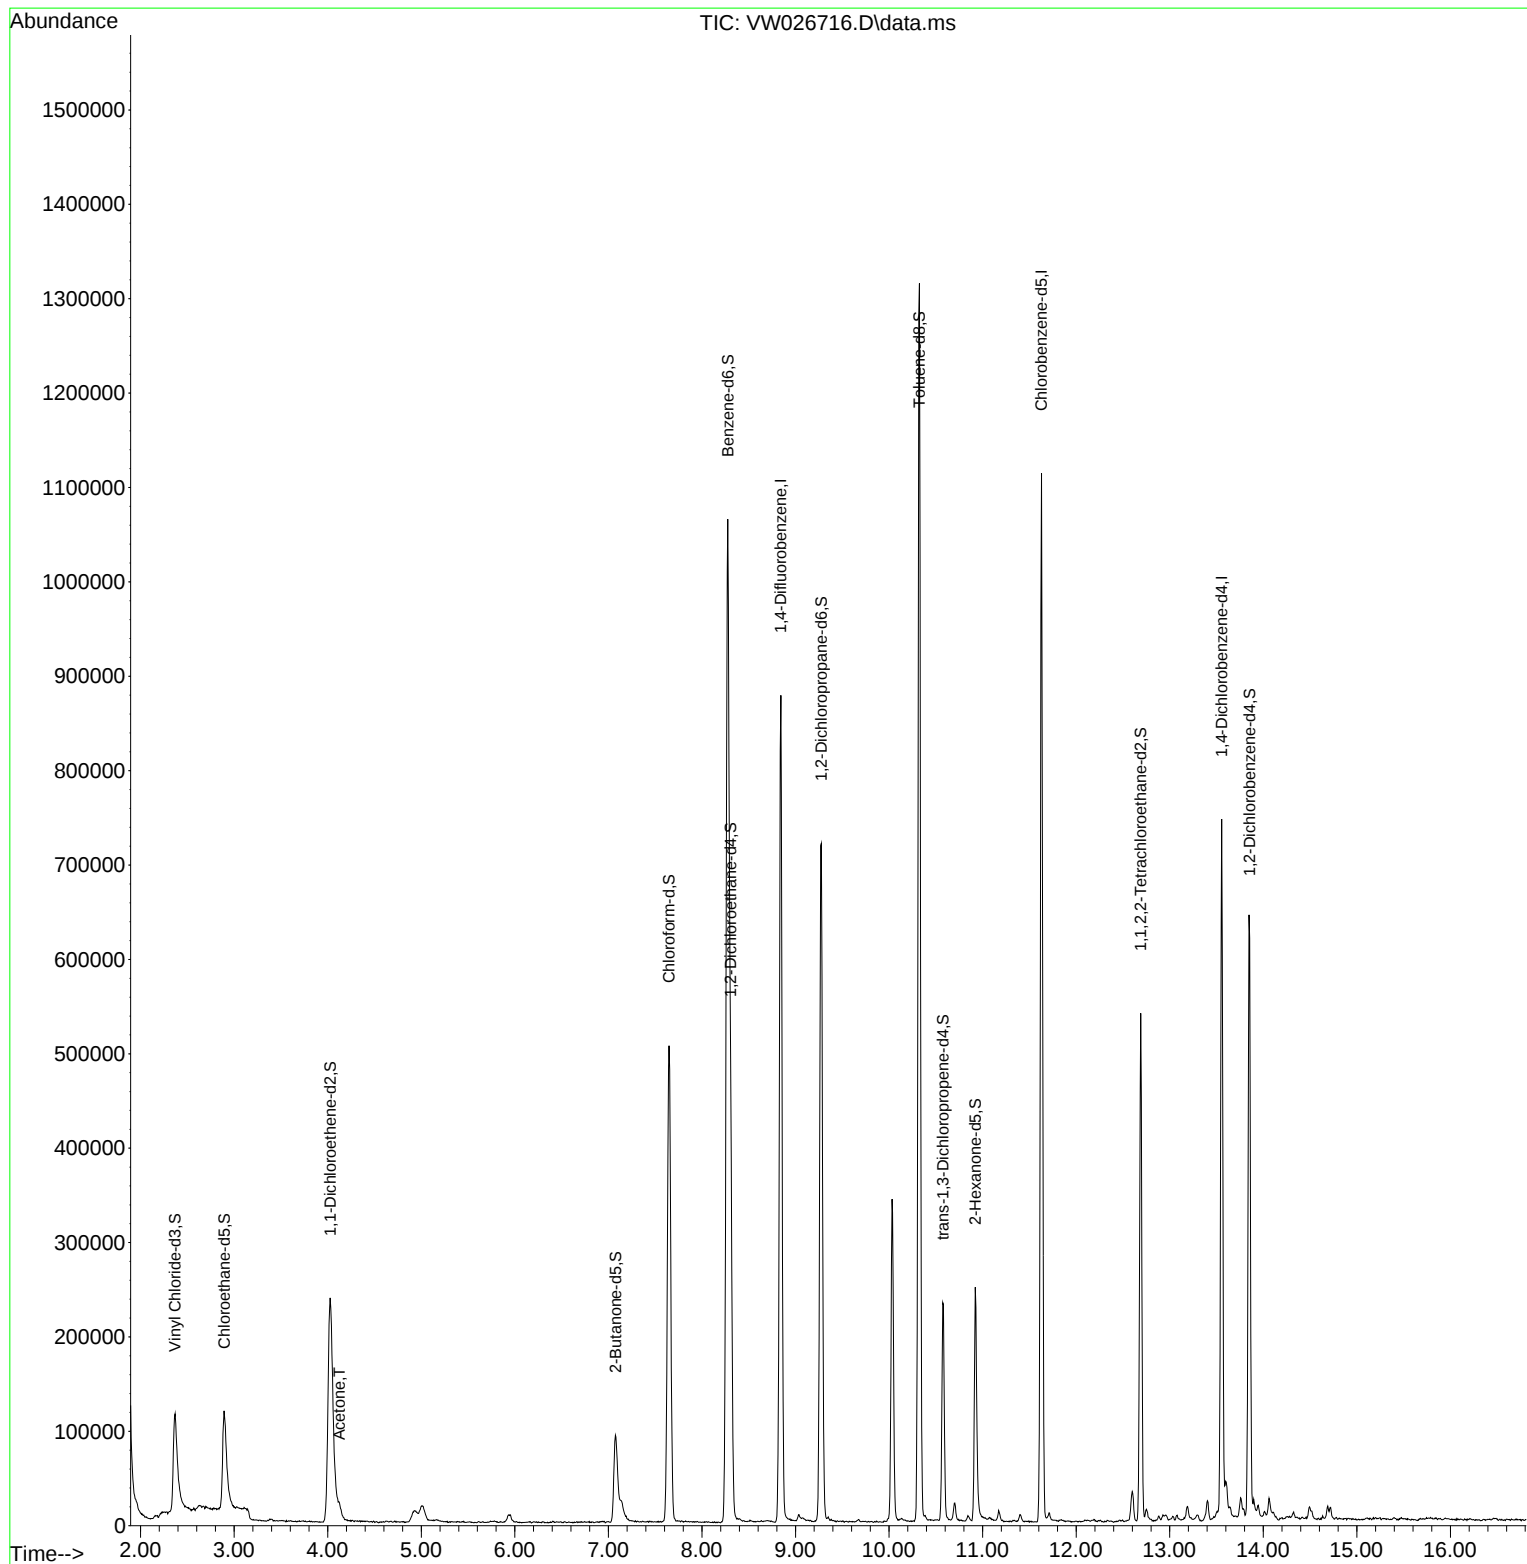

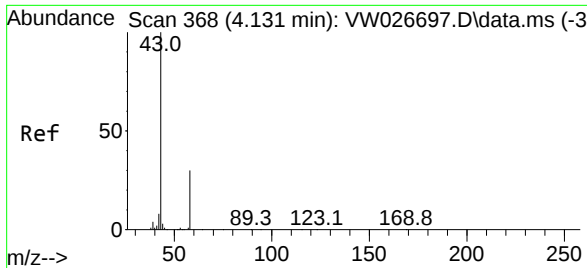

#13
 Acetone
 Concen: 5.961 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW026716.D
 Acq: 11 Aug 2023 17:35

Instrument :
 MSVOA_W
 ClientSampleId :
 A48M9

Tgt Ion: 43 Resp: 18896
 Ion Ratio Lower Upper
 43 100
 58 33.2 0.0 57.4

