

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081123\
 Data File : VW026718.D
 Acq On : 11 Aug 2023 18:23
 Operator : SY/MD
 Sample : 03967-23
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A48N4

Quant Time: Aug 12 00:46:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 12 00:39:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	784520	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	677823	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	237893	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	228120	17.688	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.760%
7) Chloroethane-d5	2.893	69	170455	17.774	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.080%
11) 1,1-Dichloroethene-d2	4.033	65	119832	18.892	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.560%
21) 2-Butanone-d5	7.081	46	128690	34.718	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.440%
24) Chloroform-d	7.648	84	586349	22.269	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.080%
26) 1,2-Dichloroethane-d4	8.307	65	335746	23.106	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.440%
32) Benzene-d6	8.276	84	1149914	24.615	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.480%
36) 1,2-Dichloropropane-d6	9.270	67	381945	26.248	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.000%
41) Toluene-d8	10.325	98	966010	24.090	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.360%
43) trans-1,3-Dichloroprop...	10.575	79	102701	17.094	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	68.360%
47) 2-Hexanone-d5	10.922	63	38387	25.106	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	50.220%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	272501	23.713	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.840%
66) 1,2-Dichlorobenzene-d4	13.848	152	215204	25.274	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.080%
Target Compounds					Qvalue	
13) Acetone	4.125	43	11185	3.035	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081123\
Data File : VW026718.D
Acq On : 11 Aug 2023 18:23
Operator : SY/MD
Sample : 03967-23
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A48N4

Quant Time: Aug 12 00:46:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 12 00:39:51 2023
Response via : Initial Calibration

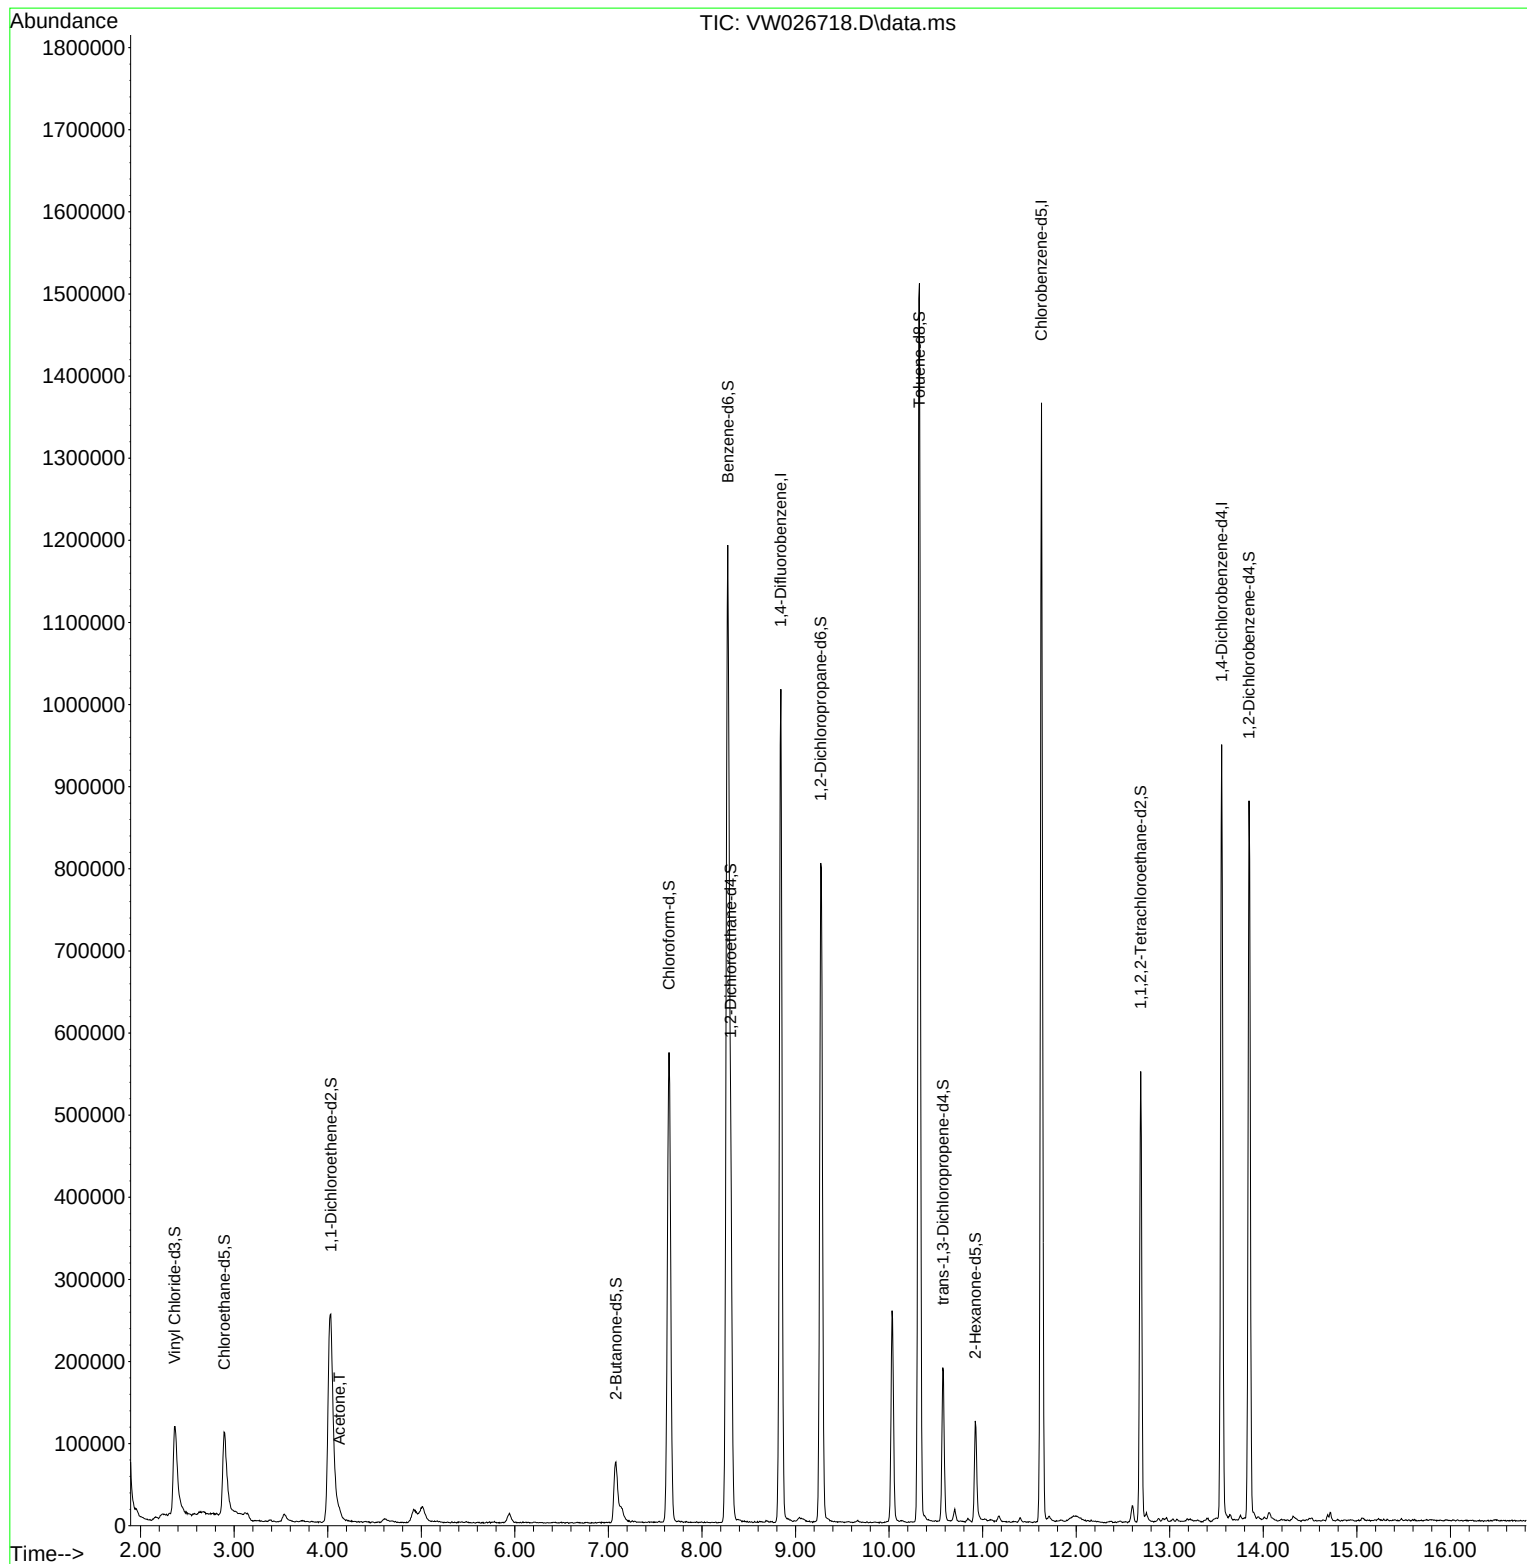

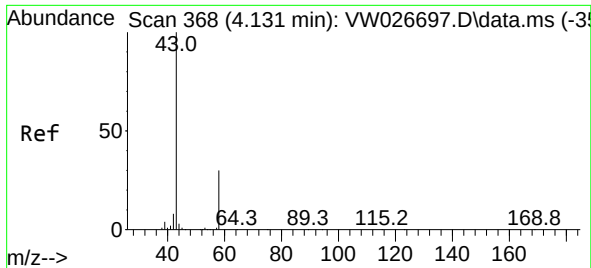

#13
 Acetone
 Concen: 3.035 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW026718.D
 Acq: 11 Aug 2023 18:23

Instrument :
 MSVOA_W
 ClientSampleId :
 A48N4

Tgt Ion: 43 Resp: 11185
 Ion Ratio Lower Upper
 43 100
 58 29.4 0.0 57.4

