




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081123\
 Data File : VW026714.D
 Acq On : 11 Aug 2023 16:47
 Operator : SY/MD
 Sample : 03967-19
 Misc : 5.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A48M5

Manual IntegrationsAPPROVED

Quant Time: Aug 12 00:45:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 12 00:39:51 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2023
 Supervised By :Mahesh Dadoda 08/15/2023

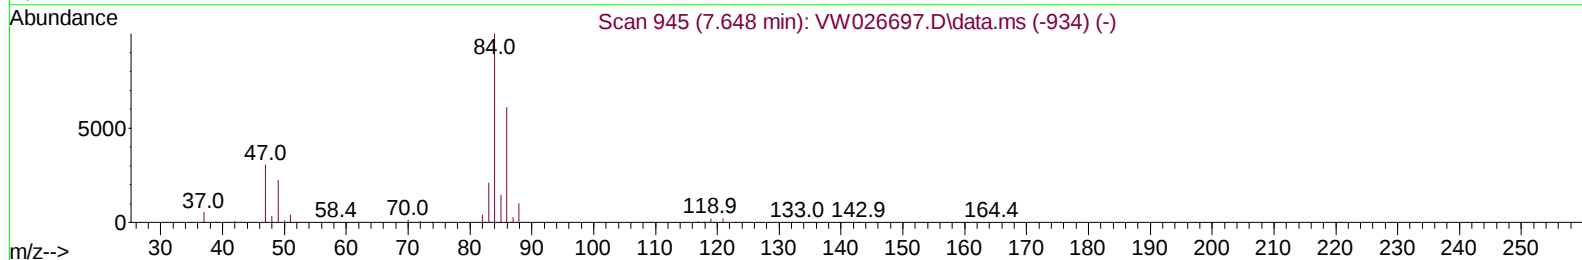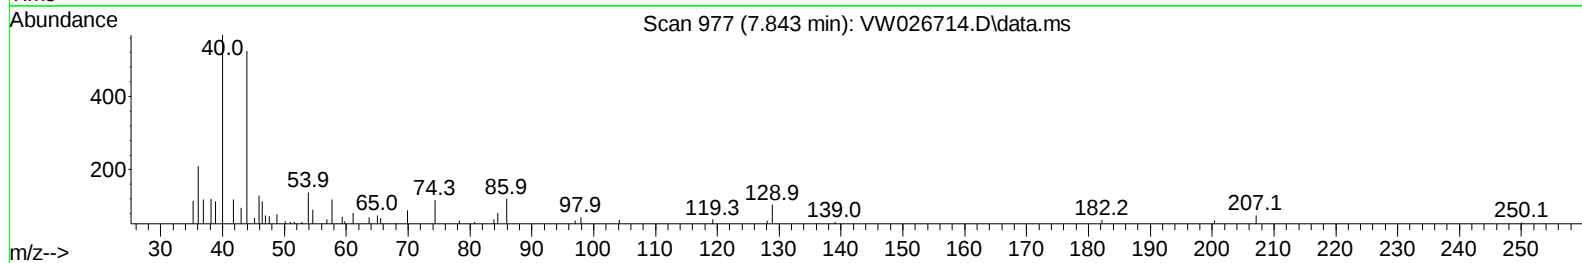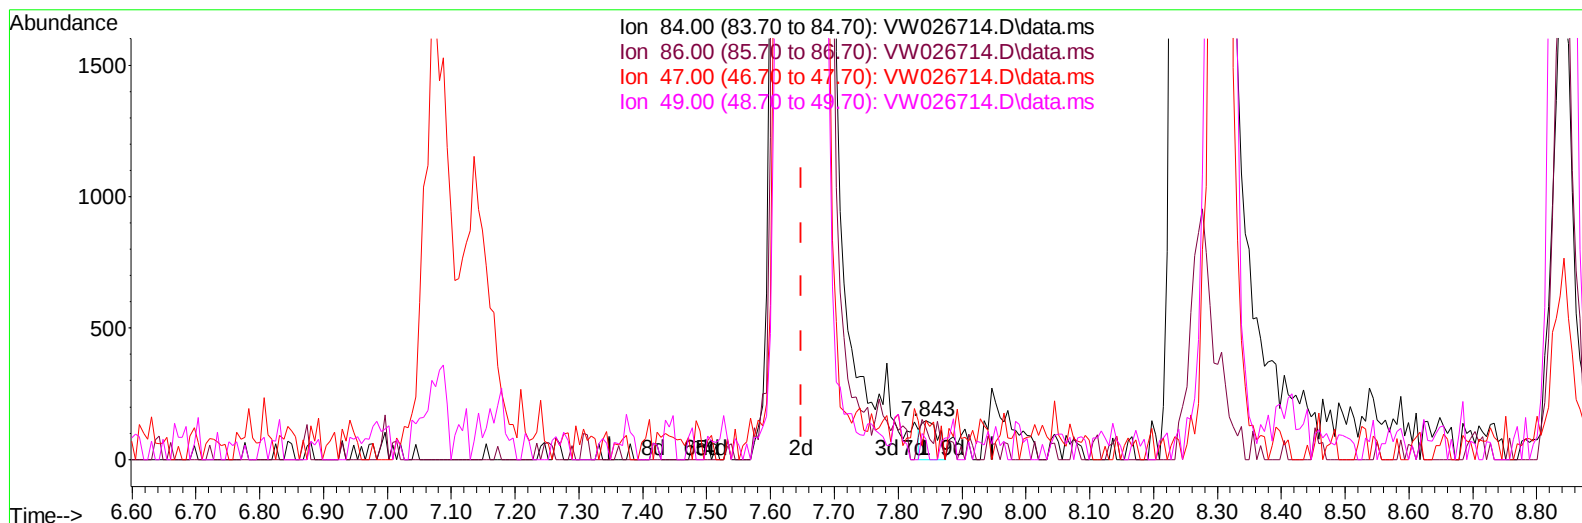

TIC: VW026714.D\data.ms

(24) Chloroform-d (S)

7.843min (+ 0.195) 0.01 ug/L

response 271

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	66.79
47.00	49.30	56.09
49.00	28.20	23.99




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081123\
 Data File : VW026714.D
 Acq On : 11 Aug 2023 16:47
 Operator : SY/MD
 Sample : 03967-19
 Misc : 5.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A48M5

Manual IntegrationsAPPROVED

Quant Time: Aug 12 00:45:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 12 00:39:51 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2023
 Supervised By :Mahesh Dadoda 08/15/2023

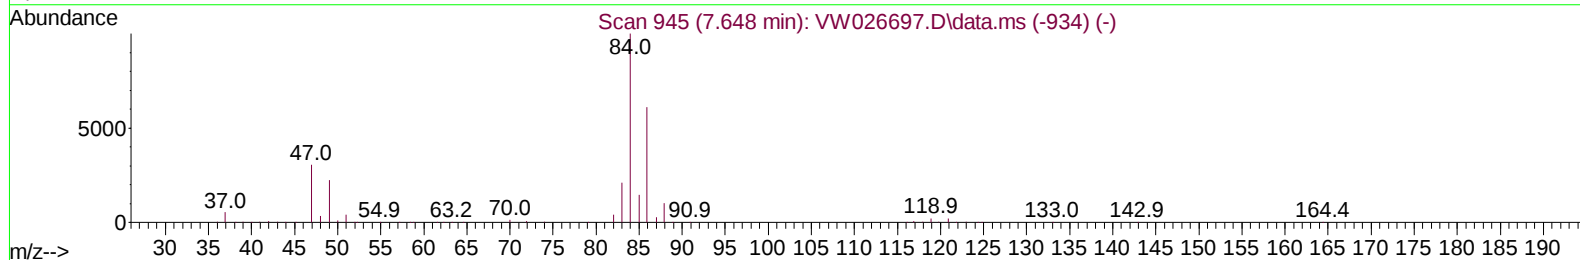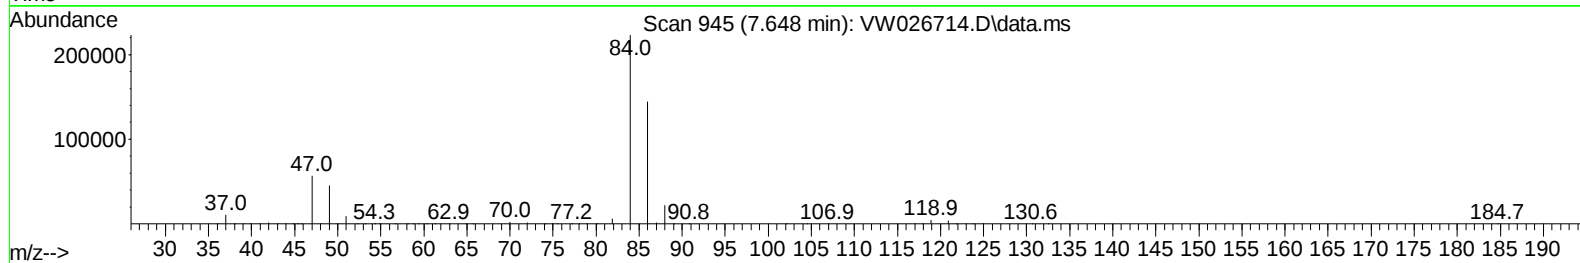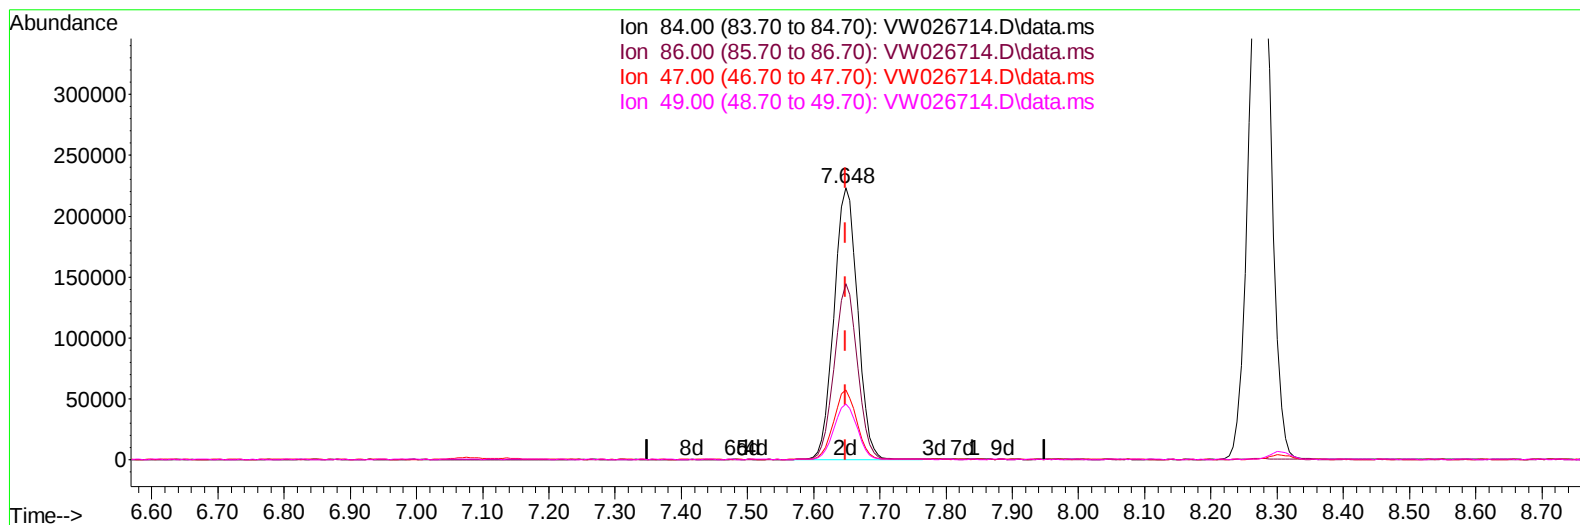

TIC: VW026714.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 21.21 ug/L m

response 550664

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	0.03#
47.00	49.30	0.03#
49.00	28.20	0.01#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081123\
 Data File : VW026714.D
 Acq On : 11 Aug 2023 16:47
 Operator : SY/MD
 Sample : 03967-19
 Misc : 5.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A48M5

Manual IntegrationsAPPROVED

Quant Time: Aug 12 00:45:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 12 00:39:51 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2023
 Supervised By :Mahesh Dadoda 08/15/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		773475	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		609260	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		180488	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		239776	18.858	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	75.440%	
7) Chloroethane-d5	2.899	69		185581	19.628	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	78.520%	
11) 1,1-Dichloroethene-d2	4.027	65		117641	18.812	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	75.240%	
21) 2-Butanone-d5	7.075	46		185325	50.711	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	101.420%	
24) Chloroform-d	7.648	84		550664m	21.212	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	84.840%	
26) 1,2-Dichloroethane-d4	8.307	65		335403	23.412	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	93.640%	
32) Benzene-d6	8.276	84		1117332	26.610	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	106.440%	
36) 1,2-Dichloropropane-d6	9.276	67		358293	27.394	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	109.560%	
41) Toluene-d8	10.325	98		905216	25.114	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	100.440%	
43) trans-1,3-Dichloroprop...	10.575	79		134809	24.963	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	99.840%	
47) 2-Hexanone-d5	10.922	63		88097	64.101	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	128.200%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		236198	22.867	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	91.480%	
66) 1,2-Dichlorobenzene-d4	13.848	152		135836	21.027	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	84.120%	
Target Compounds							
						Qvalue	
13) Acetone	4.118	43		105985	29.167	ug/L	97
22) 2-Butanone	7.173	43		42490	7.935	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081123\
Data File : VW026714.D
Acq On : 11 Aug 2023 16:47
Operator : SY/MD
Sample : 03967-19
Misc : 5.30g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A48M5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2023
Supervised By :Mahesh Dadoda 08/15/2023

Quant Time: Aug 12 00:45:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 12 00:39:51 2023
Response via : Initial Calibration

