

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081219\
 Data File : VW011831.D
 Acq On : 10 Aug 2019 00:17
 Operator : SY/VA
 Sample : K4227-18
 Misc : 5.37G/5ML/MSVOA W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 1S-O-(1)

Quant Time: Aug 11 02:02:44 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 27 00:23:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	205584	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	341365	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	286260	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	112990	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	138387	58.62	ug/l	0.00
Spiked Amount 50.000			Recovery	=	117.24%	
35) Dibromofluoromethane	7.88	113	107908	56.35	ug/l	0.00
Spiked Amount 50.000			Recovery	=	112.70%	
50) Toluene-d8	10.32	98	419545	53.51	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.02%	
62) 4-Bromofluorobenzene	12.62	95	132593	47.43	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.86%	
Target Compounds						
16) Acetone	4.14	43	33956	45.219	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW081219\
Data File : VW011831.D
Acq On : 10 Aug 2019 00:17
Operator : SY/VA
Sample : K4227-18
Misc : 5.37G/5ML/MSVOA W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
1S-O-(1)

Quant Time: Aug 11 02:02:44 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 27 00:23:30 2019
Response via : Initial Calibration

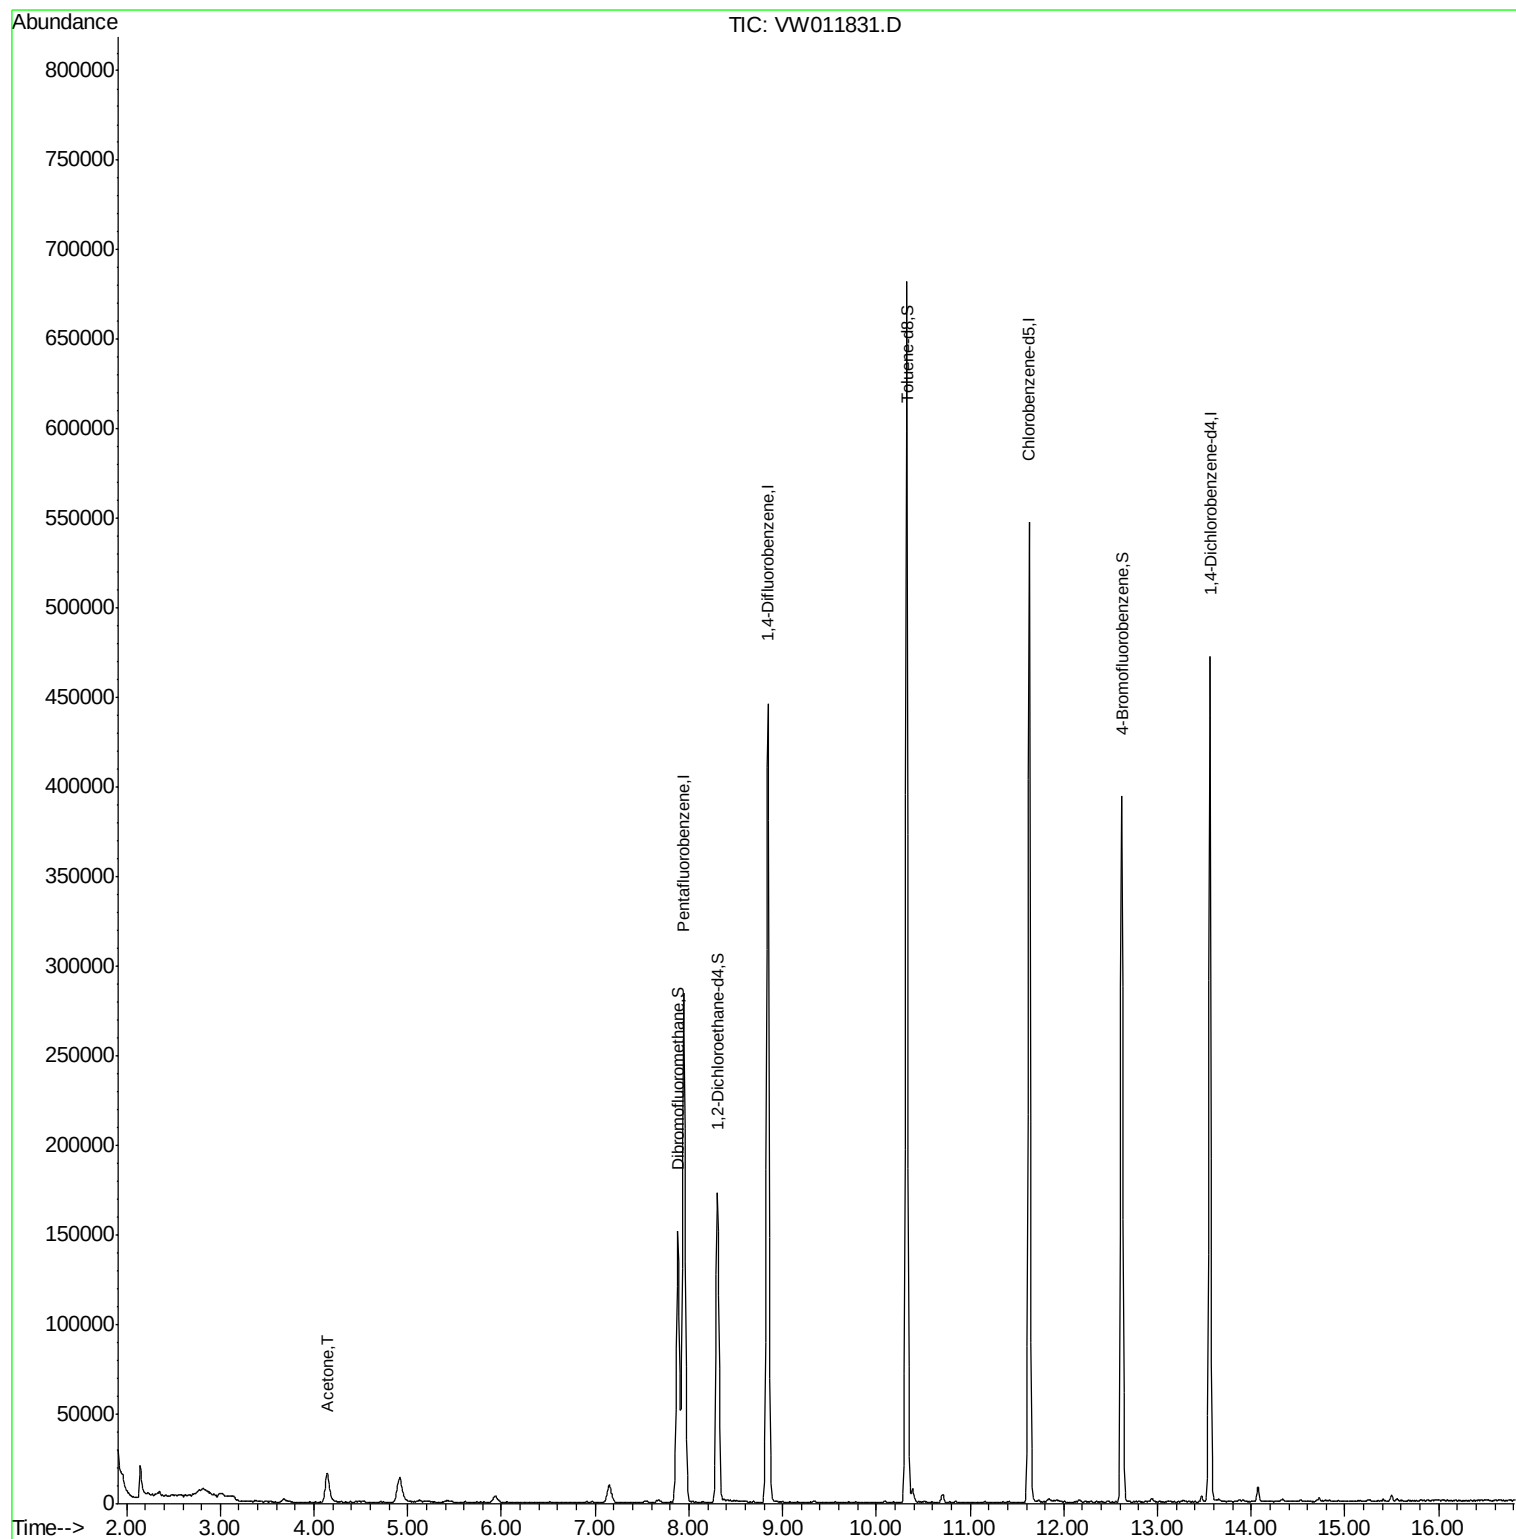

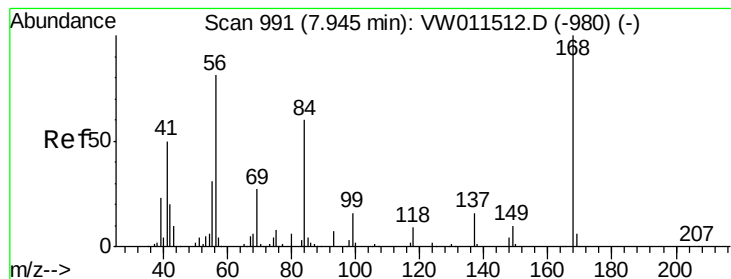

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW011831.D

Acq: 10 Aug 2019 00:17

Instrument :

MSVOA_W

ClientSampled :


1S-O-(1)

Tot Ion:168 Resp: 205584

Ion Ratio Lower Upper

168 100

99 61.0 48.2 72.4

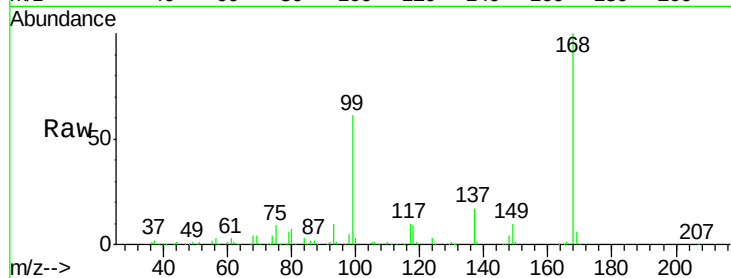

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00

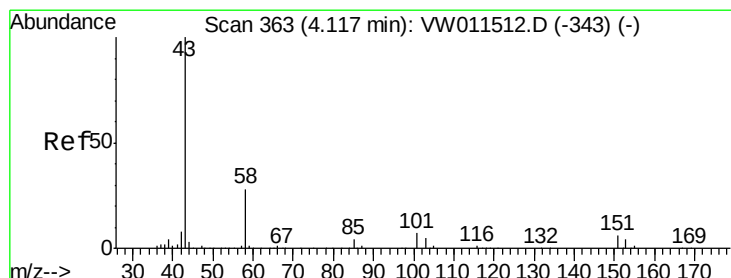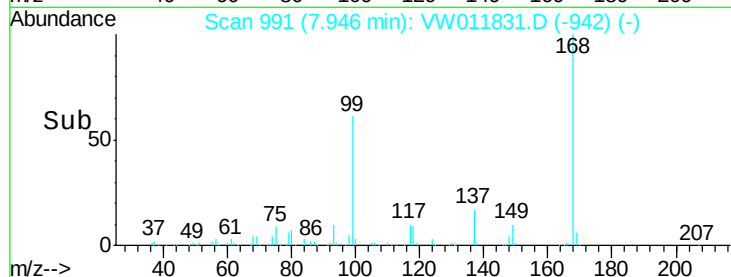

#16

Acetone

Concen: 45.219 ug/l

RT: 4.14 min Scan# 367

Delta R.T. 0.02 min

Lab File: VW011831.D


Acq: 10 Aug 2019 00:17

Tgt Ion: 43 Resp: 33956

Ion Ratio Lower Upper

43 100

58 28.5 22.3 33.5

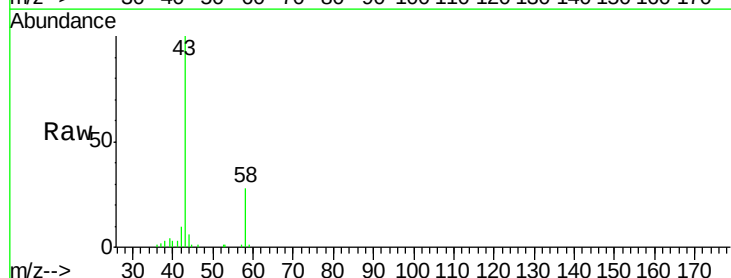

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

12000

10000

8000


6000


4000

2000

0

Time--> 4.00 4.10 4.20 4.30




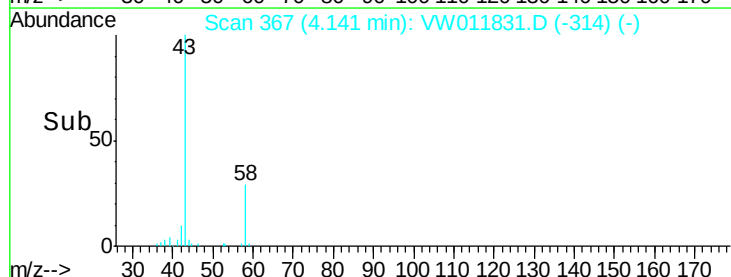


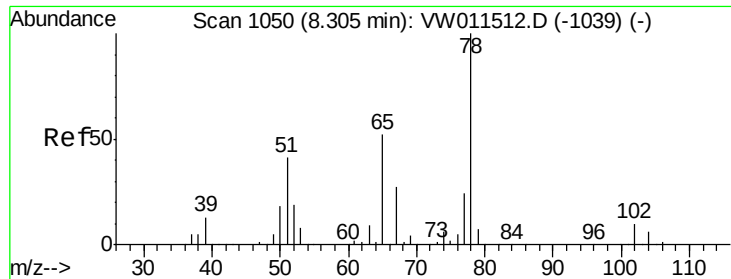

#33
 1,2-Dichloroethane-d4
 Concen: 58.622 ug/l
 RT: 8.31 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: VW011831.D
 Acq: 10 Aug 2019 00:17




Instrument :
 MSVOA_W
 ClientSampleId :
 1S-O-(1)


Tot Ion: 65 Resp: 138387
 Ion Ratio Lower Upper
 65 100
 67 51.2 0.0 105.2

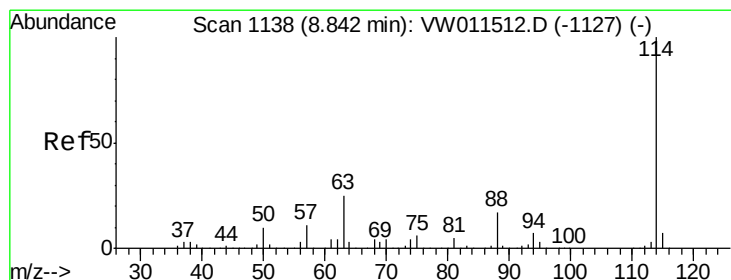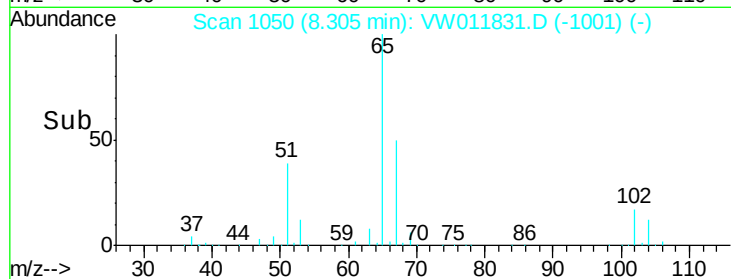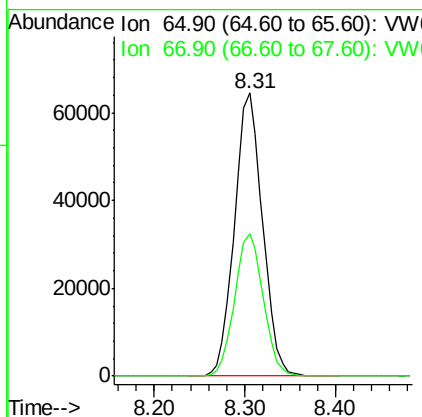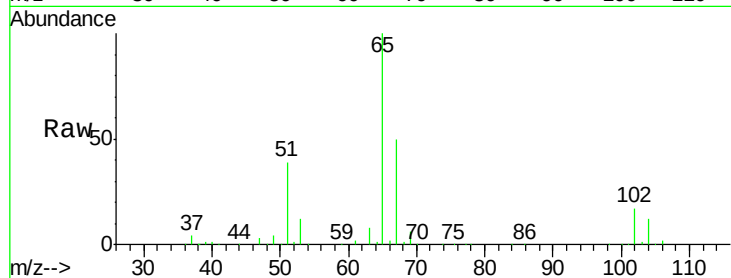

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW011831.D
 Acq: 10 Aug 2019 00:17

Tgt Ion: 114 Resp: 341365
 Ion Ratio Lower Upper
 114 100
 63 25.2 0.0 49.2
 88 16.9 0.0 33.8


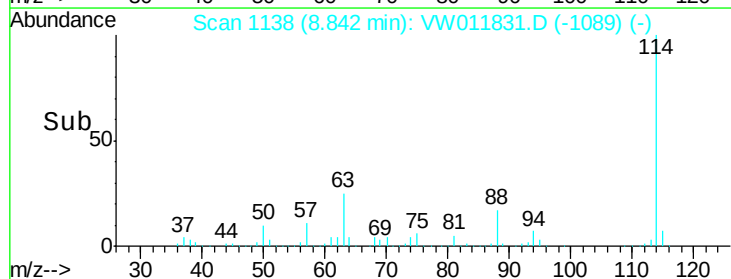
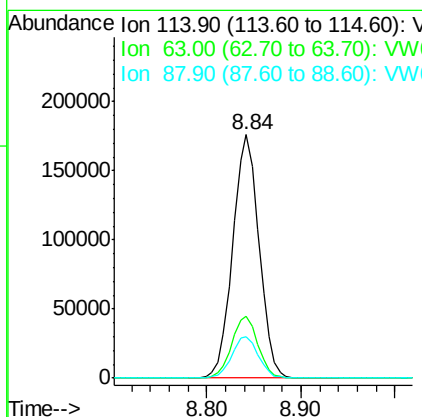
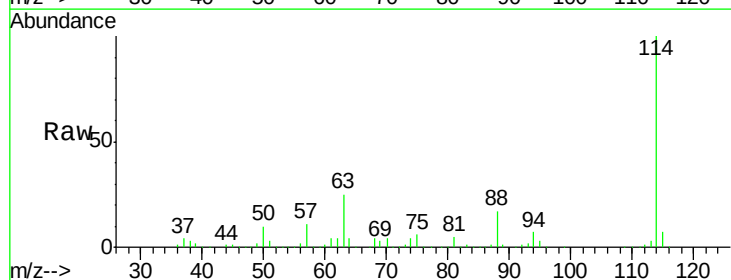


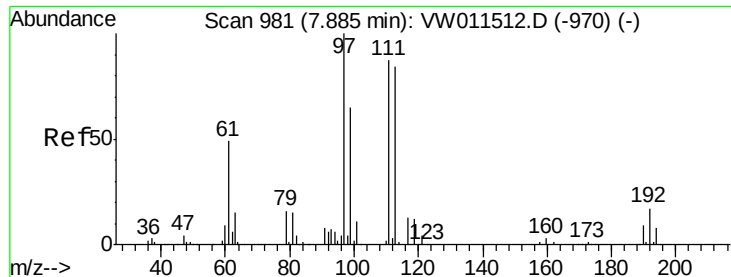

#35
 Dibromofluoromethane
 Concen: 56.345 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. 0.00 min
 Lab File: VW011831.D
 Acq: 10 Aug 2019 00:17




Instrument :
 MSVOA_W
 ClientSampleId :
 1S-O-(1)


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.3	82.7	124.1
192	19.9	16.1	24.1

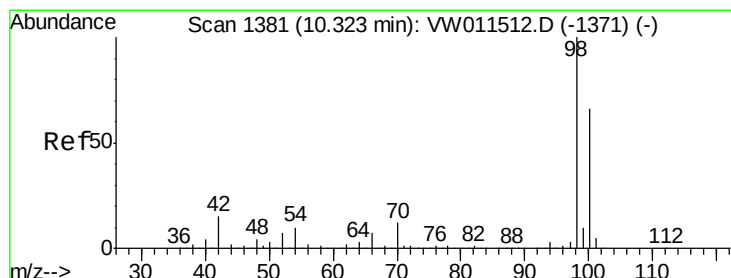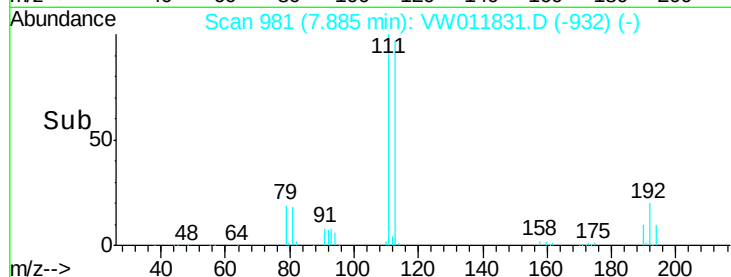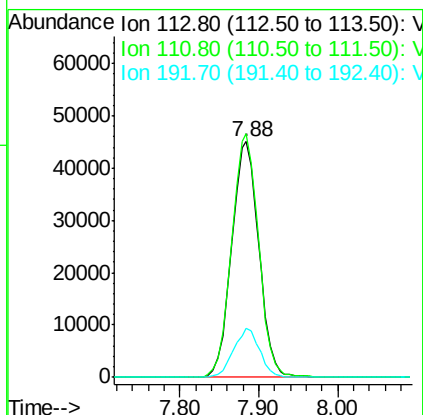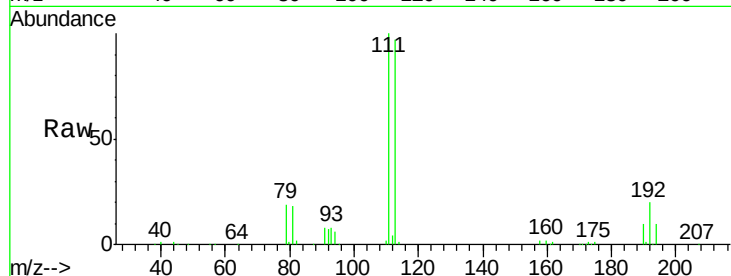

#50
 Toluene-d8
 Concen: 53.506 ug/l
 RT: 10.32 min Scan# 1381
 Delta R.T. 0.00 min
 Lab File: VW011831.D
 Acq: 10 Aug 2019 00:17

Tgt Ion	Ratio	Lower	Upper
98	100		
100	65.5	52.7	79.1


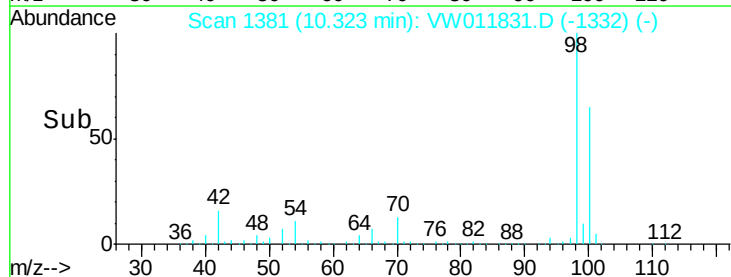
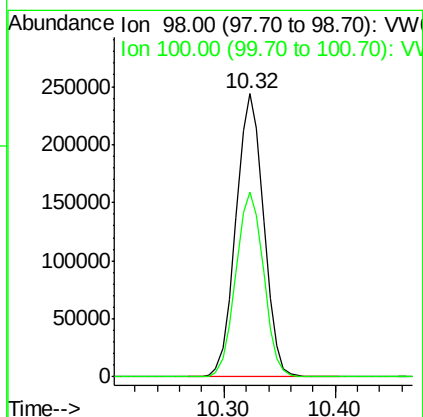
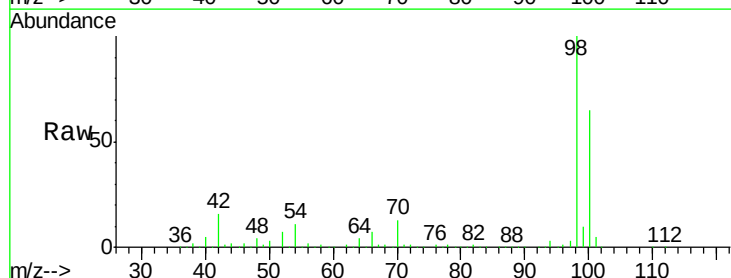


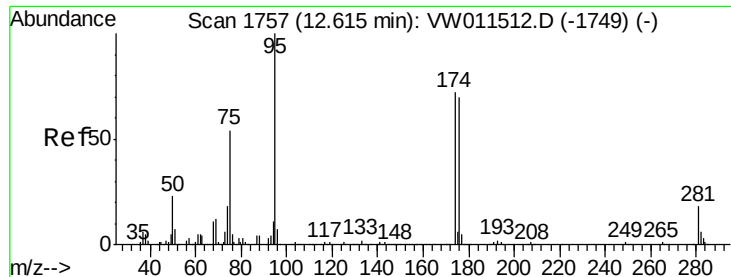

#62
4-Bromofluorobenzene
Concen: 47.431 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. 0.01 min
Lab File: VW011831.D
Acq: 10 Aug 2019 00:17




Instrument :
MSVOA_W
ClientSampleId :
1S-O-(1)


Tot Ion: 95 Resp: 132593
Ion Ratio Lower Upper
95 100
174 74.9 0.0 150.2
176 72.4 0.0 144.4

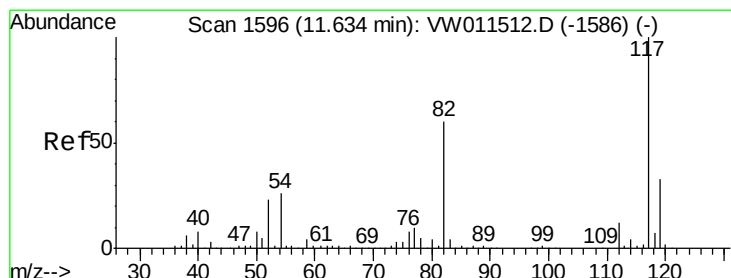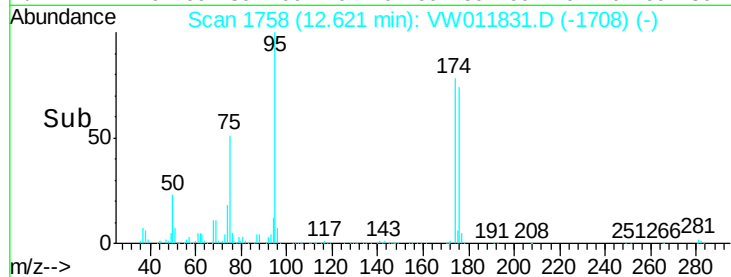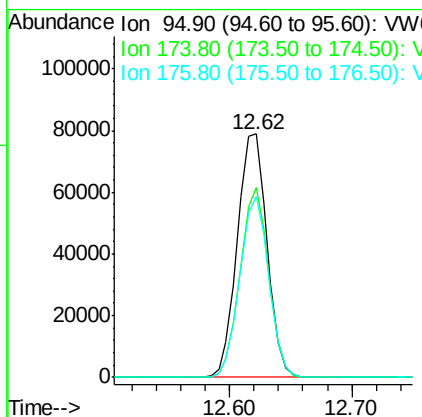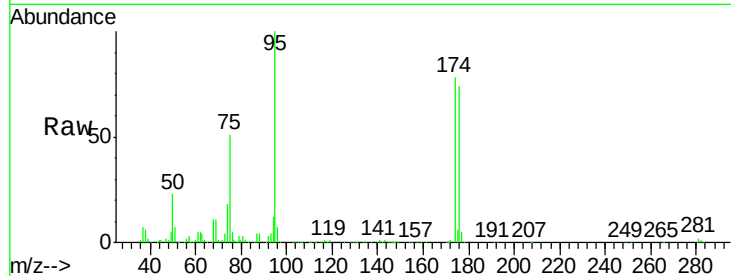

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW011831.D
Acq: 10 Aug 2019 00:17

Tgt Ion: 117 Resp: 286260
Ion Ratio Lower Upper
117 100
82 59.3 47.9 71.9
119 31.4 26.2 39.2

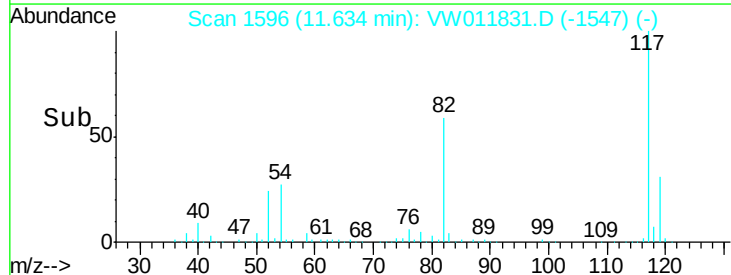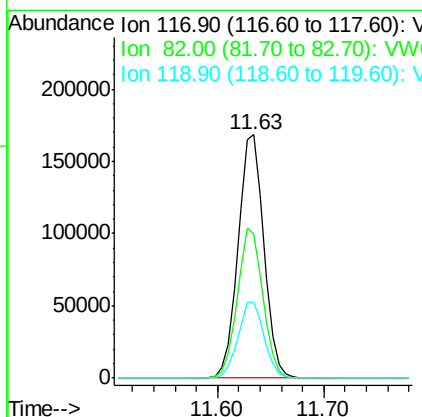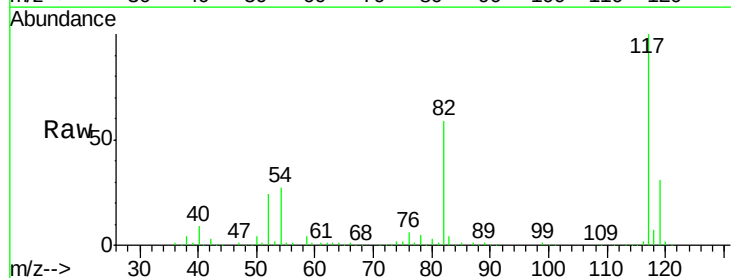

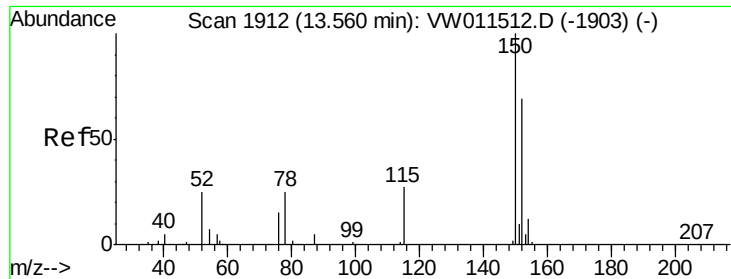

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. 0.00 min

Lab File: VW011831.D

Acq: 10 Aug 2019 00:17

Instrument :

MSVOA_W

ClientSampleId :

1S-O-(1)


Tot Ion:152 Resp: 112990

Ion Ratio Lower Upper

152 100

115 60.3 30.5 91.5

150 157.2 0.0 352.6

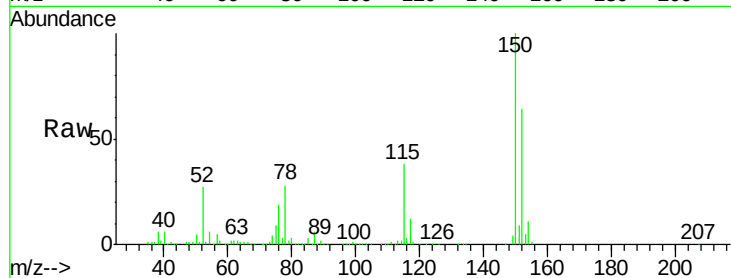

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

