

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081219\
 Data File : VW011840.D
 Acq On : 12 Aug 2019 09:56
 Operator : SY/VA
 Sample : VW0812SBL02
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0812SBL02

Quant Time: Aug 13 07:59:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 27 00:23:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	210043	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	347734	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	288939	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	119464	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	132704	55.02	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.04%	
35) Dibromofluoromethane	7.88	113	108508	55.62	ug/l	0.00
Spiked Amount 50.000			Recovery	=	111.24%	
50) Toluene-d8	10.32	98	422554	52.90	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.80%	
62) 4-Bromofluorobenzene	12.62	95	137169	48.17	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.34%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW081219\
Data File : VW011840.D
Acq On : 12 Aug 2019 09:56
Operator : SY/VA
Sample : VW0812SBL02
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW0812SBL02

Quant Time: Aug 13 07:59:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 27 00:23:30 2019
Response via : Initial Calibration

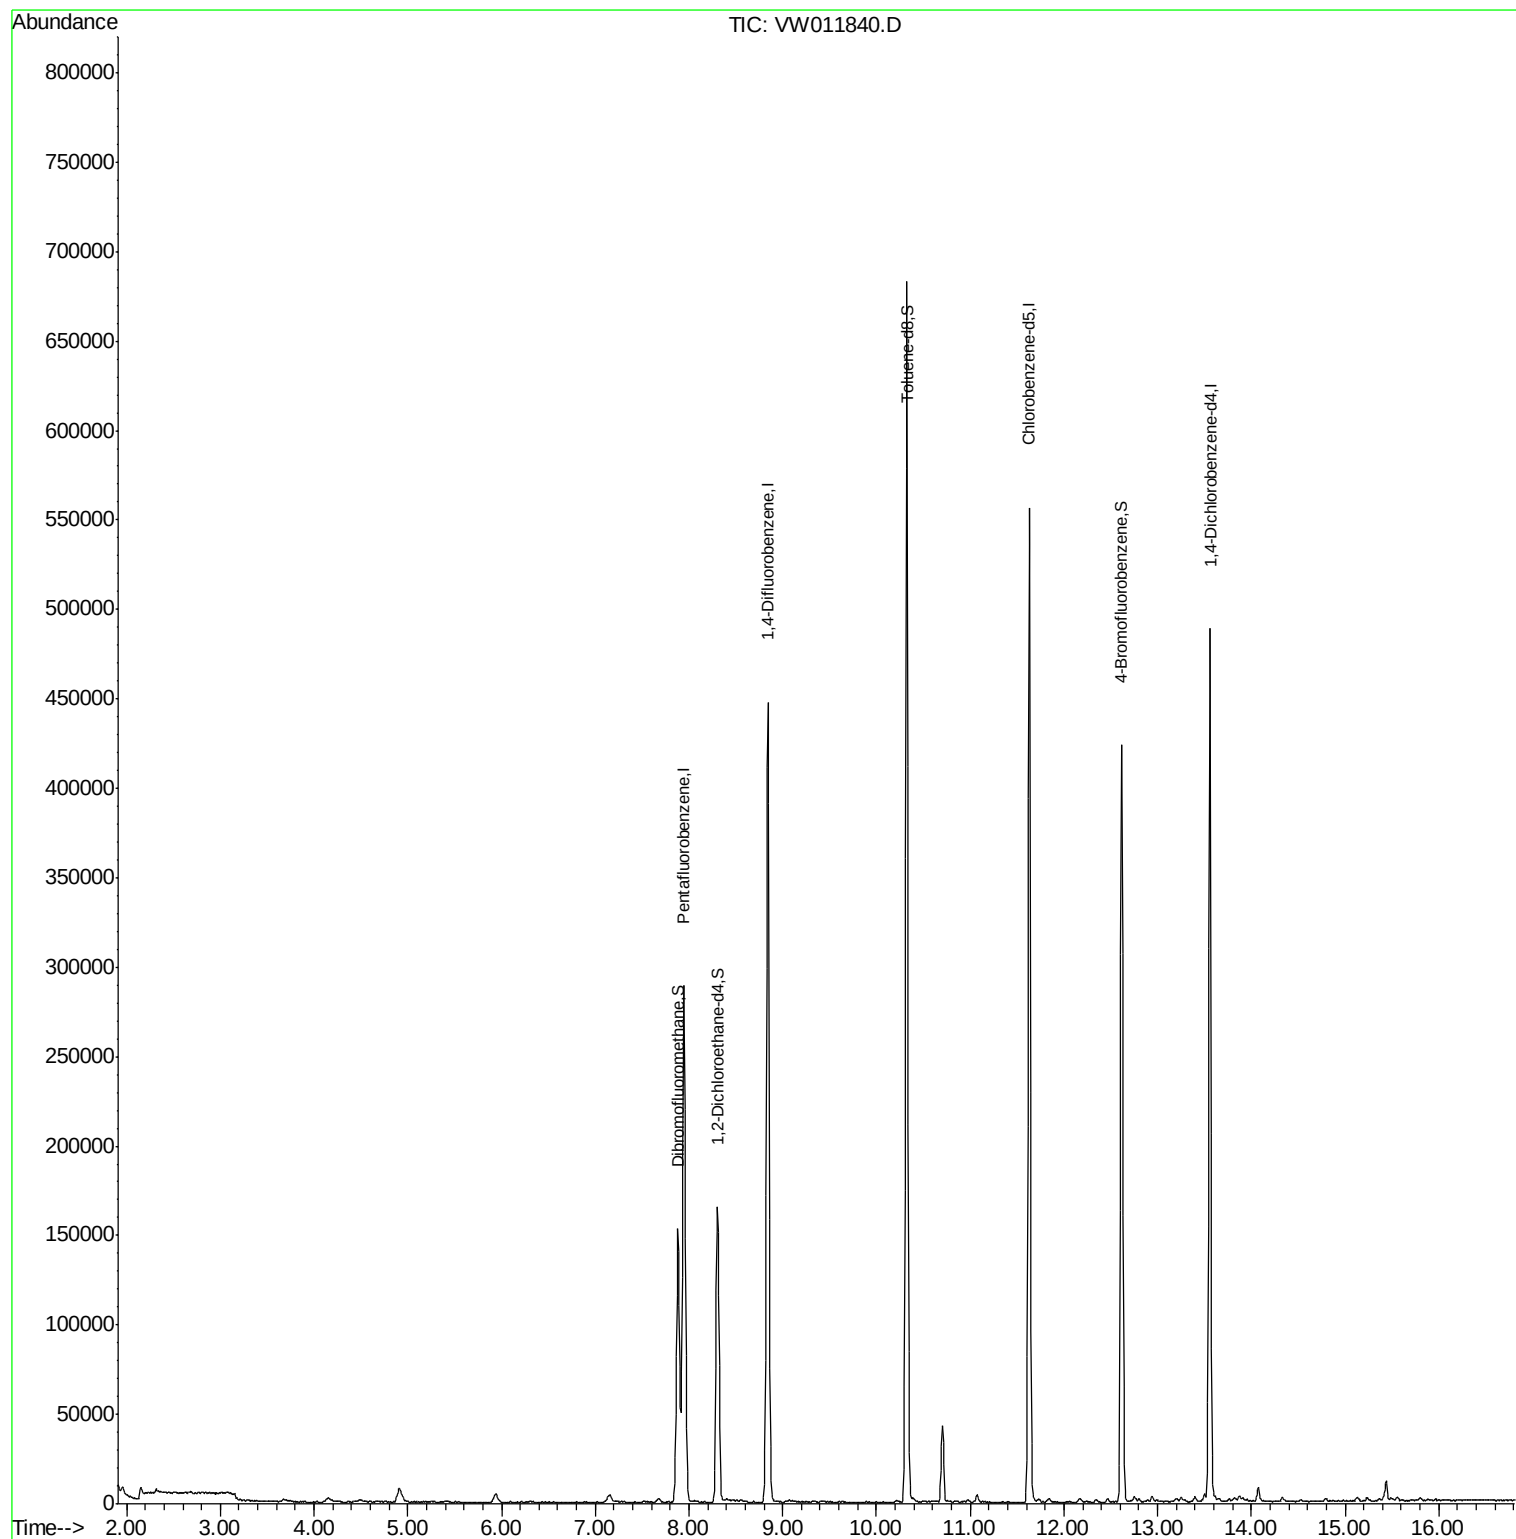

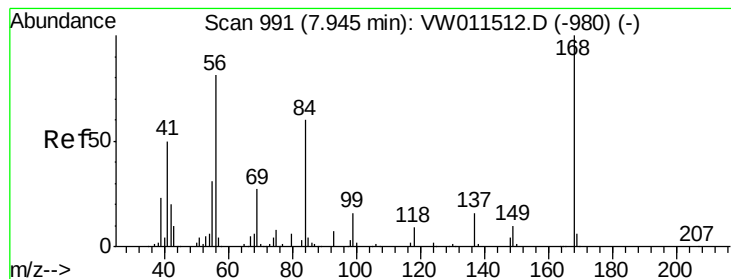

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW011840.D

Acq: 12 Aug 2019 09:56

Instrument :

MSVOA_W

ClientSampleId :


VW0812SBL02

Tot Ion:168 Resp: 210043

Ion Ratio Lower Upper

168 100

99 60.8 48.2 72.4

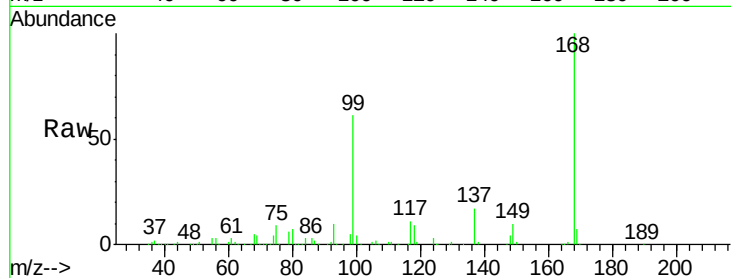

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00 8.10

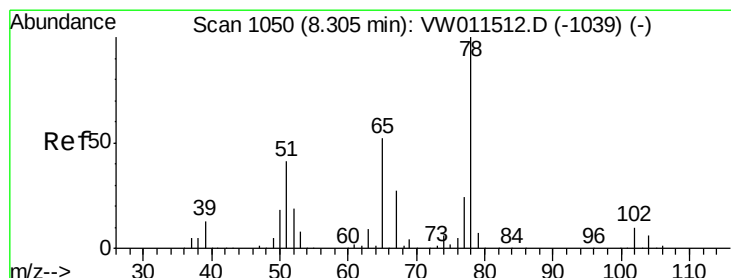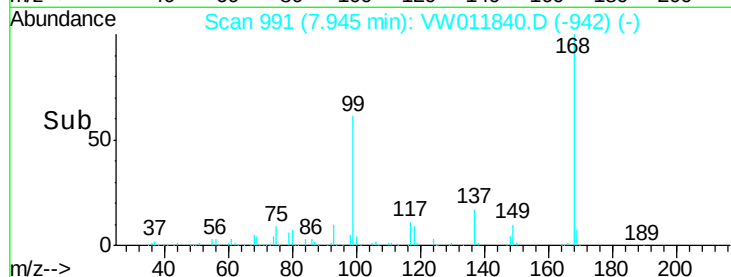

#33

1,2-Dichloroethane-d4

Concen: 55.021 ug/l

RT: 8.30 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW011840.D


Acq: 12 Aug 2019 09:56

Tgt Ion: 65 Resp: 132704

Ion Ratio Lower Upper

65 100

67 51.6 0.0 105.2

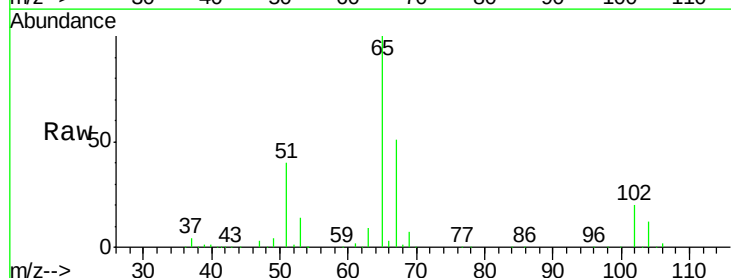

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.30


60000


40000

20000

0

Time--> 8.20 8.30 8.40

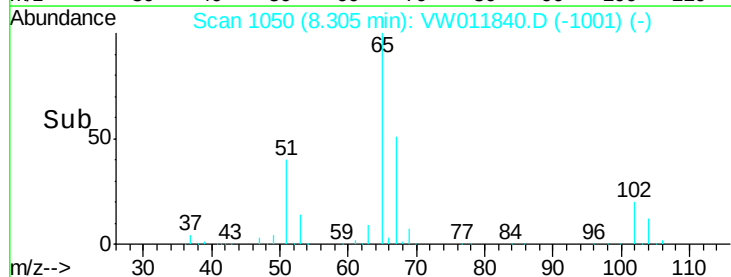


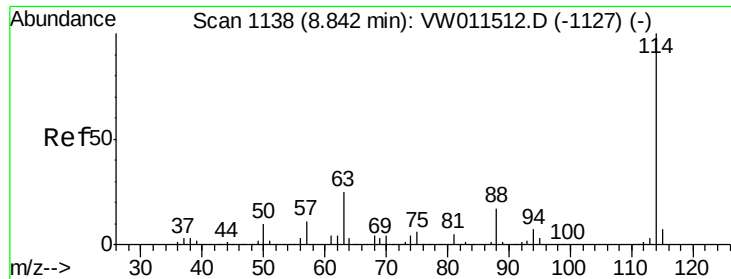




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VW011840.D
 Acq: 12 Aug 2019 09:56

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0812SBL02

Tot Ion:	114	Resp:	347734
Ion	Ratio	Lower	Upper
114	100		
63	24.0	0.0	49.2
88	16.9	0.0	33.8

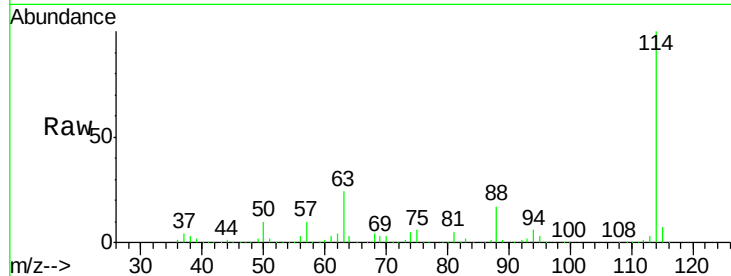


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

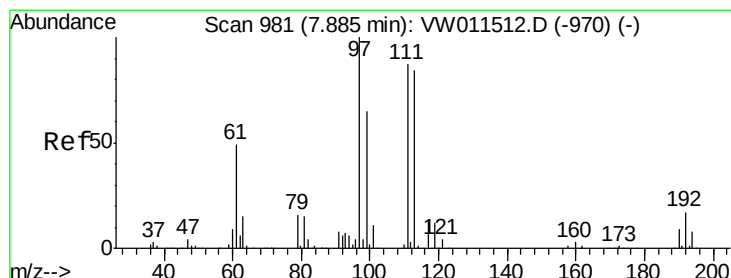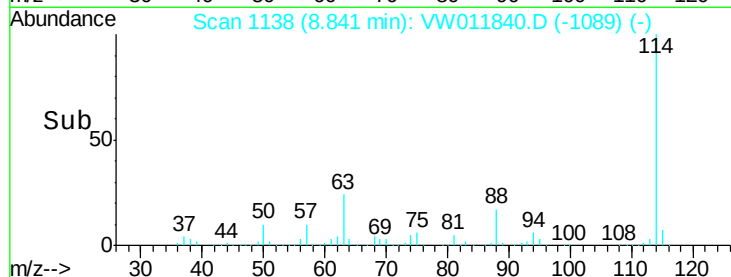
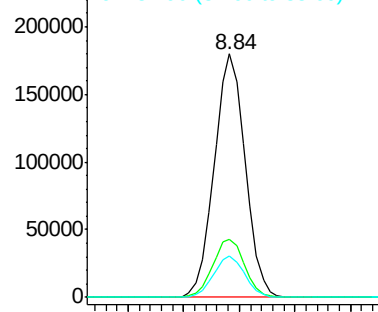



#35
 Dibromofluoromethane
 Concen: 55.621 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.00 min
 Lab File: VW011840.D
 Acq: 12 Aug 2019 09:56

Tgt Ion:	113	Resp:	108508
Ion	Ratio	Lower	Upper
113	100		
111	102.3	82.7	124.1
192	20.8	16.1	24.1

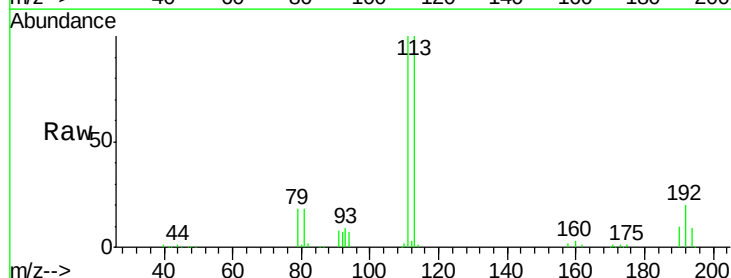

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



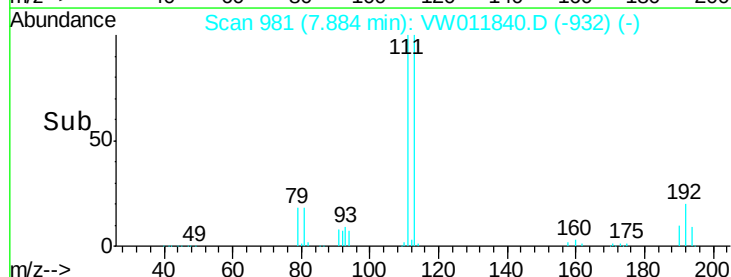
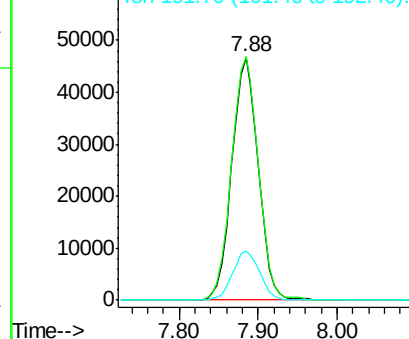


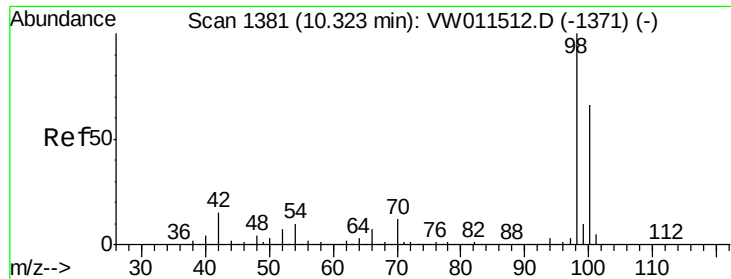

#50
Toluene-d8
Concen: 52.903 ug/l
RT: 10.32 min Scan# 1381
Delta R.T. -0.00 min
Lab File: VW011840.D
Acq: 12 Aug 2019 09:56




Instrument :
MSVOA_W
ClientSampleId :
VW0812SBL02


Tot Ion: 98 Resp: 422554
Ion Ratio Lower Upper
98 100
100 65.3 52.7 79.1

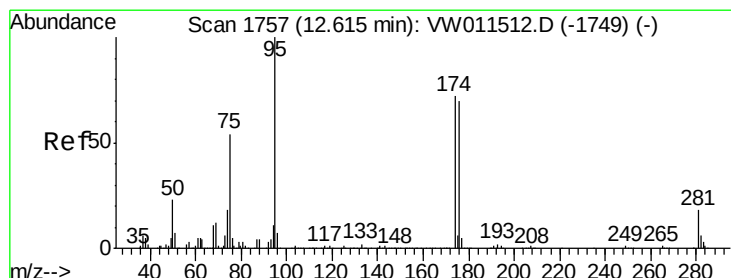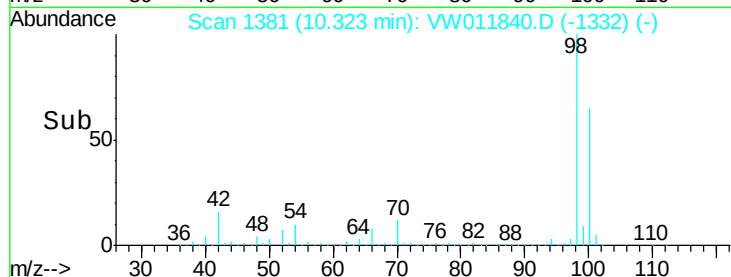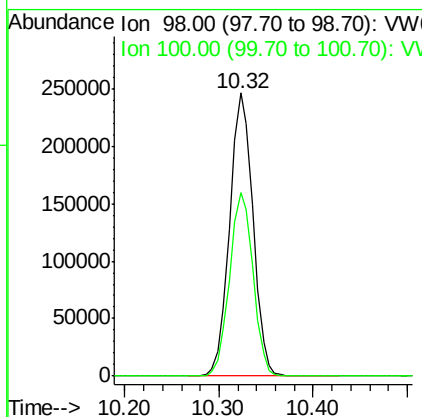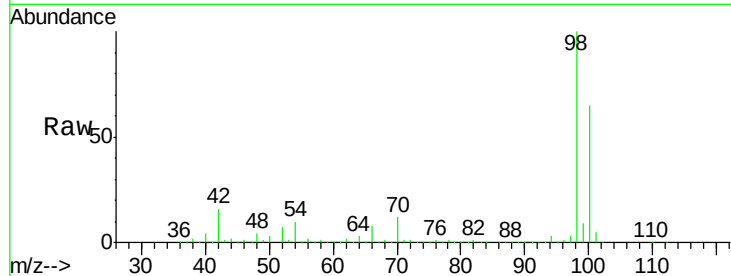

#62
4-Bromofluorobenzene
Concen: 48.169 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. 0.01 min
Lab File: VW011840.D
Acq: 12 Aug 2019 09:56

Tgt Ion: 95 Resp: 137169
Ion Ratio Lower Upper
95 100
174 75.5 0.0 150.2
176 72.9 0.0 144.4


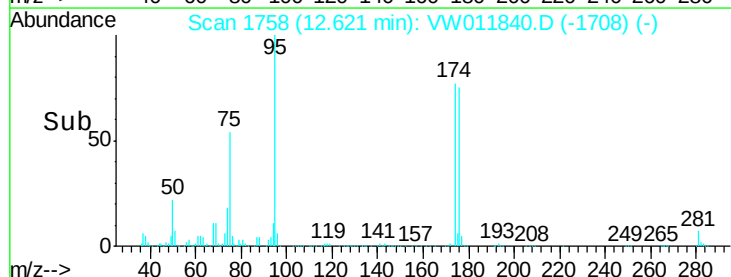
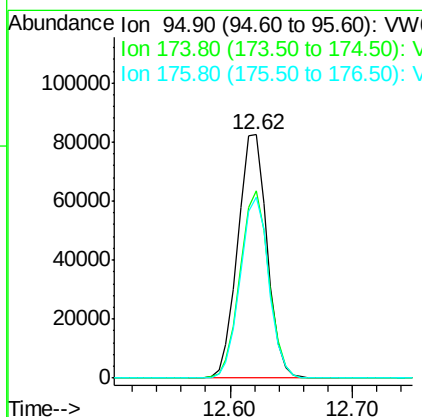
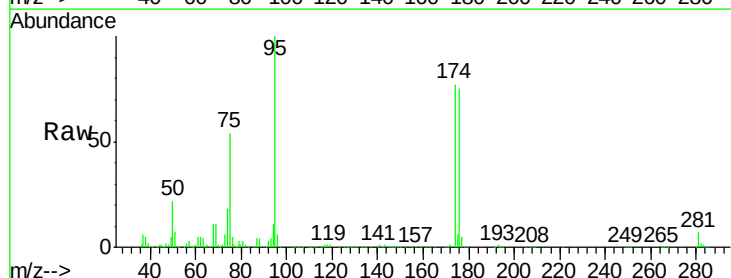


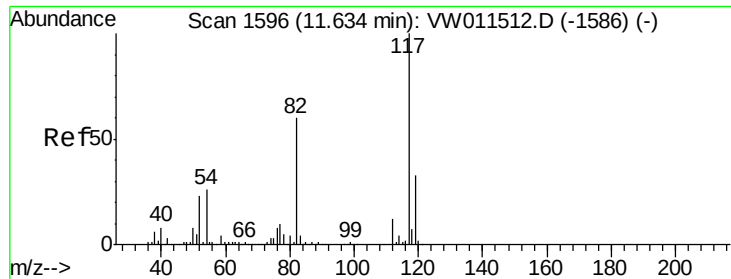

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW011840.D
Acq: 12 Aug 2019 09:56

Instrument :
MSVOA_W
ClientSampleId :
VW0812SBL02

Tot Ion:117 Resp: 288939
Ion Ratio Lower Upper
117 100
82 60.3 47.9 71.9
119 31.5 26.2 39.2

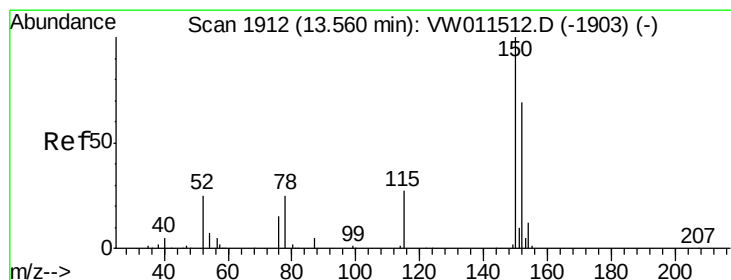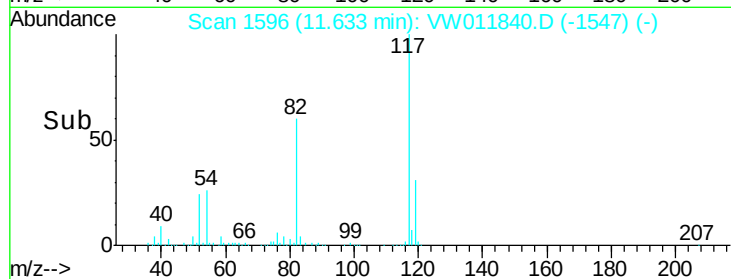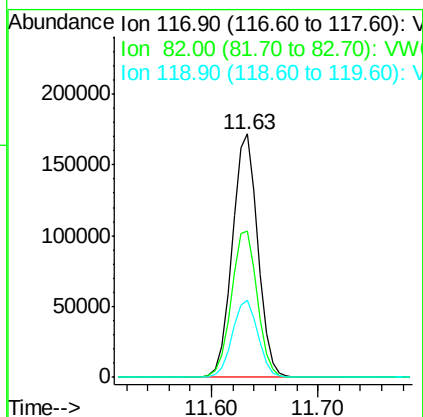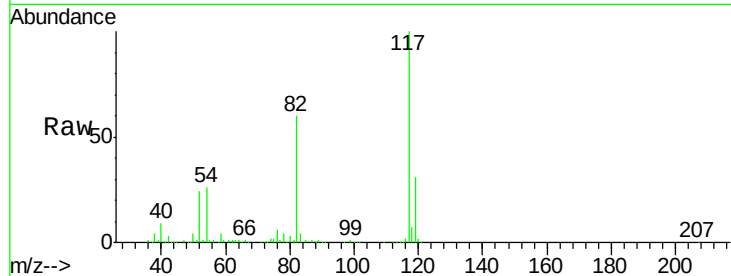

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW011840.D
Acq: 12 Aug 2019 09:56

Tgt Ion:152 Resp: 119464
Ion Ratio Lower Upper
152 100
115 60.6 30.5 91.5
150 158.7 0.0 352.6

