

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081219\
 Data File : VW011881.D
 Acq On : 13 Aug 2019 05:28
 Operator : SY/VA
 Sample : K4230-11
 Misc : 6.14G/5ML/MSVOA W/SOIL
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 2S-D3-(1)

Quant Time: Aug 13 10:06:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 27 00:23:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	225636	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	380141	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	304474	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	108685	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	152759	58.96	ug/l	0.00
Spiked Amount 50.000			Recovery	=	117.92%	
35) Dibromofluoromethane	7.88	113	117697	55.19	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.38%	
50) Toluene-d8	10.32	98	459934	52.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.34%	
62) 4-Bromofluorobenzene	12.62	95	137218	44.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.16%	
Target Compounds						
16) Acetone	4.14	43	17236	20.913	ug/l	99
20) Methylene Chloride	4.90	84	4132	1.454	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW081219\
Data File : VW011881.D
Acq On : 13 Aug 2019 05:28
Operator : SY/VA
Sample : K4230-11
Misc : 6.14G/5ML/MSVOA W/SOIL
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
2S-D3-(1)

Quant Time: Aug 13 10:06:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 27 00:23:30 2019
Response via : Initial Calibration

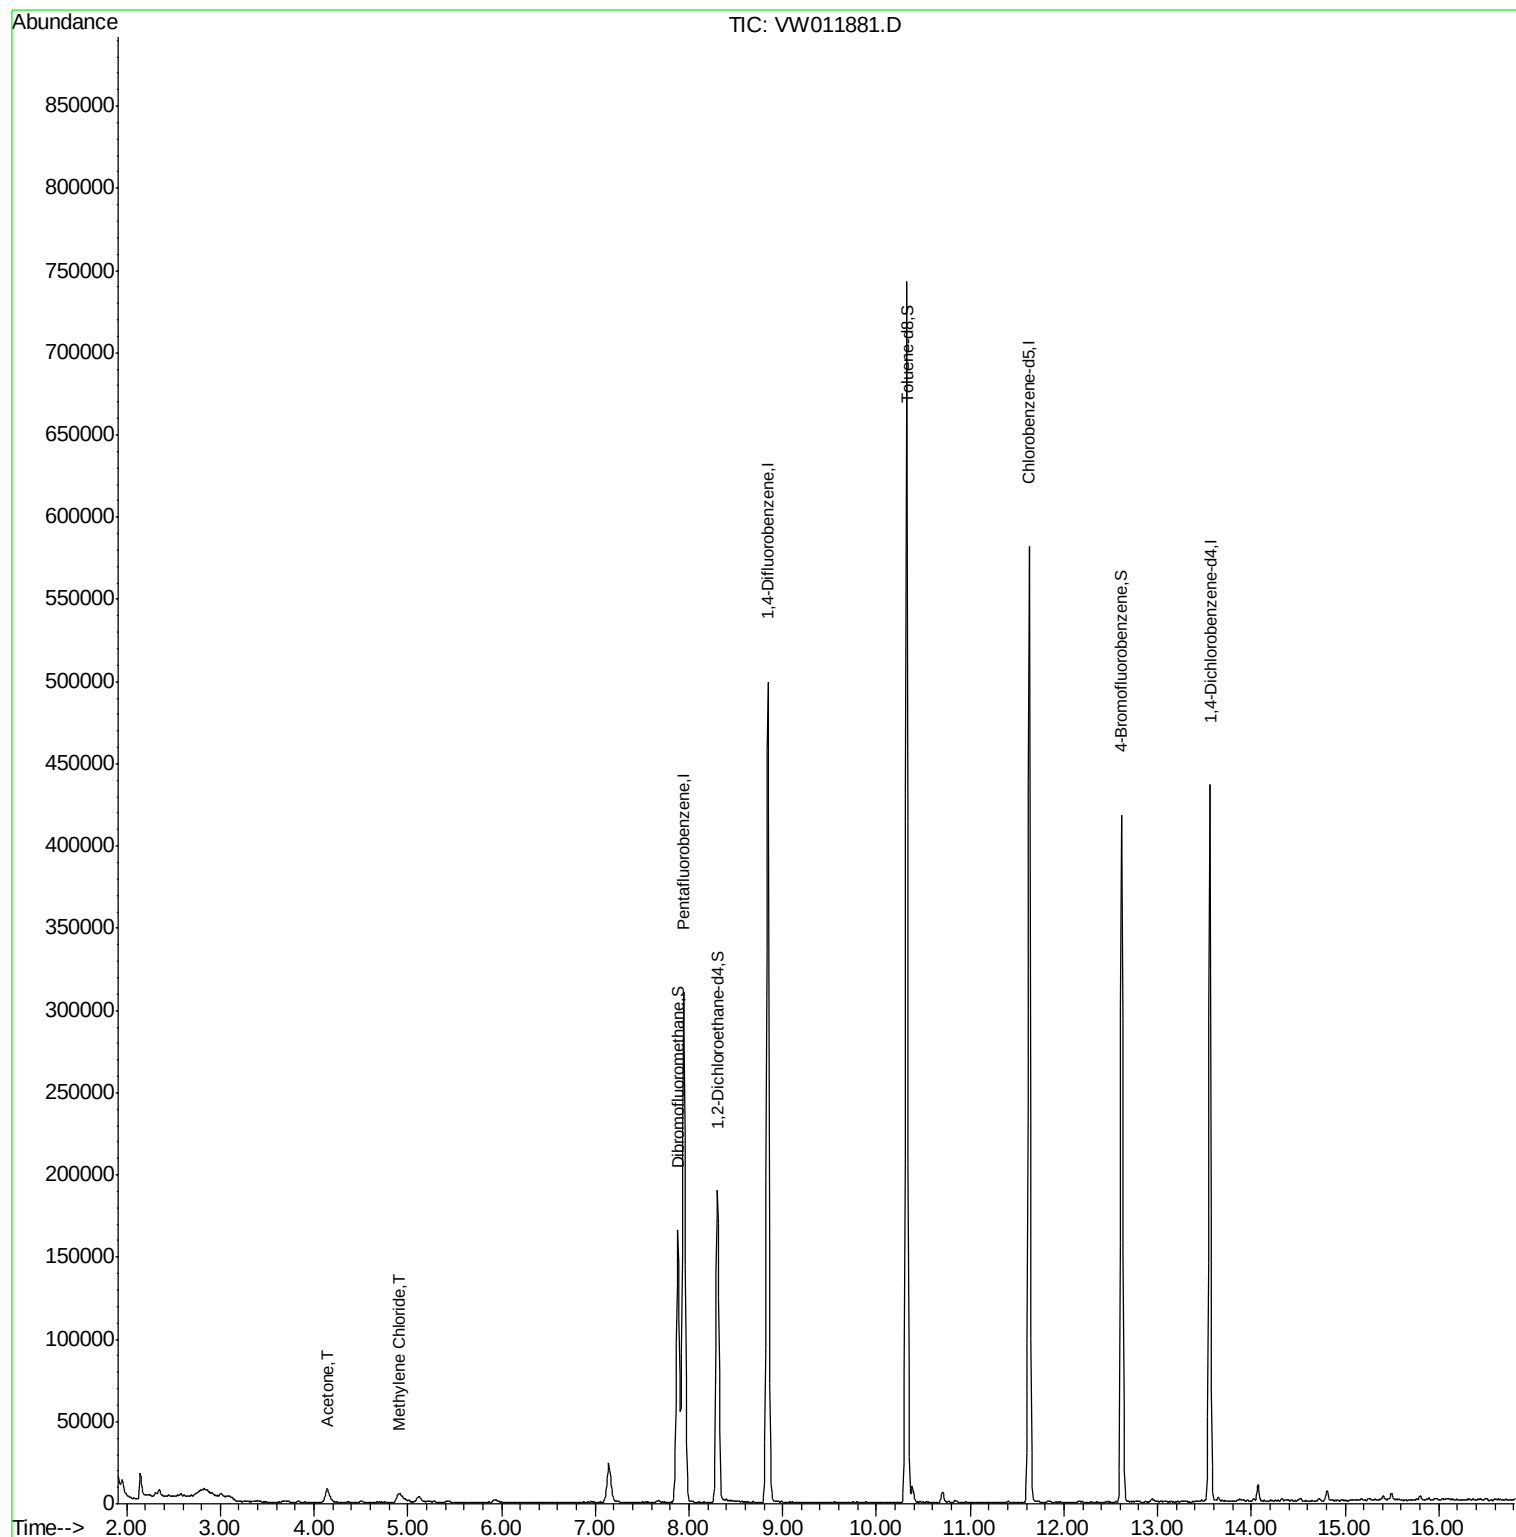

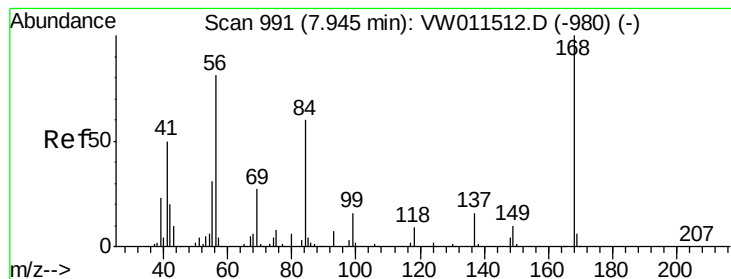

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW011881.D

Acq: 13 Aug 2019 05:28

Instrument :

MSVOA_W

ClientSampleId :


2S-D3-(1)

Tot Ion:168 Resp: 225636

Ion Ratio Lower Upper

168 100

99 61.3 48.2 72.4

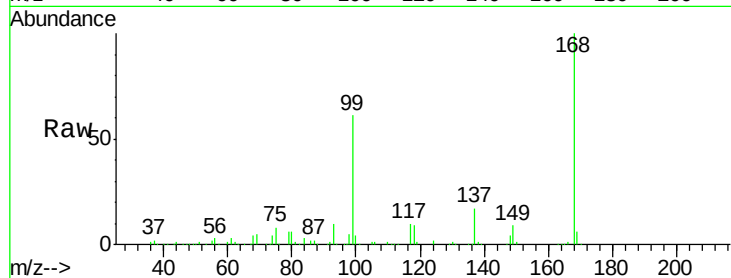

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00 8.10

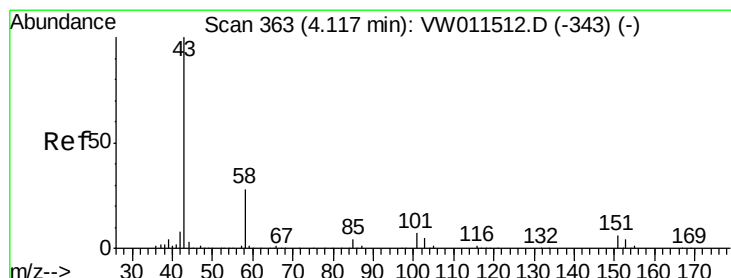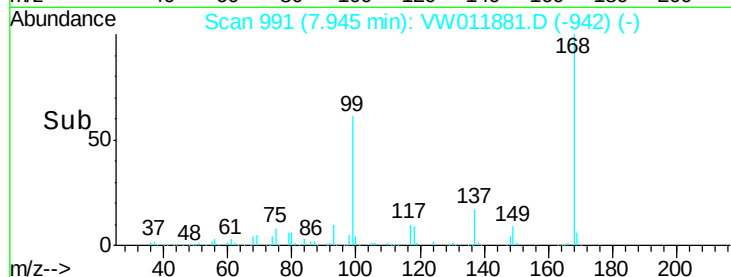

#16

Acetone

Concen: 20.913 ug/l

RT: 4.14 min Scan# 367

Delta R.T. 0.02 min

Lab File: VW011881.D


Acq: 13 Aug 2019 05:28

Tgt Ion: 43 Resp: 17236

Ion Ratio Lower Upper

43 100

58 27.1 22.3 33.5

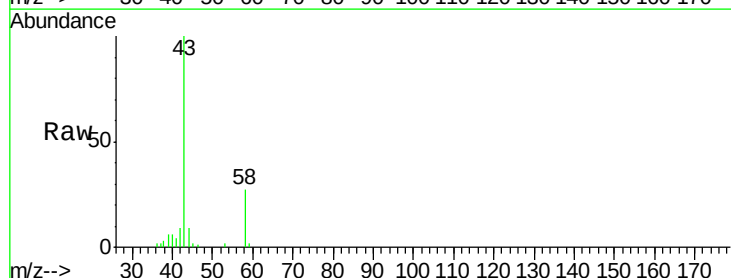

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.14

6000

5000

4000


3000


2000

1000

0

Time--> 4.00 4.10 4.20 4.30

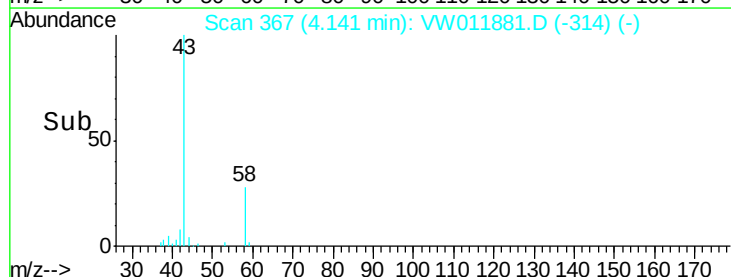

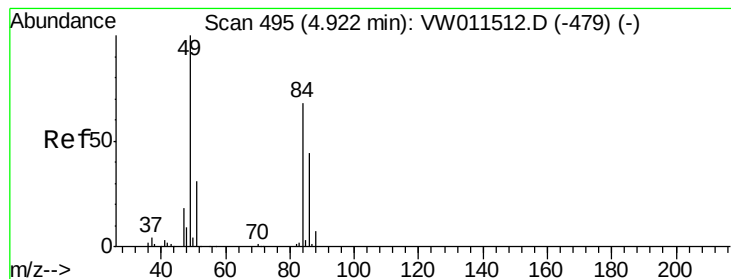

#20

Methylene Chloride

Concen: 1.454 ug/l

RT: 4.90 min Scan# 492

Delta R.T. -0.02 min

Lab File: VW011881.D

Acq: 13 Aug 2019 05:28

Instrument :

MSVOA_W

ClientSampleId :

2S-D3-(1)

Tot Ion: 84 Resp: 4132





Ion Ratio Lower Upper

84 100

49 143.0 117.8 176.6

51 54.9 37.0 55.4

86 60.2 51.8 77.8

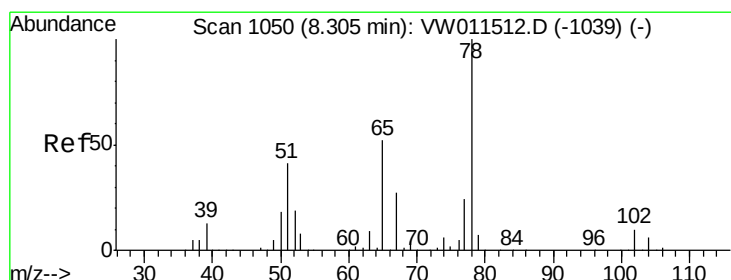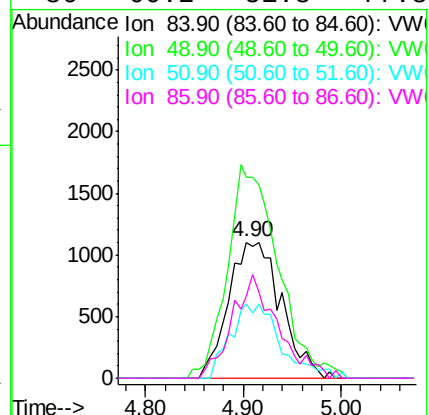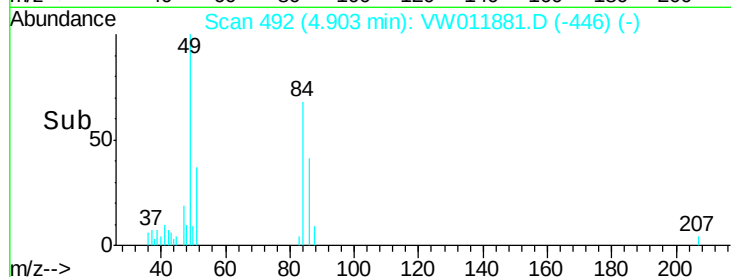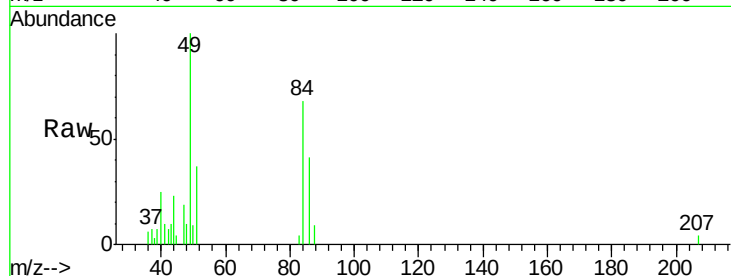

#33

1,2-Dichloroethane-d4

Concen: 58.959 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW011881.D




Acq: 13 Aug 2019 05:28


Tgt Ion: 65 Resp: 152759

Ion Ratio Lower Upper

65 100

67 51.1 0.0 105.2

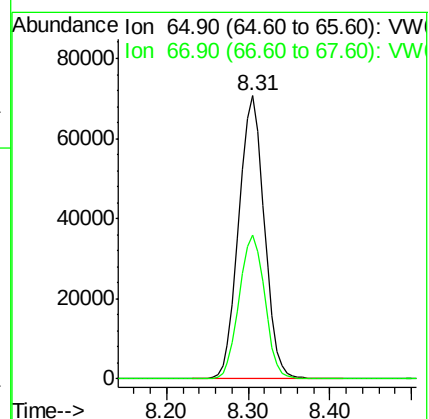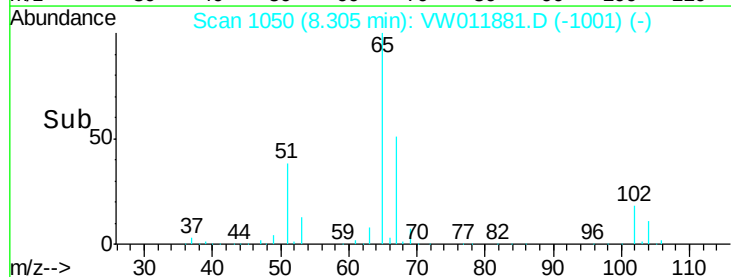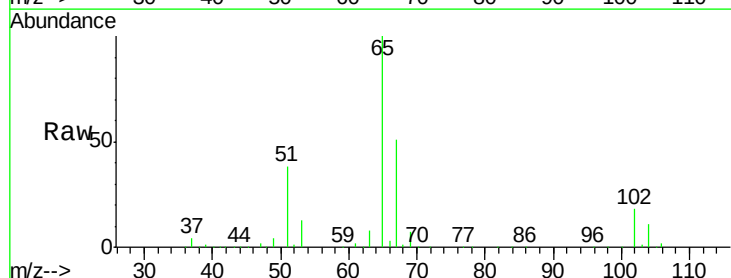

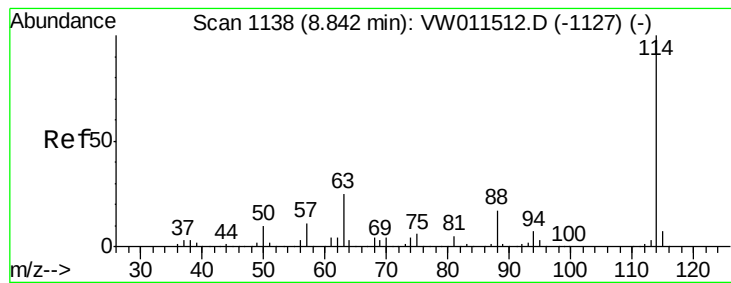

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. -0.00 min

Lab File: VW011881.D

Acq: 13 Aug 2019 05:28

Instrument :

MSVOA_W

ClientSampleId :

2S-D3-(1)


Tot Ion:114 Resp: 380141

Ion Ratio Lower Upper

114 100

63 24.6 0.0 49.2




88 16.4 0.0 33.8

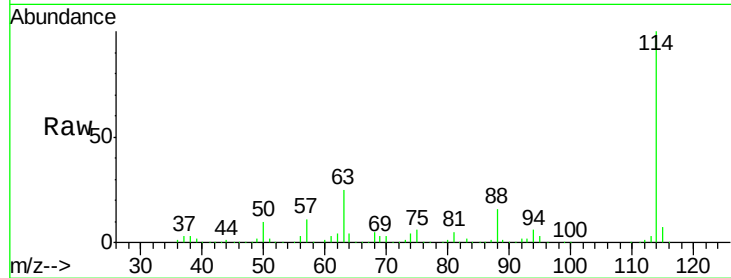

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

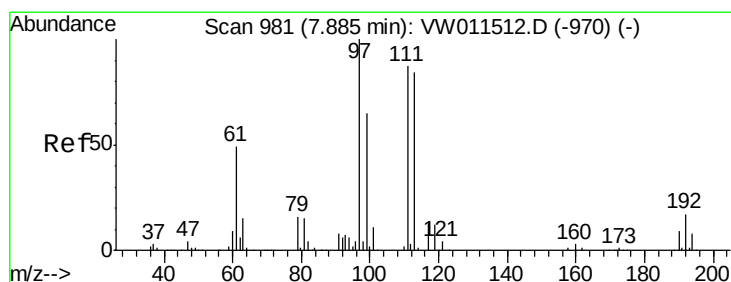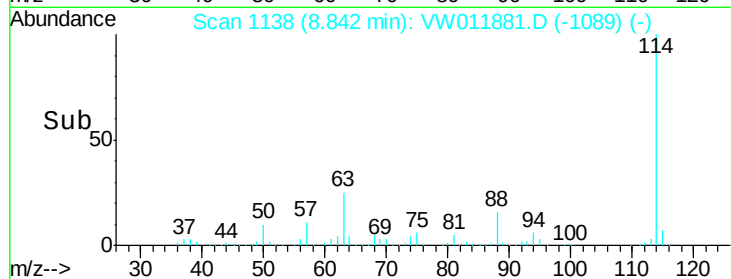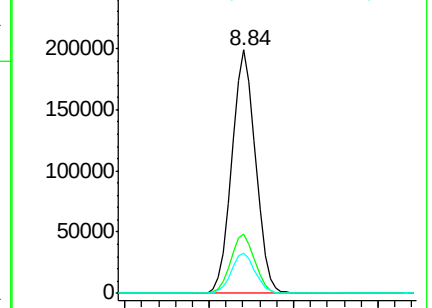

#35

Dibromofluoromethane

Concen: 55.188 ug/l

RT: 7.88 min Scan# 981

Delta R.T. -0.00 min

Lab File: VW011881.D

Acq: 13 Aug 2019 05:28


Tgt Ion:113 Resp: 117697

Ion Ratio Lower Upper

113 100

111 101.7 82.7 124.1



192 19.7 16.1 24.1

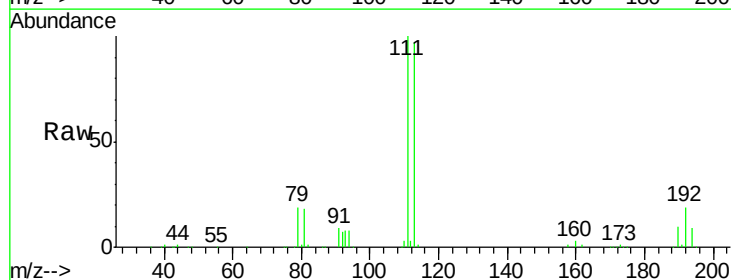


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

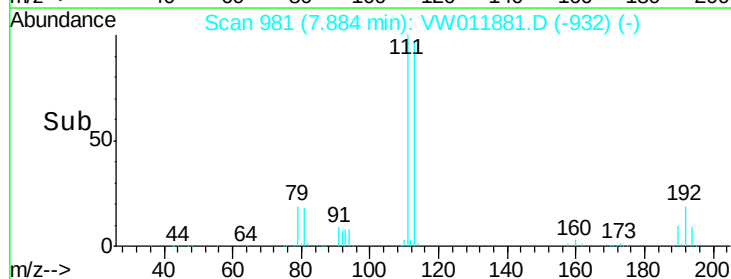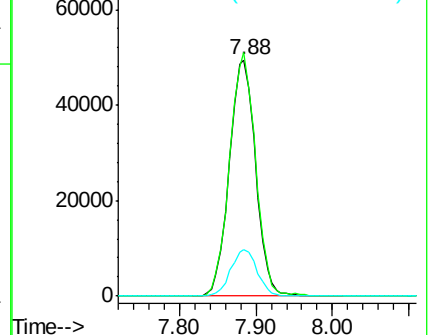

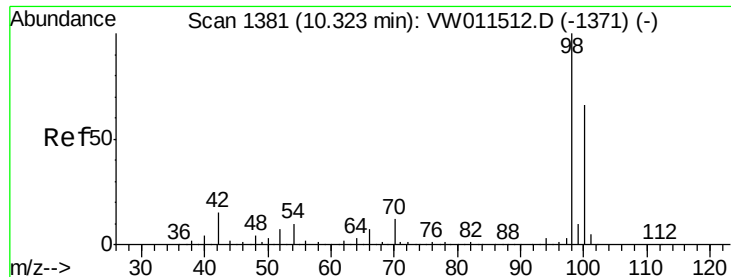

#50

Toluene-d8

Concen: 52.674 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.00 min

Lab File: VW011881.D

Acq: 13 Aug 2019 05:28

Instrument :

MSVOA_W

ClientSampleId :


2S-D3-(1)

Tot Ion: 98 Resp: 459934

Ion Ratio Lower Upper




98 100

100 65.3 52.7 79.1

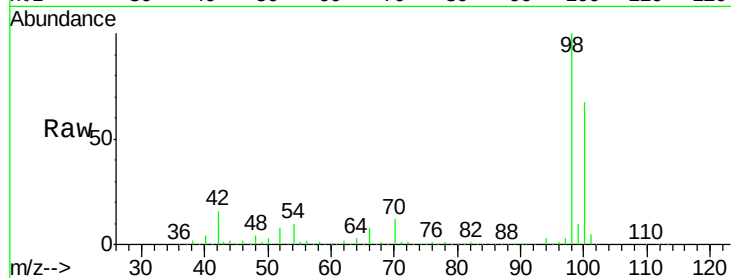

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

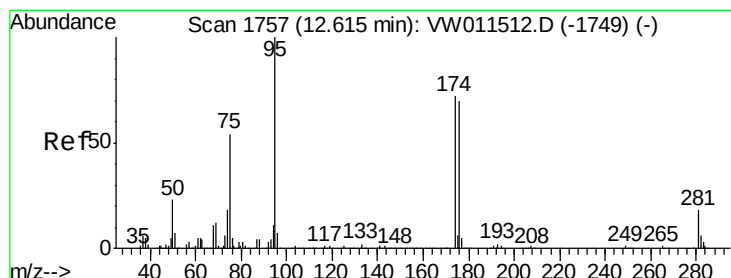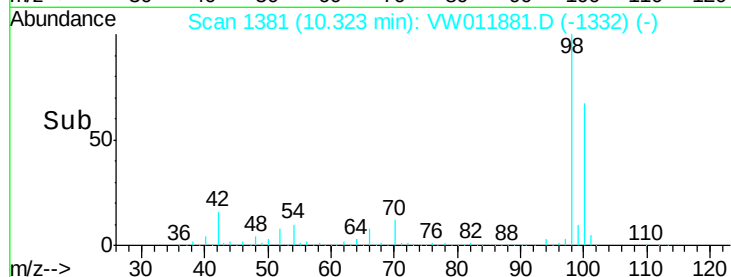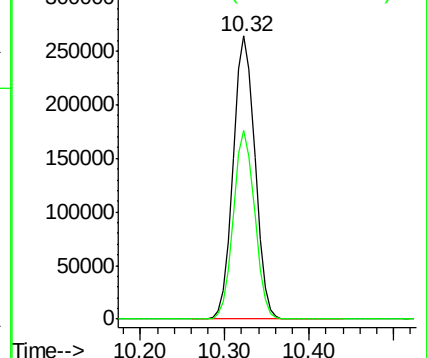

#62

4-Bromofluorobenzene

Concen: 44.079 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.01 min

Lab File: VW011881.D

Acq: 13 Aug 2019 05:28


Tgt Ion: 95 Resp: 137218

Ion Ratio Lower Upper

95 100

174 74.1 0.0 150.2



176 72.0 0.0 144.4

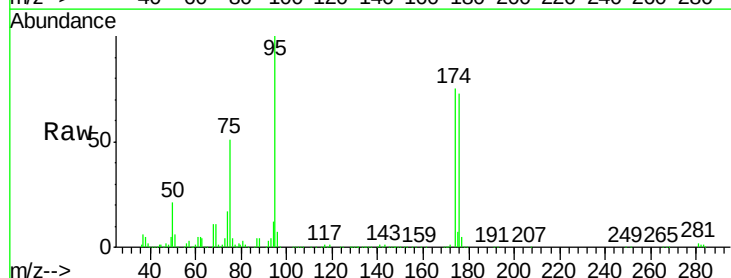


Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW



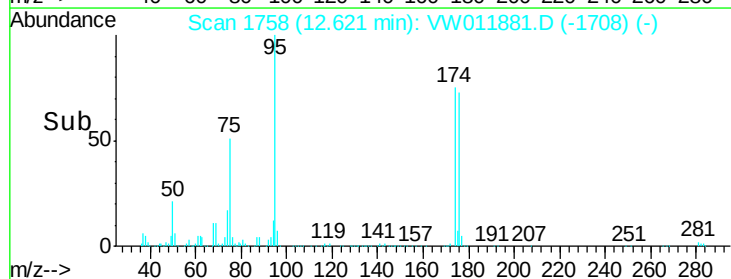
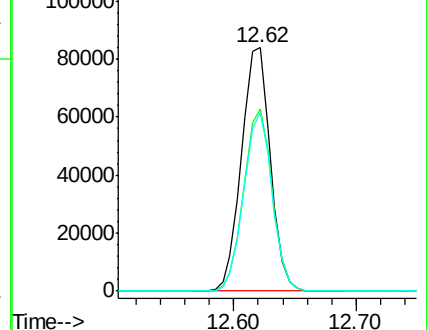


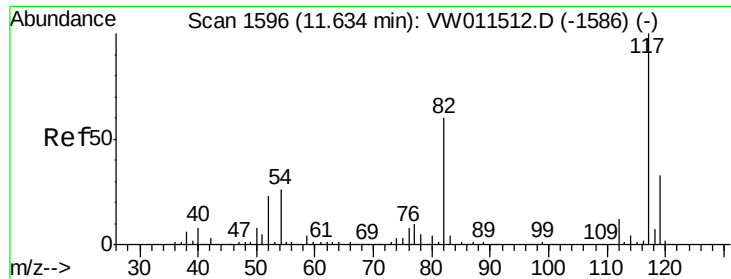

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW011881.D
Acq: 13 Aug 2019 05:28

Instrument :
MSVOA_W
ClientSampleId :
2S-D3-(1)

Tot Ion:117 Resp: 304474
Ion Ratio Lower Upper
117 100
82 60.3 47.9 71.9
119 32.9 26.2 39.2

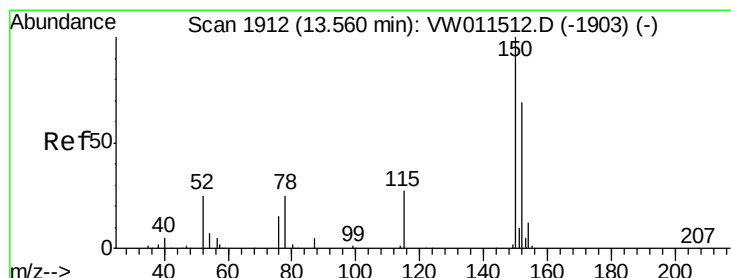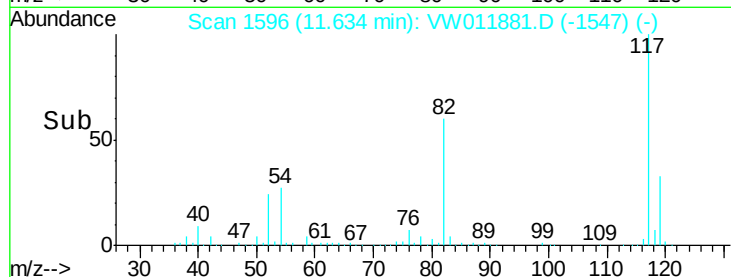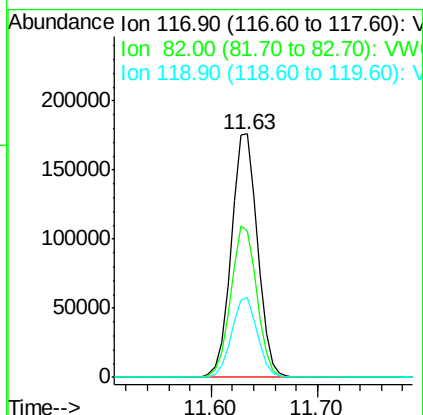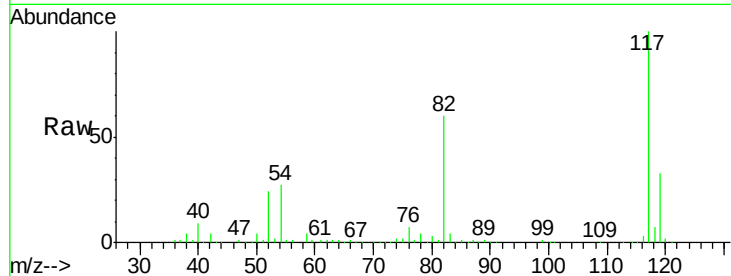

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW011881.D
Acq: 13 Aug 2019 05:28

Tgt Ion:152 Resp: 108685
Ion Ratio Lower Upper
152 100
115 59.5 30.5 91.5
150 156.1 0.0 352.6

