

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081221\
 Data File : VW019725.D
 Acq On : 12 Aug 2021 14:27
 Operator : SY/VA
 Sample : M3365-08
 Misc : 5.53g/10mL/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBKA0

Quant Time: Aug 13 02:03:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 13 02:01:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	299579	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	288445	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	138237	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	85154	24.341	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.360%		
7) Chloroethane-d5	2.897	69	88913	25.714	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	102.840%		
11) 1,1-Dichloroethene-d2	4.025	63	115663	16.069	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	64.280%		
21) 2-Butanone-d5	7.080	46	58616	51.306	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.620%		
24) Chloroform-d	7.653	84	191654	21.161	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.640%		
26) 1,2-Dichloroethane-d4	8.311	65	114356	21.690	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	86.760%		
32) Benzene-d6	8.275	84	373594	19.562	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	78.240%		
36) 1,2-Dichloropropane-d6	9.274	67	119741	20.841	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	83.360%		
41) Toluene-d8	10.323	98	329726	18.927	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	75.720%		
43) trans-1,3-Dichloroprop...	10.579	79	47663	20.092	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.360%		
47) 2-Hexanone-d5	10.926	63	46731	46.363	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.720%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	106473	21.357	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.440%		
66) 1,2-Dichlorobenzene-d4	13.853	152	113604	22.282	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.120%		
Target Compounds					Qvalue	
42) Toluene	10.390	91	6926	0.330	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081221\
Data File : VW019725.D
Acq On : 12 Aug 2021 14:27
Operator : SY/VA
Sample : M3365-08
Misc : 5.53g/10mL/MSVOA_W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBKA0

Quant Time: Aug 13 02:03:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081121SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 13 02:01:28 2021
Response via : Initial Calibration

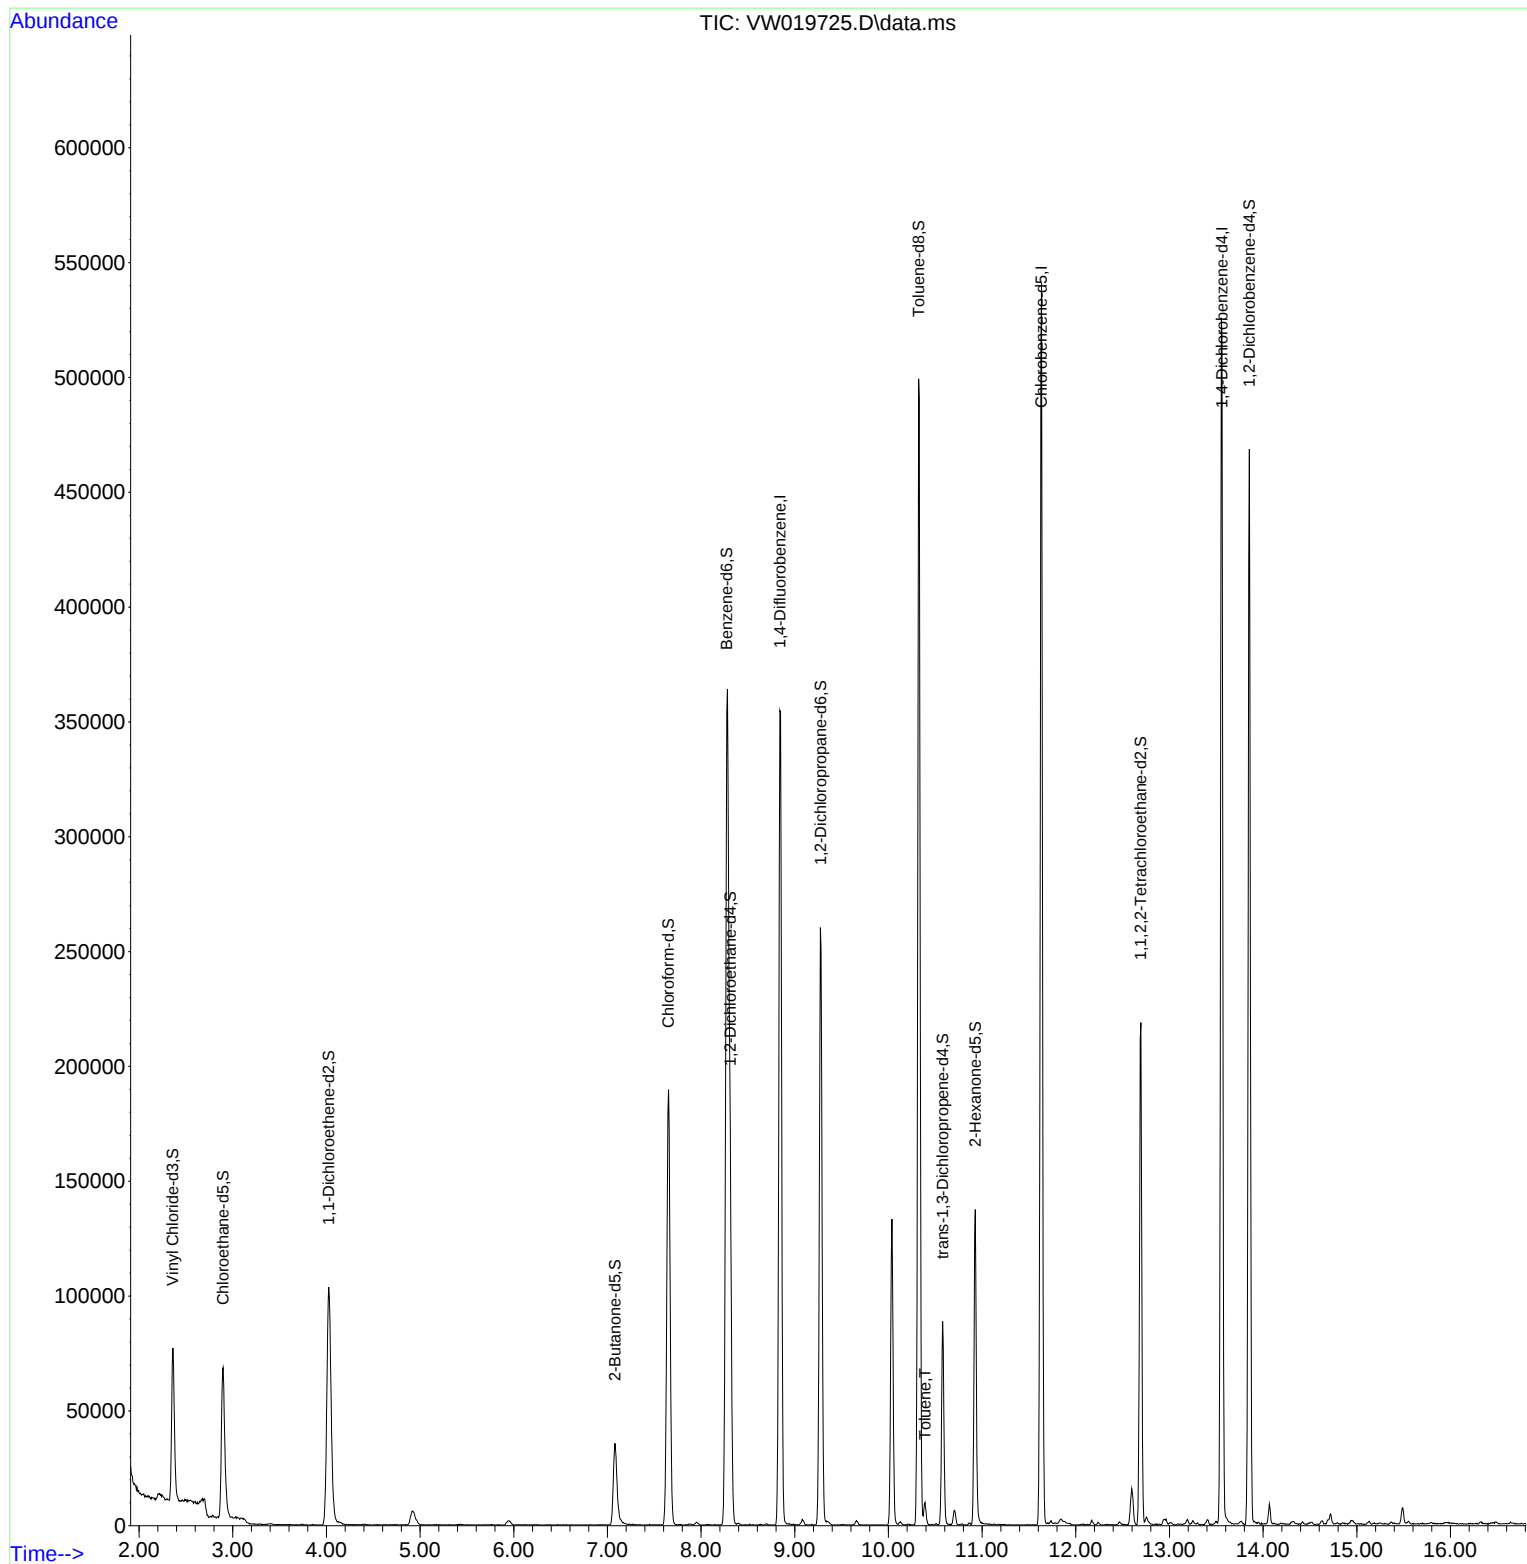

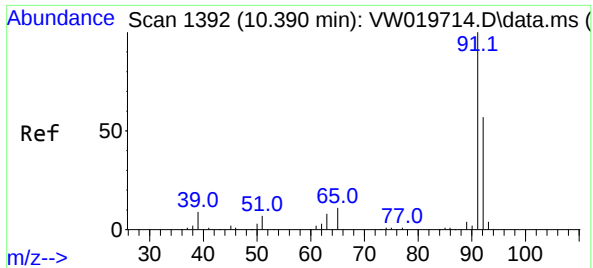

#42
Toluene
Concen: 0.330 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. 0.000 min
Lab File: VW019725.D
Acq: 12 Aug 2021 14:27

Instrument :
MSVOA_W
ClientSampleId :
DBKA0

Tgt Ion: 91 Resp: 6926
Ion Ratio Lower Upper
91 100
92 52.2 39.5 73.3

