


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW081318\
 Data File : VW004586.D
 Acq On : 10 Aug 2018 09:59
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W080618S.M
 Title : SW846 8260
 Last Update : Tue Aug 07 08:22:01 2018

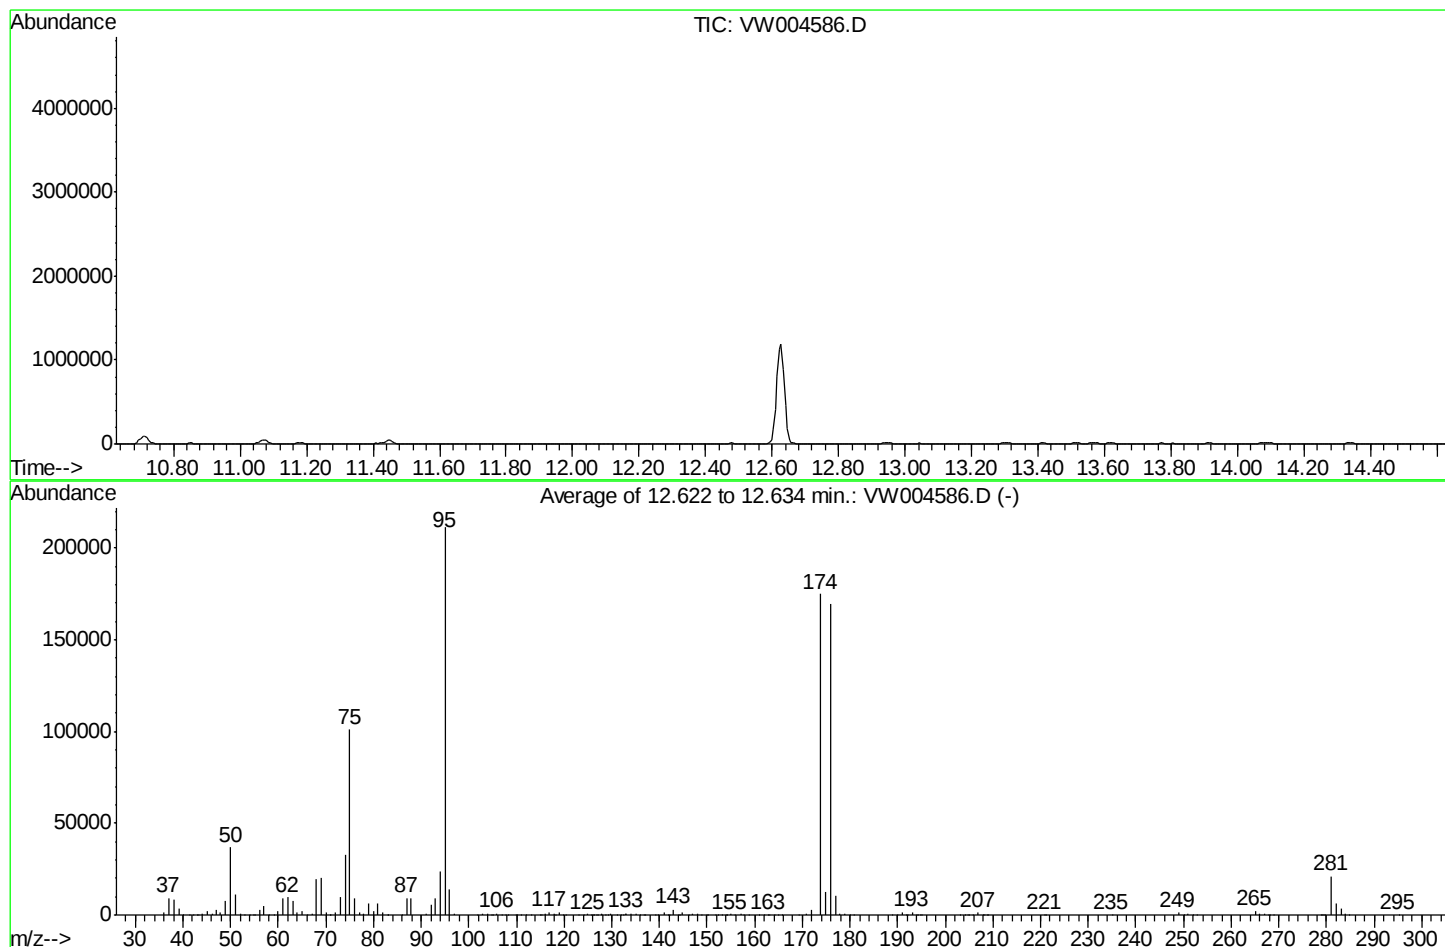

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	36661	PASS
75	95	30	60	47.8	100912	PASS
95	95	100	100	100.0	211285	PASS
96	95	5	9	6.7	14210	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.9	175061	PASS
175	174	5	9	7.3	12744	PASS
176	174	95	101	96.7	169301	PASS
177	176	5	9	6.2	10537	PASS