
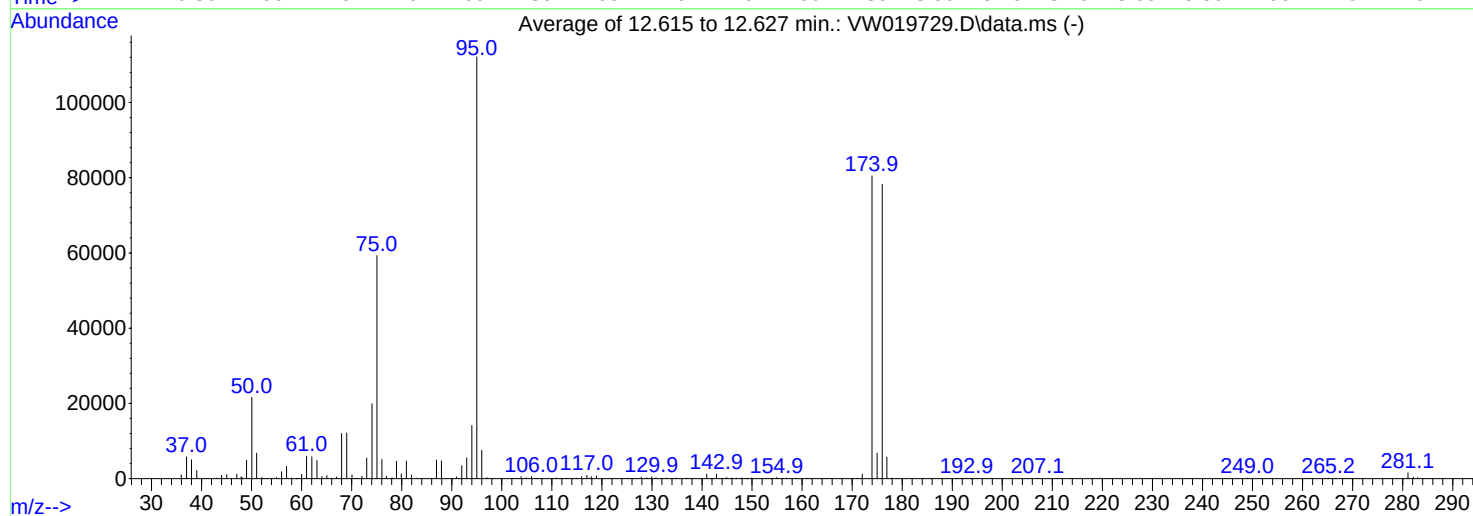


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081321\
 Data File : VW019729.D
 Acq On : 13 Aug 2021 09:27
 Operator : SY/VA
 Sample : BFB416
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB416

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081121SMA.M
 Title : SFAM01.0
 Last Update : Tue Aug 17 12:14:46 2021

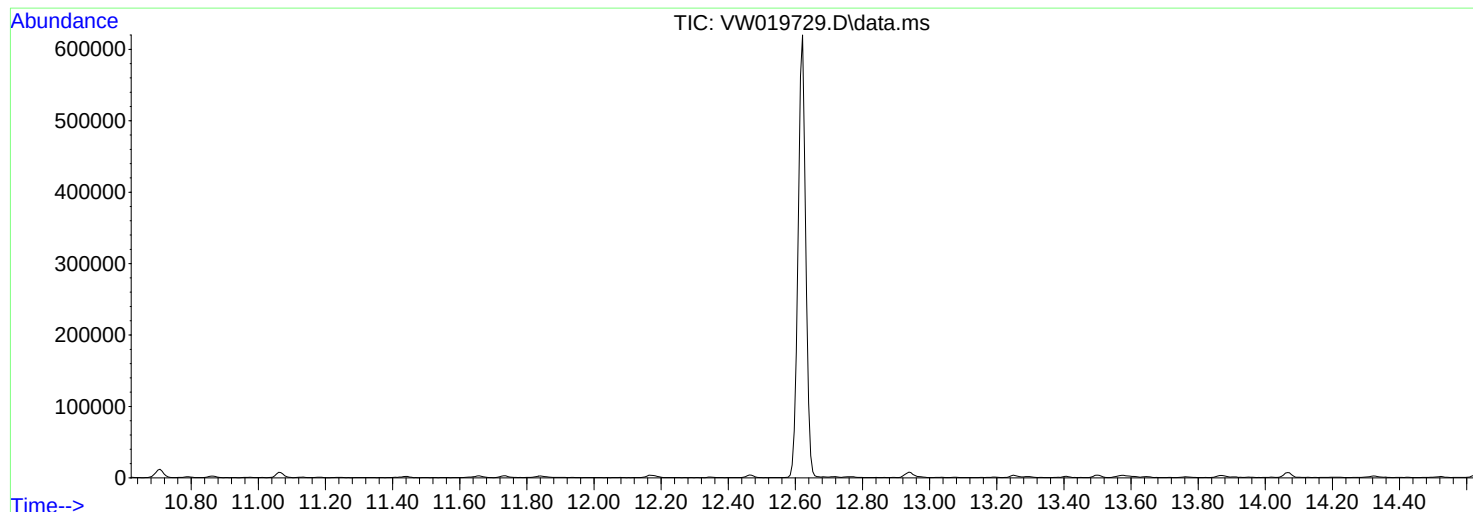

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	21608	PASS
75	95	30	80	52.9	59317	PASS
95	95	100	100	100.0	112139	PASS
96	95	5	9	6.7	7532	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.8	80464	PASS
175	174	5	9	8.4	6752	PASS
176	174	95	105	97.2	78240	PASS
177	176	5	10	7.4	5751	PASS

Scan 1749 (12.566 min): VW019729.D\data.ms
BFB416

m/z	Abundance
40.10	146.0
44.00	189.0
55.10	55.0
57.30	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB416

m/z	Abundance
36.00	1157.0
37.00	6321.0
38.00	5608.0
39.10	2574.0
39.90	250.0
43.10	116.0
44.00	1070.0
45.00	1084.0
46.00	173.0
47.00	1278.0
47.90	844.0
49.00	5640.0
50.00	23752.0
51.00	7469.0
52.20	293.0
52.90	70.0
55.00	401.0
56.00	2066.0
57.00	3484.0
58.00	137.0
58.90	51.0
60.00	1226.0
61.00	6297.0
62.00	6212.0
63.10	5164.0
64.10	706.0
65.10	975.0
66.10	128.0
66.90	475.0
68.00	12897.0
69.00	13482.0
70.10	950.0
71.00	71.0
72.00	691.0
73.00	5697.0
74.00	20592.0
75.10	63616.0
76.00	5298.0
76.90	688.0
77.90	376.0
79.00	5234.0
79.90	1326.0
80.90	4981.0
81.90	1083.0
83.00	172.0
85.90	142.0
86.90	4731.0
87.90	5298.0
90.90	535.0
92.00	3682.0
93.00	5843.0
94.00	14401.0
95.00	117432.0
96.00	8023.0
97.00	257.0
102.80	87.0
103.90	510.0
105.00	226.0
106.00	529.0
107.00	150.0
109.90	95.0
110.90	204.0
111.90	69.0
112.80	150.0
115.00	125.0
115.90	579.0
117.00	969.0
117.90	552.0
118.90	821.0
123.80	85.0
125.00	166.0
126.10	57.0
127.80	412.0
129.00	183.0
130.00	394.0
130.90	275.0
132.90	282.0
133.80	108.0
134.80	266.0
136.80	210.0
139.90	162.0
141.00	1019.0
142.90	1324.0
144.90	344.0
146.00	220.0
147.00	83.0
147.80	241.0
148.80	151.0
149.90	162.0
152.80	60.0
153.80	51.0
155.00	293.0

Instrument :
MSVOA_W
ClientSampleId :
BFB416

155.90	65.0
156.90	273.0
158.70	104.0
161.00	136.0
165.10	72.0
170.20	90.0
171.00	179.0
172.00	1321.0
174.00	75776.0
175.00	6826.0
176.00	71952.0
177.00	5549.0
177.90	182.0
179.10	108.0
190.90	220.0
192.10	63.0
193.00	167.0
193.70	56.0
194.10	69.0
195.00	83.0
207.10	129.0
249.00	237.0
249.80	72.0
265.20	333.0
266.00	75.0
266.50	88.0
281.10	2500.0
282.10	526.0
283.10	450.0
284.20	139.0

Instrument :
MSVOA_W
ClientSampleId :
BFB416

m/z	Abundance
35.90	1099.0
37.00	6509.0
38.00	5636.0
39.00	2271.0
40.00	213.0
41.00	78.0
43.10	154.0
44.00	1097.0
45.10	1246.0
45.90	78.0
47.00	1400.0
48.10	845.0
49.00	5302.0
50.00	23736.0
51.00	7511.0
52.00	328.0
53.00	114.0
55.00	432.0
56.00	1988.0
57.00	3685.0
57.90	180.0
60.00	1221.0
61.00	6929.0
62.00	6555.0
63.00	5234.0
64.00	578.0
65.00	876.0
66.00	117.0
67.00	492.0
68.00	12955.0
69.00	13251.0
70.00	1177.0
70.90	54.0
72.10	758.0
73.00	6201.0
74.00	23440.0
75.00	65912.0
76.00	5712.0
77.00	641.0
78.10	506.0
78.90	5133.0
79.90	1442.0
80.90	5092.0
82.00	954.0
83.00	108.0
86.00	184.0
87.00	5376.0
88.00	5093.0
90.90	479.0
92.00	3880.0
93.00	6485.0
94.00	16156.0
95.00	126360.0
96.00	8279.0
97.10	327.0
102.80	86.0
103.90	733.0
104.90	280.0
105.90	698.0
107.10	124.0
109.90	166.0
110.80	149.0
111.90	88.0
112.80	132.0
115.00	139.0
116.00	455.0
117.00	928.0
117.90	600.0
118.90	693.0
123.80	101.0
125.10	123.0
125.80	97.0
127.00	81.0
127.90	486.0
128.90	182.0
129.90	488.0
130.80	198.0
133.00	169.0
134.00	76.0
135.00	224.0
137.00	228.0
140.20	146.0
140.90	1375.0
143.00	1287.0
145.00	294.0
145.90	199.0
146.80	148.0
148.10	327.0
148.80	97.0
149.90	179.0
152.90	95.0
154.90	274.0

Instrument :
MSVOA_W
ClientSampleId :
BFB416

156.90	168.0
158.90	161.0
160.90	239.0
171.00	253.0
172.00	1234.0
173.90	92816.0
175.00	7214.0
176.00	94456.0
176.90	6506.0
177.90	238.0
191.10	158.0
192.80	127.0
207.10	213.0
249.10	70.0
264.90	112.0
281.00	1496.0
282.10	351.0
283.00	256.0

Instrument :
MSVOA_W
ClientSampleId :
BFB416

m/z	Abundance
36.00	776.0
37.00	4503.0
38.00	3815.0
39.10	1659.0
39.90	189.0
41.00	89.0
43.10	88.0
44.00	904.0
45.00	863.0
47.10	1054.0
47.90	646.0
49.00	3755.0
50.10	17336.0
51.00	5319.0
52.10	246.0
52.90	89.0
55.00	331.0
56.00	1425.0
57.00	2660.0
58.10	178.0
60.00	1013.0
61.00	4646.0
62.10	4749.0
63.00	4139.0
64.00	442.0
65.00	598.0
65.90	125.0
66.90	335.0
68.00	10126.0
69.00	9610.0
70.10	779.0
71.00	93.0
72.00	623.0
73.00	4616.0
74.10	15632.0
75.00	48424.0
76.10	4287.0
76.90	530.0
79.00	3606.0
79.90	1095.0
81.00	3911.0
81.90	875.0
83.10	132.0
87.00	4826.0
87.90	3827.0
91.00	350.0
92.00	2740.0
93.00	4220.0
94.00	11790.0
95.00	92624.0
96.00	6293.0
97.00	222.0
103.80	479.0
104.90	175.0
105.90	458.0
106.80	118.0
109.90	52.0
110.80	167.0
111.80	79.0
113.00	139.0
114.90	111.0
115.90	485.0
117.00	814.0
117.80	349.0
118.90	604.0
123.90	74.0
127.80	268.0
128.90	225.0
130.00	420.0
130.70	148.0
132.80	51.0
134.00	122.0
134.70	183.0
137.00	170.0
141.00	1172.0
141.70	70.0
142.80	1021.0
144.90	292.0
145.80	143.0
147.00	124.0
147.80	315.0
149.00	68.0
149.90	149.0
152.70	79.0
155.00	287.0
156.90	124.0
158.90	116.0
160.90	76.0
172.00	1028.0
174.00	72800.0
175.00	6216.0
176.00	68312.0

Instrument :
MSVOA_W
ClientSampleId :
BFB416

177.00	5199.0
178.00	137.0
191.00	66.0
192.90	70.0
207.00	77.0
249.10	75.0
265.10	72.0
281.10	723.0
282.10	155.0
283.10	170.0

Instrument :
MSVOA_W
ClientSampleId :
BFB416