

Data File : VW011915.D
Acq On : 14 Aug 2019 12:54
Operator : SY/VA
Sample : K4215-14
Misc : 5.01G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Aug 16 05:39:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 16 05:35:58 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	289857	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	263335	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	121365	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	89362	21.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.56%
7) Chloroethane-d5	2.89	69	63215	21.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.00%
10) 1,1-Dichloroethene-d2	4.02	63	149040	15.93	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.72%
20) 2-Butanone-d5	7.08	46	60613	32.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.96%
24) Chloroform-d	7.65	84	161248	20.26	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.04%
26) 1,2-Dichloroethane-d4	8.31	65	98393	20.89	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.56%
29) Benzene-d6	8.27	84	340048	20.53	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.12%
33) 1,2-Dichloropropane-d6	9.27	67	109040	20.40	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.60%
37) Toluene-d8	10.32	98	294916	20.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.28%
38) trans-1,3-Dichloropropene-	10.58	79	43851	18.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.88%
39) 2-Hexanone-d5	10.93	63	40628	32.54	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.08%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	80816	18.20	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	72.80%
61) 1,2-Dichlorobenzene-d4	13.85	152	94365	20.18	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.72%


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	13.56	75	16434	4.774 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011915.D
Acq On : 14 Aug 2019 12:54
Operator : SY/VA
Sample : K4215-14
Misc : 5.01G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Aug 16 05:39:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 16 05:35:58 2019
Response via : Initial Calibration

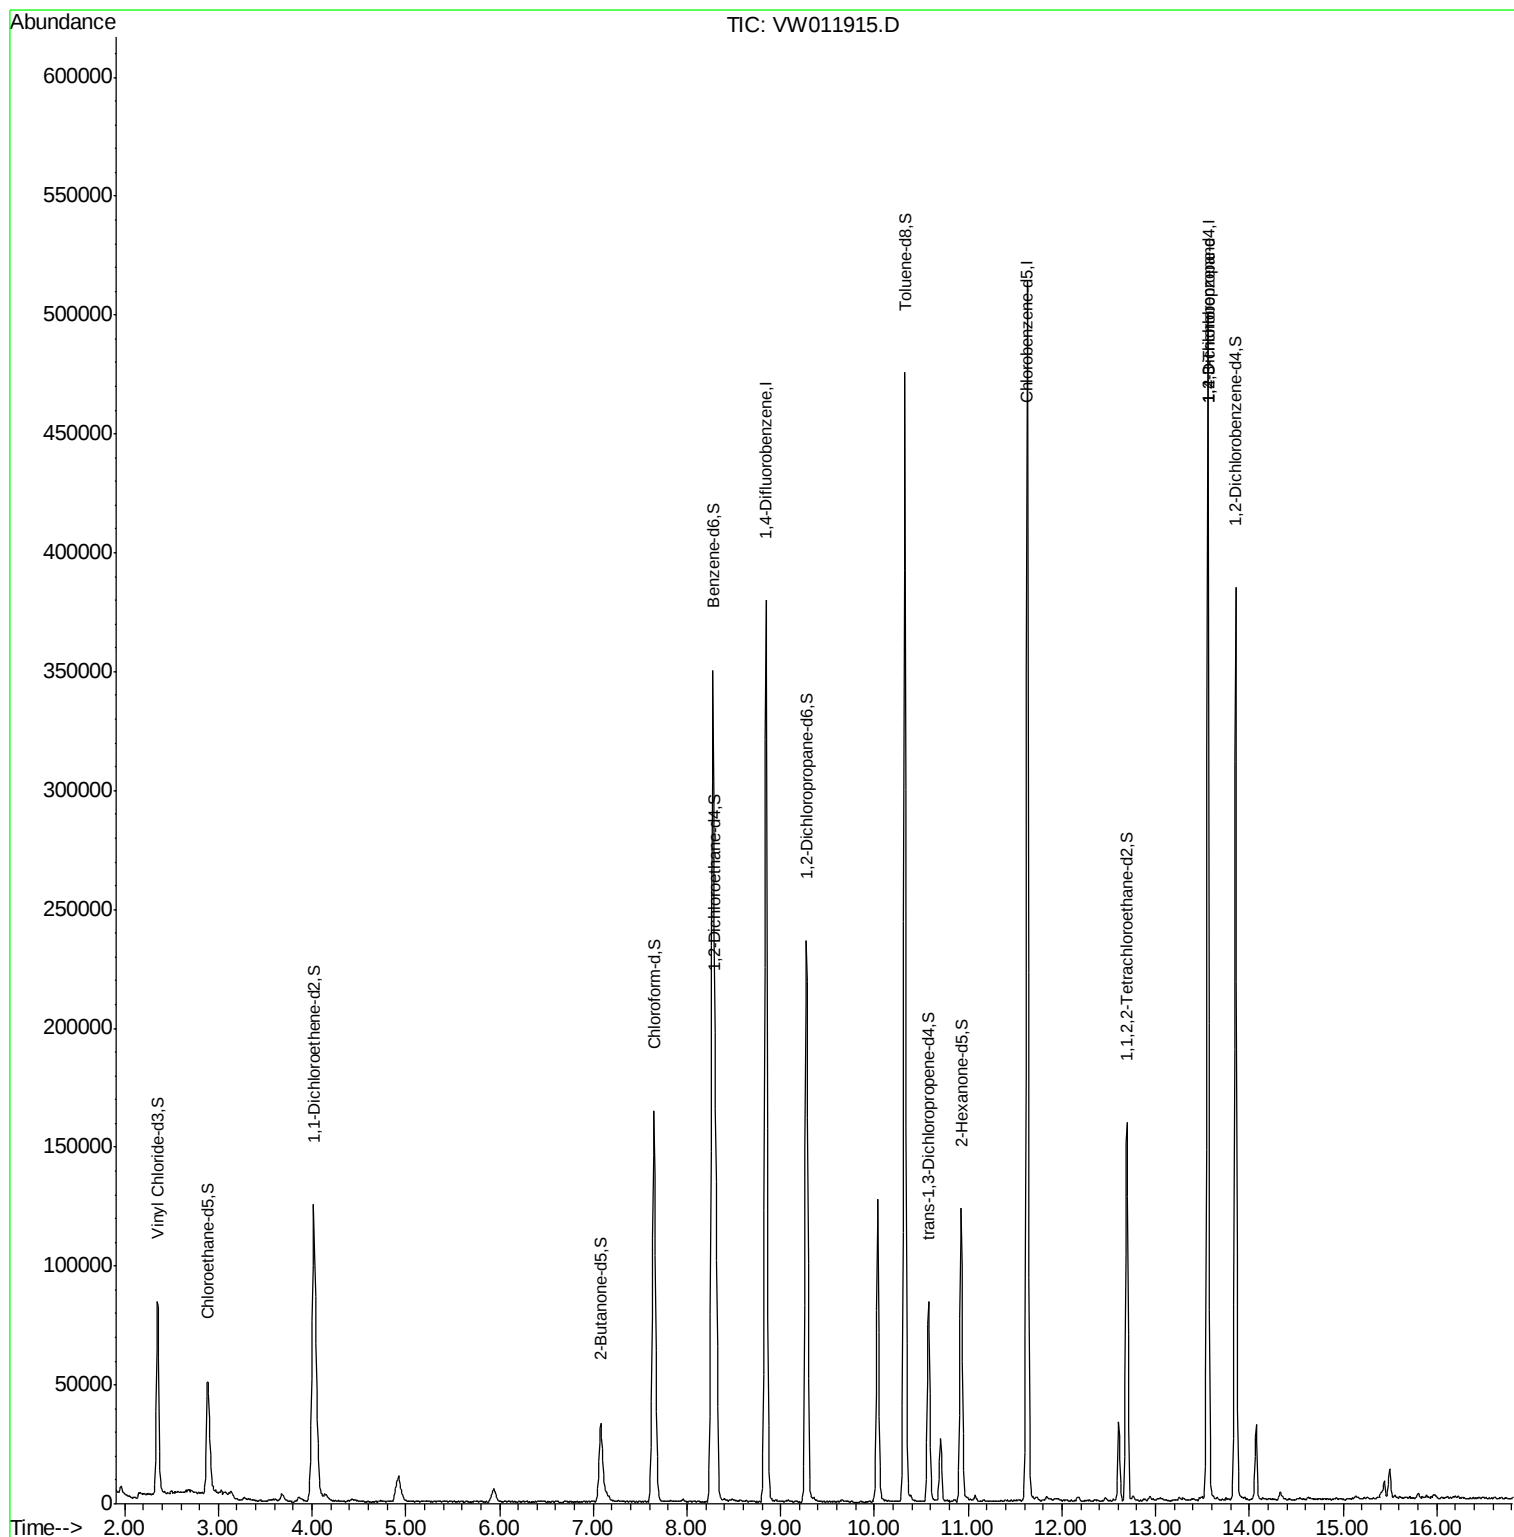

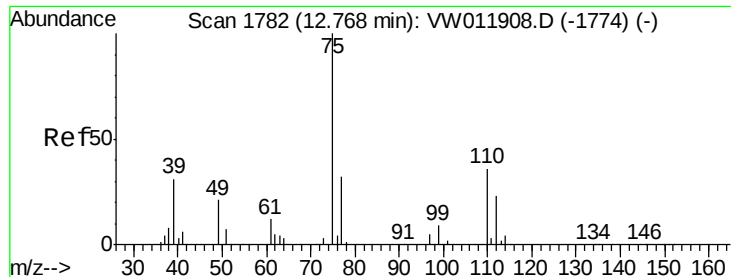

#59

1,2,3-Trichloropropane

Concen: 4.774 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW011915.D

Acq: 14 Aug 2019 12:54

Instrument :

MSVOA_W

ClientSampleId :


VHBLK01

Tgt Ion: 75 Resp: 16434

Ion Ratio Lower Upper

75 100

77 37.4 25.1 37.7

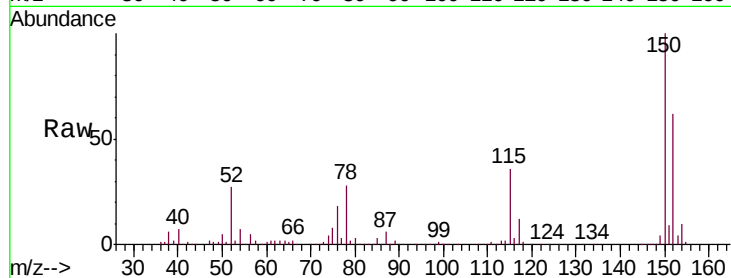

Abundance Ion 75.00 (74.70 to 75.70): VW

Ion 77.00 (76.70 to 77.70): VW

