

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
 Data File : VW024236.D
 Acq On : 15 Aug 2022 15:55
 Operator : SY/VA
 Sample : VW0815SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK576

Quant Time: Aug 16 01:18:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 16 01:17:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.835	114	272054	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	265323	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	132499	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	92000	16.178	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.720%
7) Chloroethane-d5	2.873	69	66576	18.794	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.160%
11) 1,1-Dichloroethene-d2	4.007	63	87092	13.439	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.760%
21) 2-Butanone-d5	7.080	46	54267	51.294	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.580%
24) Chloroform-d	7.647	84	178098	21.636	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.560%
26) 1,2-Dichloroethane-d4	8.299	65	99514	21.775	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.080%
32) Benzene-d6	8.268	84	328977	21.024	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.080%
36) 1,2-Dichloropropane-d6	9.274	67	100812	21.821	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.280%
41) Toluene-d8	10.323	98	289439	19.790	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.160%
43) trans-1,3-Dichloroprop...	10.573	79	39408	19.474	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.880%
47) 2-Hexanone-d5	10.920	63	39205	45.942	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.880%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	106264	23.707	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	121735	25.107	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.440%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.024	75	3764	0.660	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
Data File : VW024236.D
Acq On : 15 Aug 2022 15:55
Operator : SY/VA
Sample : VW0815SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK576

Quant Time: Aug 16 01:18:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 16 01:17:17 2022
Response via : Initial Calibration

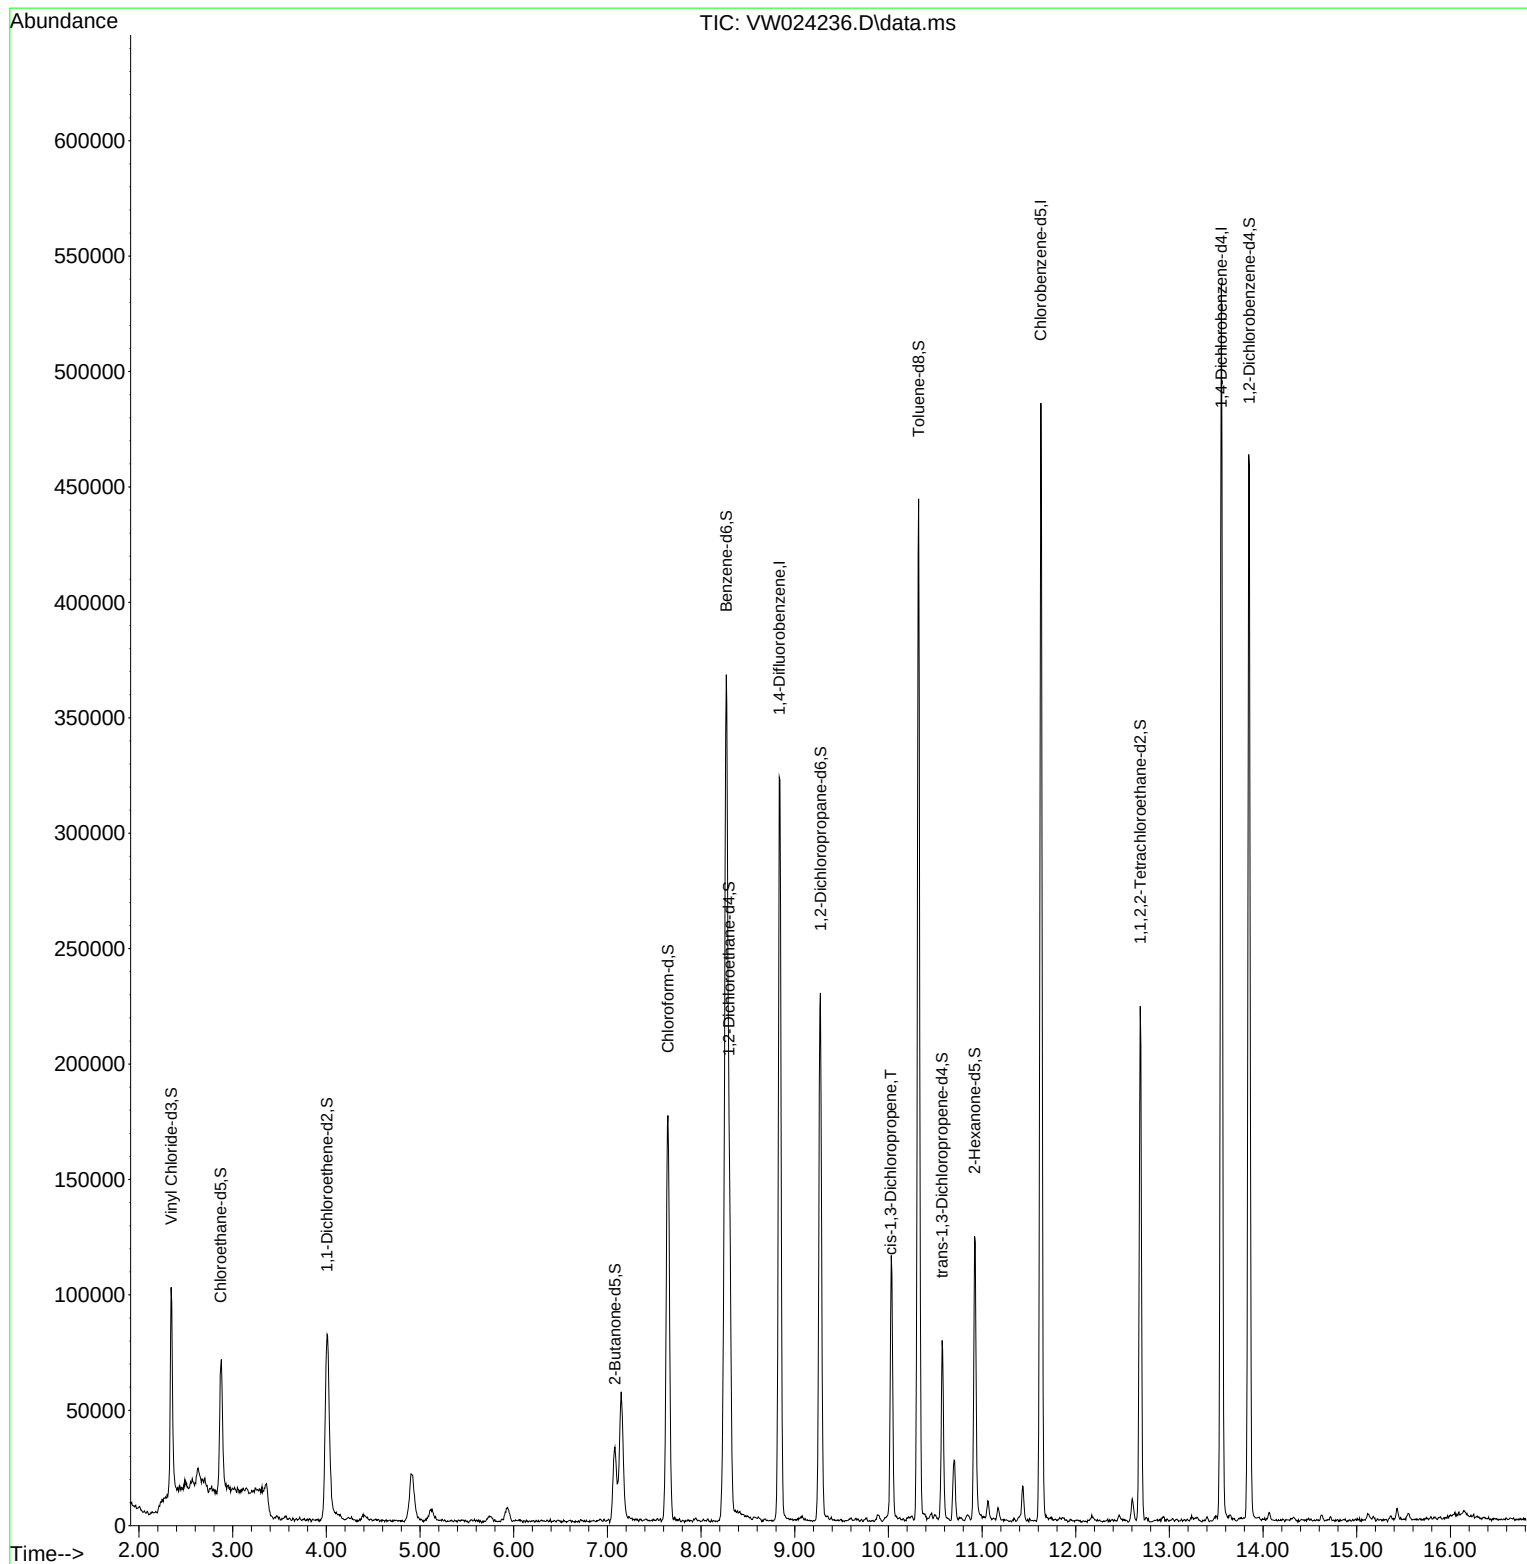

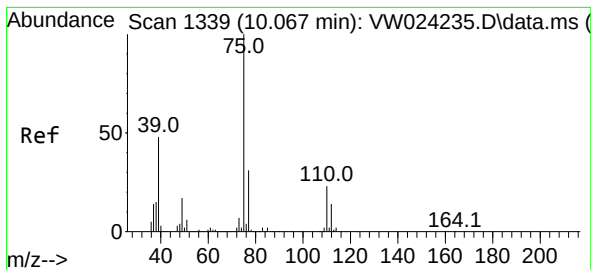

#39

cis-1,3-Dichloropropene

Concen: 0.660 ug/L

RT: 10.024 min Scan# 11

Delta R.T. -0.043 min

Lab File: VW024236.D

Acq: 15 Aug 2022 15:55

Instrument :

MSVOA_W

ClientSampleId :

VBLK576

Tgt Ion: 75 Resp: 3764

Ion Ratio Lower Upper

75 100

77 30.4 23.4 43.6

