




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
 Data File : VW024236.D
 Acq On : 15 Aug 2022 15:55
 Operator : SY/VA
 Sample : VW0815SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK576

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:54:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 16 01:17:17 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/16/2022
 Supervised By :Semsettin Yesilyurt 08/16/2022

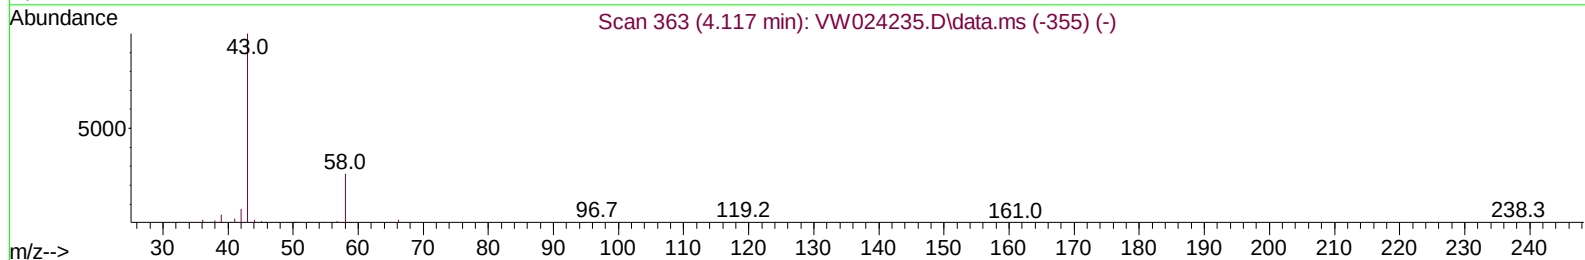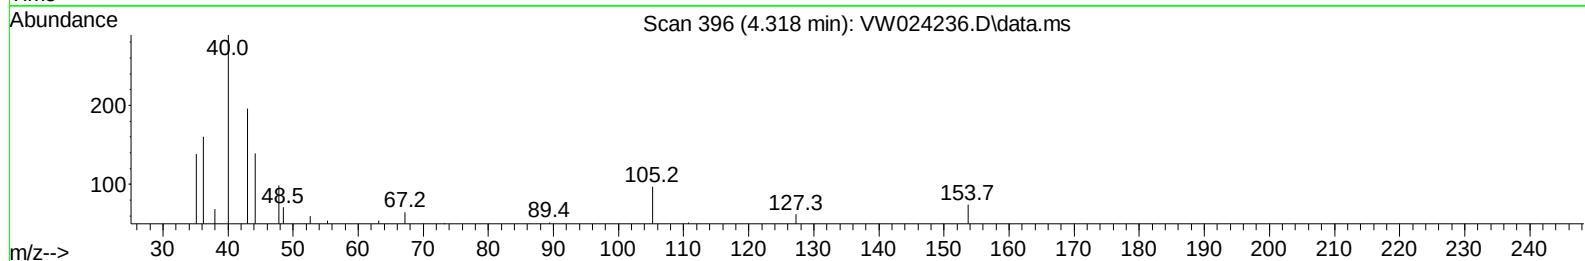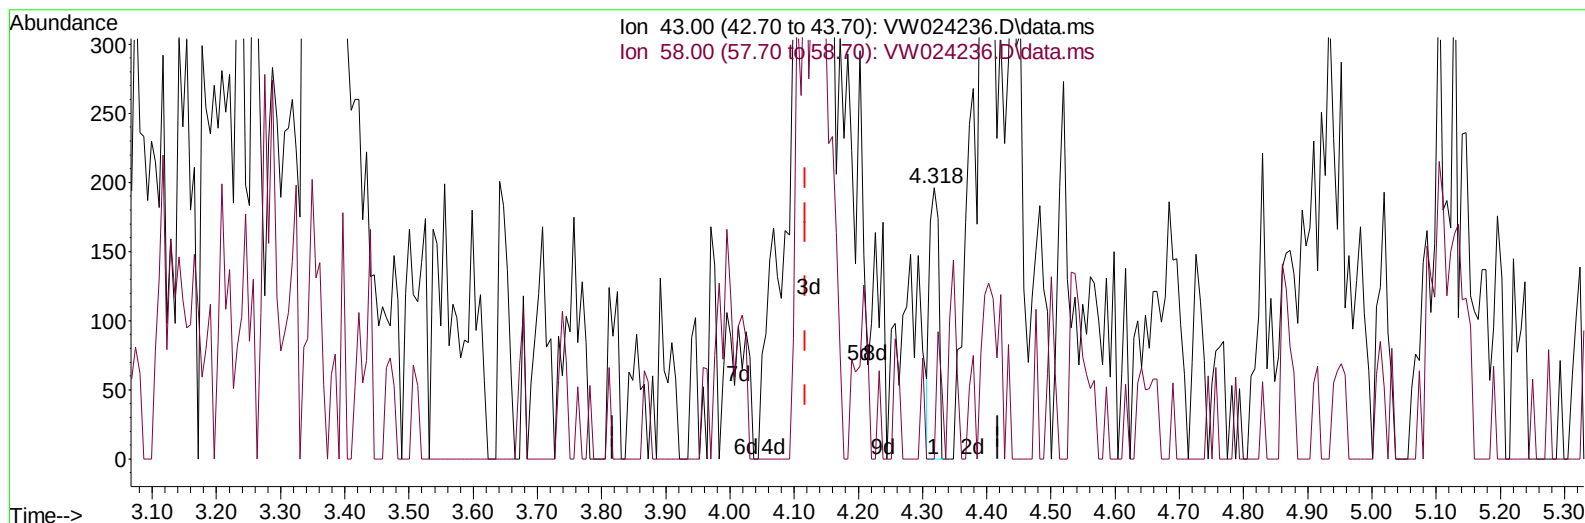

TIC: VW024236.D\data.ms

(13) Acetone (T)

4.318min (+ 0.201) 0.25 ug/L

response 198

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	26.77
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
 Data File : VW024236.D
 Acq On : 15 Aug 2022 15:55
 Operator : SY/VA
 Sample : VW0815SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK576

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/16/2022
 Supervised By :Semsettin Yesilyurt 08/16/2022

Quant Time: Aug 16 01:54:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 16 01:17:17 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.835	114		272054	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		265323	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		132499	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		92000	16.178	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.720%	
7) Chloroethane-d5	2.873	69		66576	18.794	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.160%	
11) 1,1-Dichloroethene-d2	4.007	63		87092	13.439	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.760%	
21) 2-Butanone-d5	7.080	46		54267	51.294	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.580%	
24) Chloroform-d	7.647	84		178098	21.636	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.560%	
26) 1,2-Dichloroethane-d4	8.299	65		99514	21.775	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.080%	
32) Benzene-d6	8.268	84		328977	21.024	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.080%	
36) 1,2-Dichloropropane-d6	9.274	67		100812	21.821	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.280%	
41) Toluene-d8	10.323	98		289439	19.790	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.160%	
43) trans-1,3-Dichloroprop...	10.573	79		39408	19.474	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.880%	
47) 2-Hexanone-d5	10.920	63		39205	45.942	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.880%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		106264	23.707	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.840%	
66) 1,2-Dichlorobenzene-d4	13.853	152		121735	25.107	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.440%	
Target Compounds							
13) Acetone	4.123	43		3321m	4.264	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
Data File : VW024236.D
Acq On : 15 Aug 2022 15:55
Operator : SY/VA
Sample : VW0815SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK576

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/16/2022
Supervised By :Semsettin Yesilyurt 08/16/2022

Quant Time: Aug 16 01:54:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 16 01:17:17 2022
Response via : Initial Calibration

