




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
Data File : VW024237.D
Acq On : 15 Aug 2022 16:30
Operator : SY/VA
Sample : N4210-01
Misc : 4.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC46

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/16/2022
Supervised By :Semsettin Yesilyurt 08/16/2022

Quant Time: Aug 16 01:18:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 16 01:17:17 2022
Response via : Initial Calibration

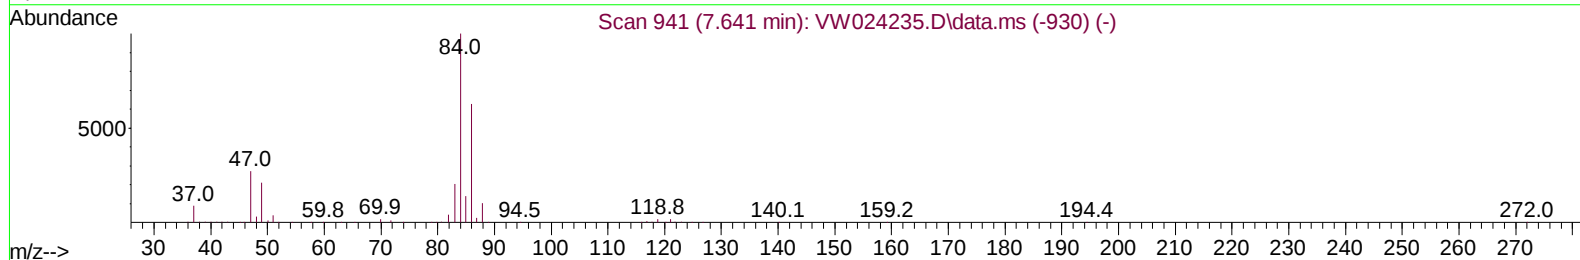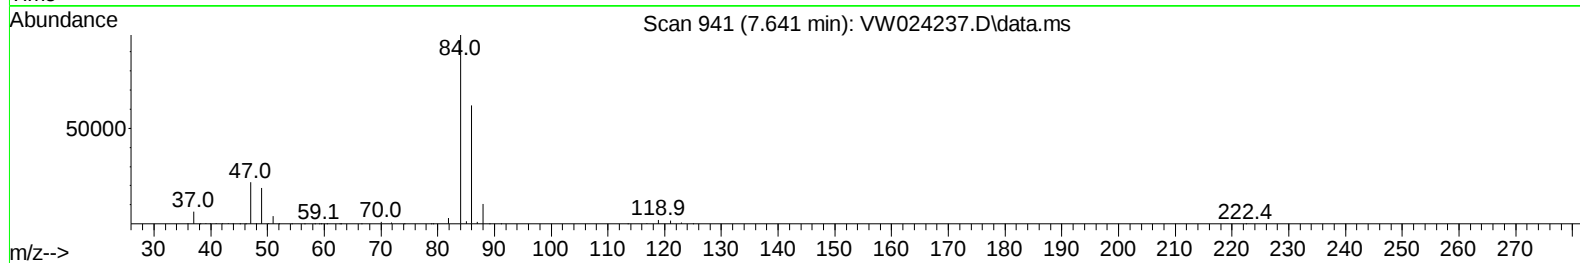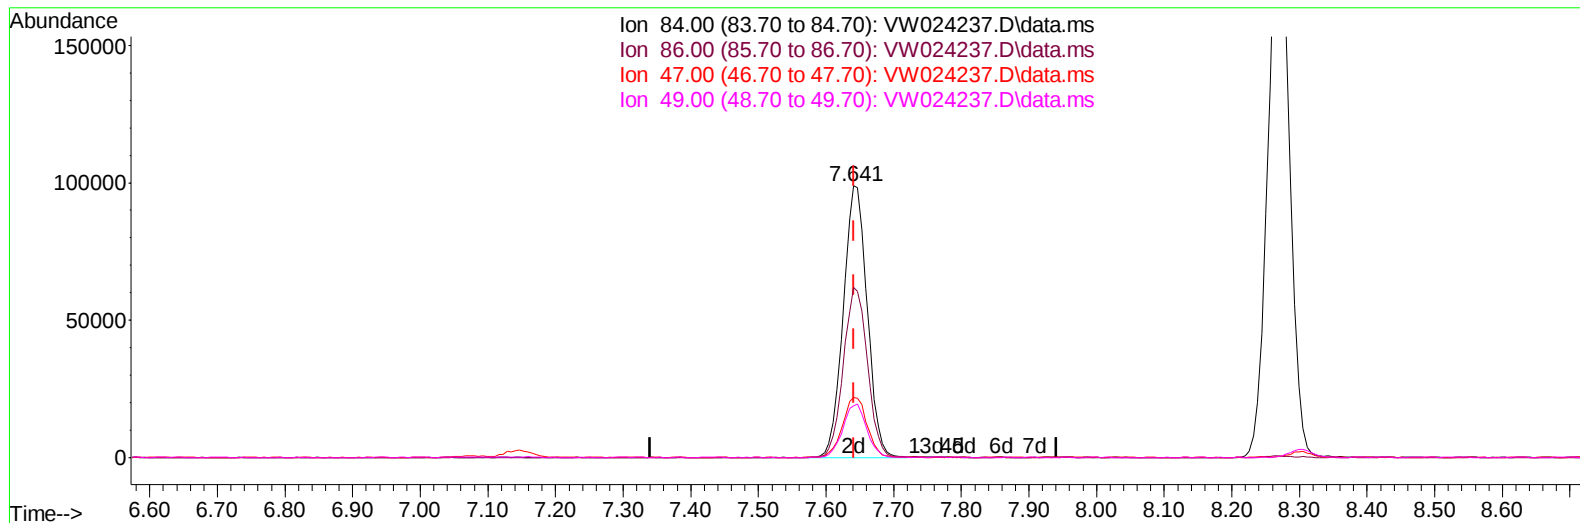

TIC: VW024237.D\data.ms

(24) Chloroform-d (S)

7.641min (-0.000) 22.79 ug/L m

response 243318

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.20	0.06#
47.00	43.20	0.03#
49.00	26.90	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
 Data File : VW024237.D
 Acq On : 15 Aug 2022 16:30
 Operator : SY/VA
 Sample : N4210-01
 Misc : 4.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC46

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:18:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 16 01:17:17 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/16/2022
 Supervised By :Semsettin Yesilyurt 08/16/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		352844	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		312086	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		131363	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		154997	21.016	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	84.080%		
7) Chloroethane-d5	2.873	69		108834	23.688	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	94.760%		
11) 1,1-Dichloroethene-d2	4.007	63		139530	16.600	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	66.400%		
21) 2-Butanone-d5	7.074	46		52316	38.127	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	76.260%		
24) Chloroform-d	7.641	84		243318m	22.791	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	91.160%		
26) 1,2-Dichloroethane-d4	8.299	65		135078	22.789	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	91.160%		
32) Benzene-d6	8.269	84		452758	24.599	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	98.400%		
36) 1,2-Dichloropropane-d6	9.268	67		137320	25.269	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	101.080%		
41) Toluene-d8	10.317	98		396254	23.033	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	92.120%		
43) trans-1,3-Dichloroprop...	10.573	79		53950	22.666	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	90.680%		
47) 2-Hexanone-d5	10.921	63		42457	42.298	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	84.600%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		122377	23.211	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	92.840%		
66) 1,2-Dichlorobenzene-d4	13.853	152		117346	24.411	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	97.640%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
Data File : VW024237.D
Acq On : 15 Aug 2022 16:30
Operator : SY/VA
Sample : N4210-01
Misc : 4.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC46

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/16/2022
Supervised By :Semsettin Yesilyurt 08/16/2022

Quant Time: Aug 16 01:18:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 16 01:17:17 2022
Response via : Initial Calibration

