




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
 Data File : VW024239.D
 Acq On : 15 Aug 2022 17:19
 Operator : SY/VA
 Sample : N4210-07
 Misc : 5.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC50

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:18:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 16 01:17:17 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/16/2022
 Supervised By :Semsettin Yesilyurt 08/16/2022

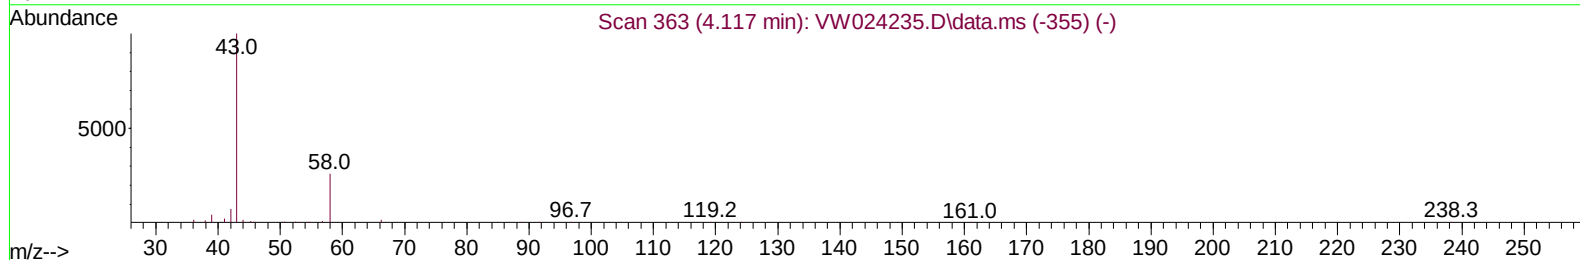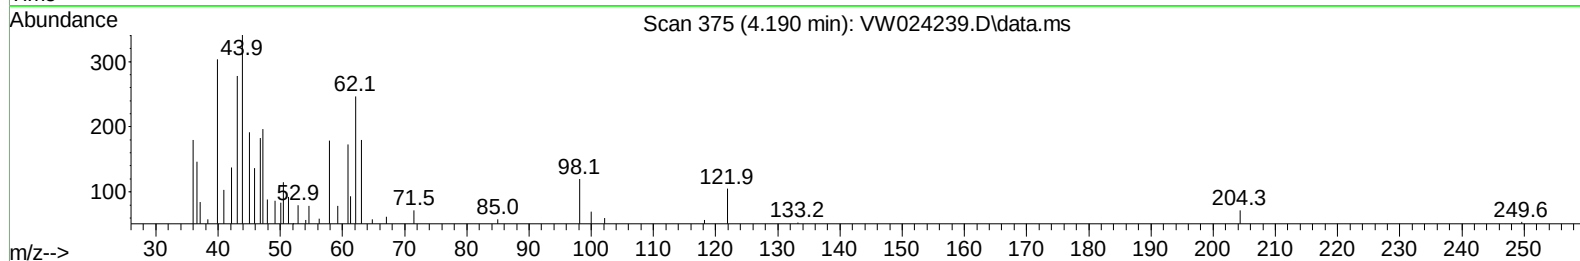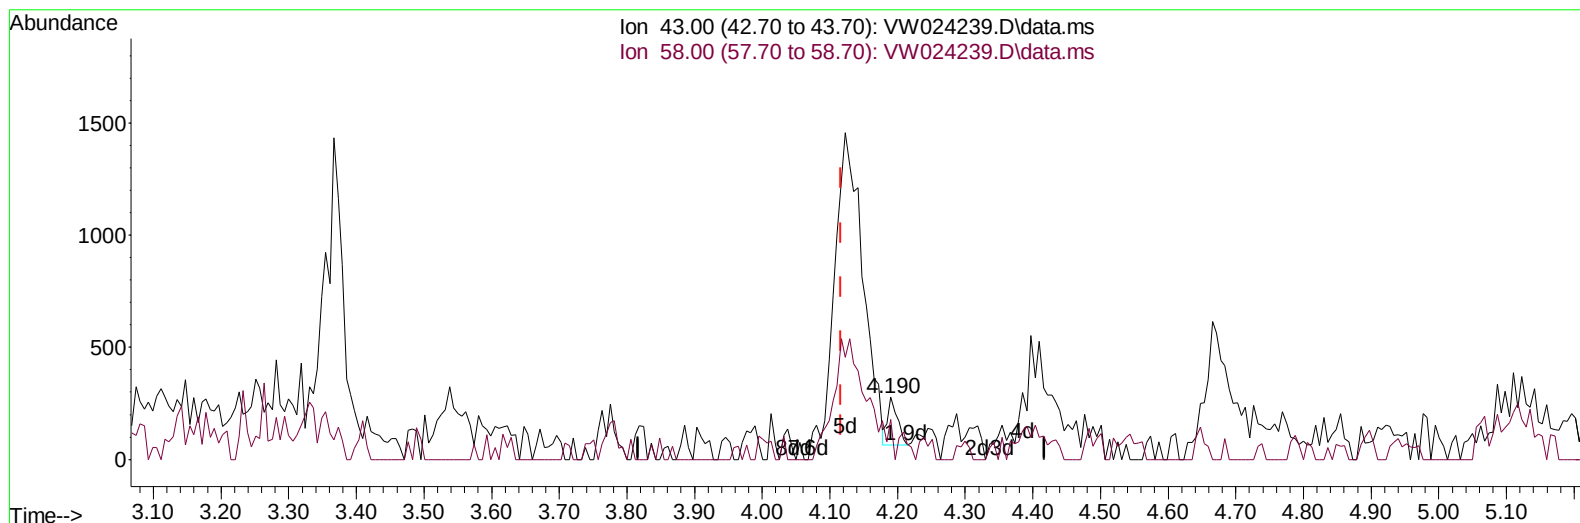

TIC: VW024239.D\data.ms

(13) Acetone (T)

4.190min (+ 0.073) 0.31 ug/L

response 211

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	30.81
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
 Data File : VW024239.D
 Acq On : 15 Aug 2022 17:19
 Operator : SY/VA
 Sample : N4210-07
 Misc : 5.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC50

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:18:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 16 01:17:17 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/16/2022
 Supervised By :Semsettin Yesilyurt 08/16/2022

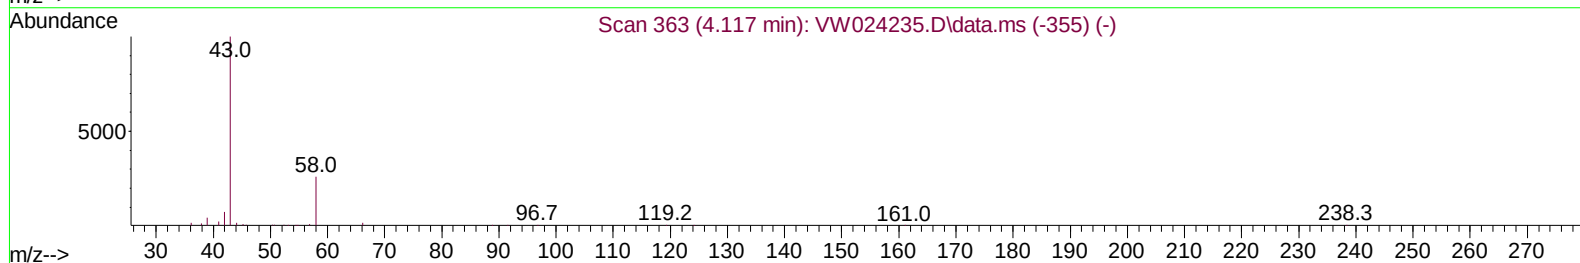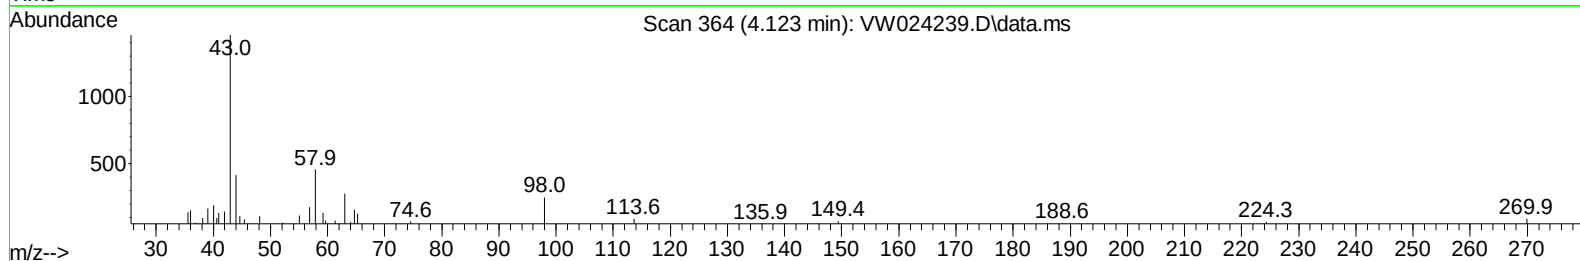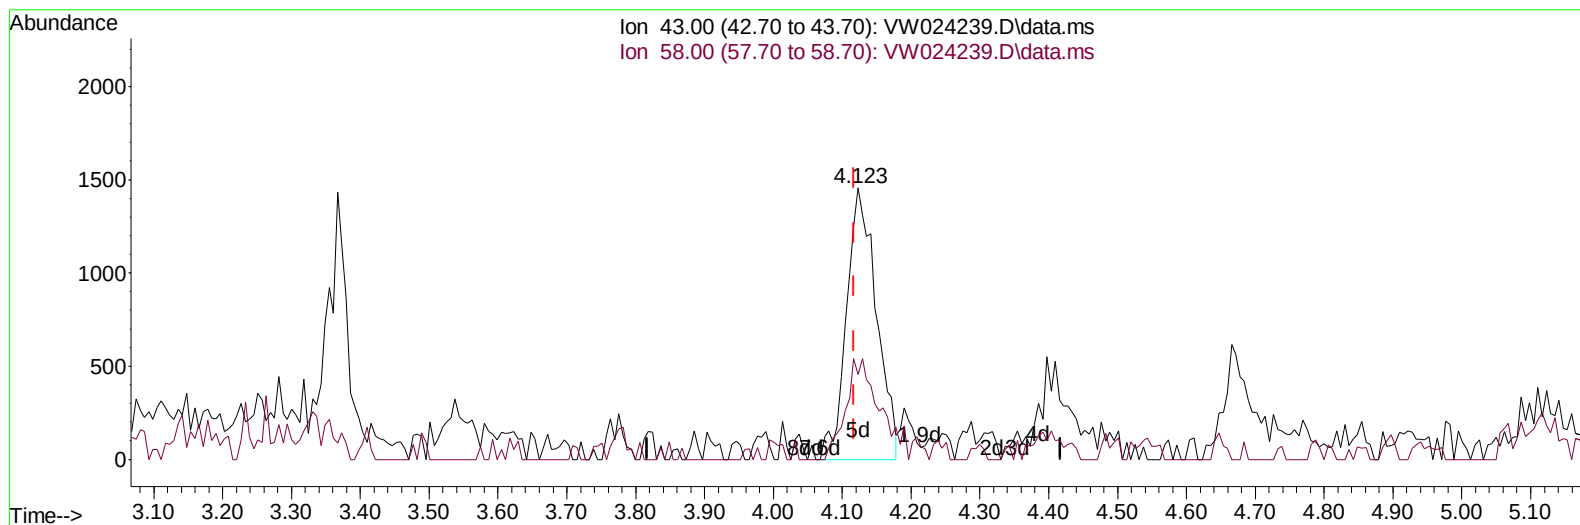

TIC: VW024239.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 6.54 ug/L m

response 4387

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	1.48
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
 Data File : VW024239.D
 Acq On : 15 Aug 2022 17:19
 Operator : SY/VA
 Sample : N4210-07
 Misc : 5.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC50

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:18:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 16 01:17:17 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/16/2022
 Supervised By :Semsettin Yesilyurt 08/16/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		234224	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		200599	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		68574	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		137622	28.110	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	112.440%	
7) Chloroethane-d5	2.873	69		82777	27.141	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	108.560%	
11) 1,1-Dichloroethene-d2	4.007	63		94152	16.874	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	67.480%	
21) 2-Butanone-d5	7.080	46		34390	37.756	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	75.520%	
24) Chloroform-d	7.647	84		173355	24.461	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	97.840%	
26) 1,2-Dichloroethane-d4	8.305	65		104604	26.585	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	106.360%	
32) Benzene-d6	8.275	84		320120	27.059	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	108.240%	
36) 1,2-Dichloropropane-d6	9.274	67		98329	28.150	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	112.600%	
41) Toluene-d8	10.323	98		271773	24.577	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	98.320%	
43) trans-1,3-Dichloroprop...	10.579	79		33036	21.593	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	86.360%	
47) 2-Hexanone-d5	10.921	63		26209	40.623	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	81.240%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		91191	26.908	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	107.640%	
66) 1,2-Dichlorobenzene-d4	13.853	152		61514	24.514	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	98.040%	
Target Compounds							
13) Acetone	4.123	43		4387m	6.542	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
Data File : VW024239.D
Acq On : 15 Aug 2022 17:19
Operator : SY/VA
Sample : N4210-07
Misc : 5.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC50

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:18:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 16 01:17:17 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/16/2022
Supervised By :Semsettin Yesilyurt 08/16/2022

