




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
Data File : VW024240.D
Acq On : 15 Aug 2022 17:43
Operator : SY/VA
Sample : N4210-08
Misc : 5.86g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC51

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:18:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 16 01:17:17 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/16/2022
Supervised By :Semsettin Yesilyurt 08/16/2022

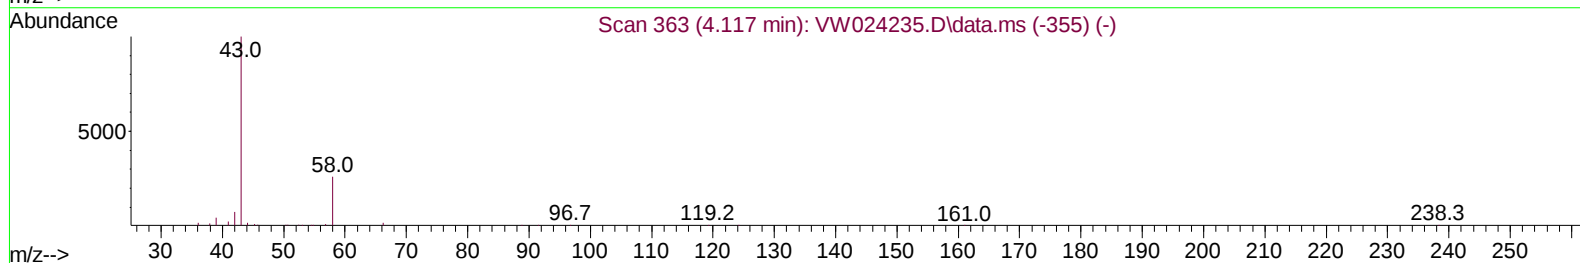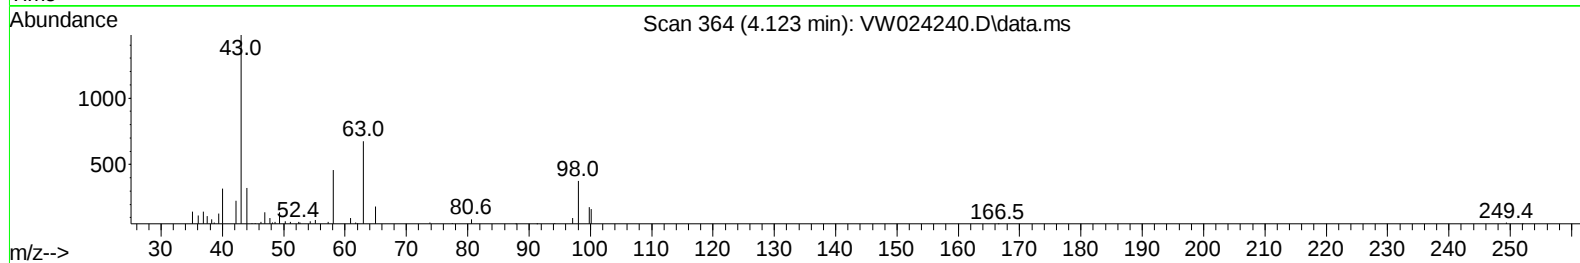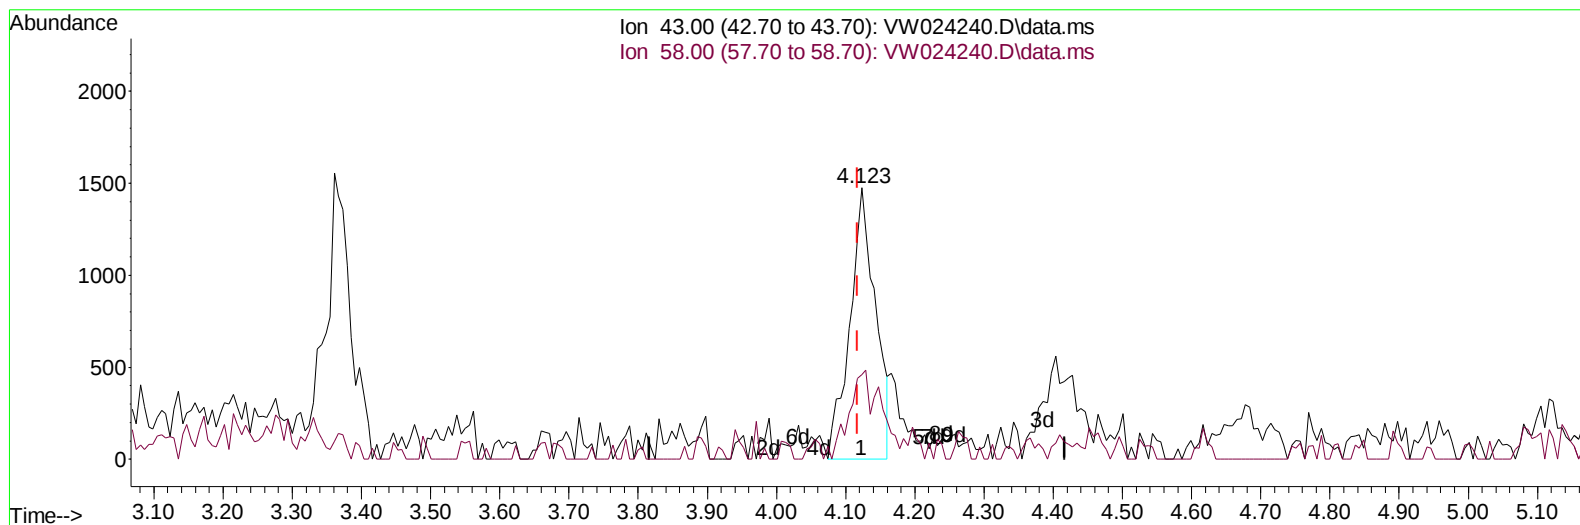

TIC: VW024240.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 4.61 ug/L

response 3785

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	21.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
Data File : VW024240.D
Acq On : 15 Aug 2022 17:43
Operator : SY/VA
Sample : N4210-08
Misc : 5.86g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC51

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:18:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 16 01:17:17 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/16/2022
Supervised By :Semsettin Yesilyurt 08/16/2022

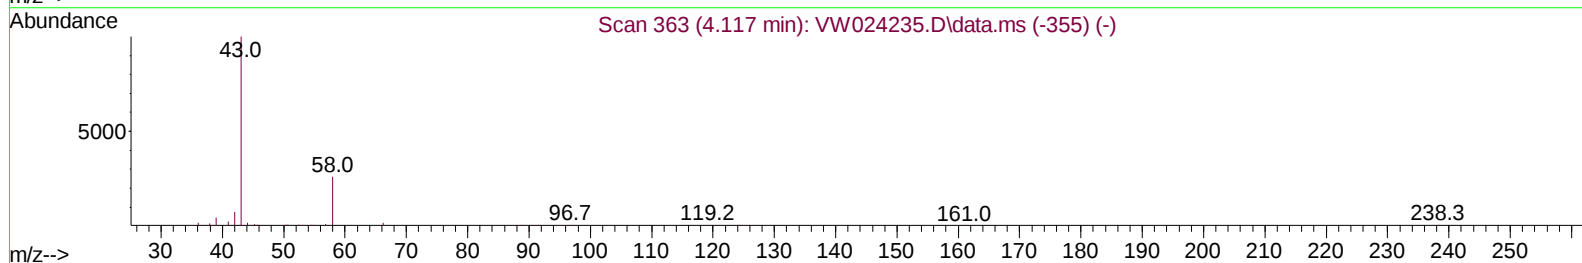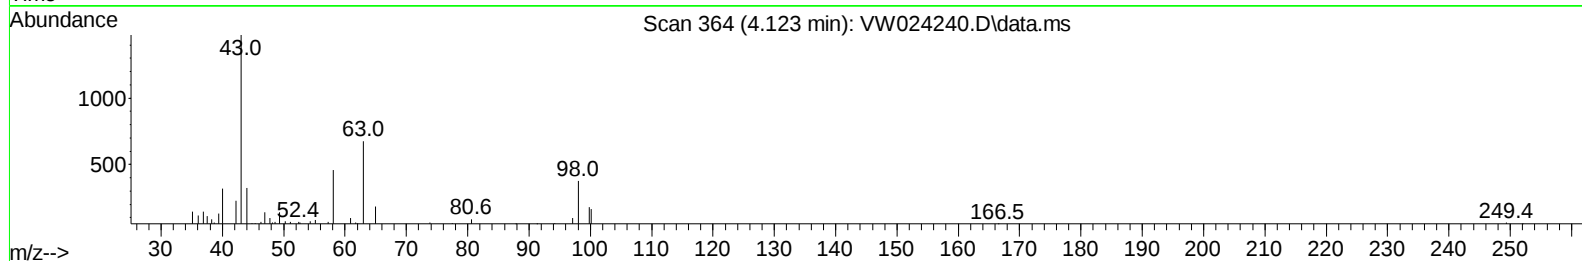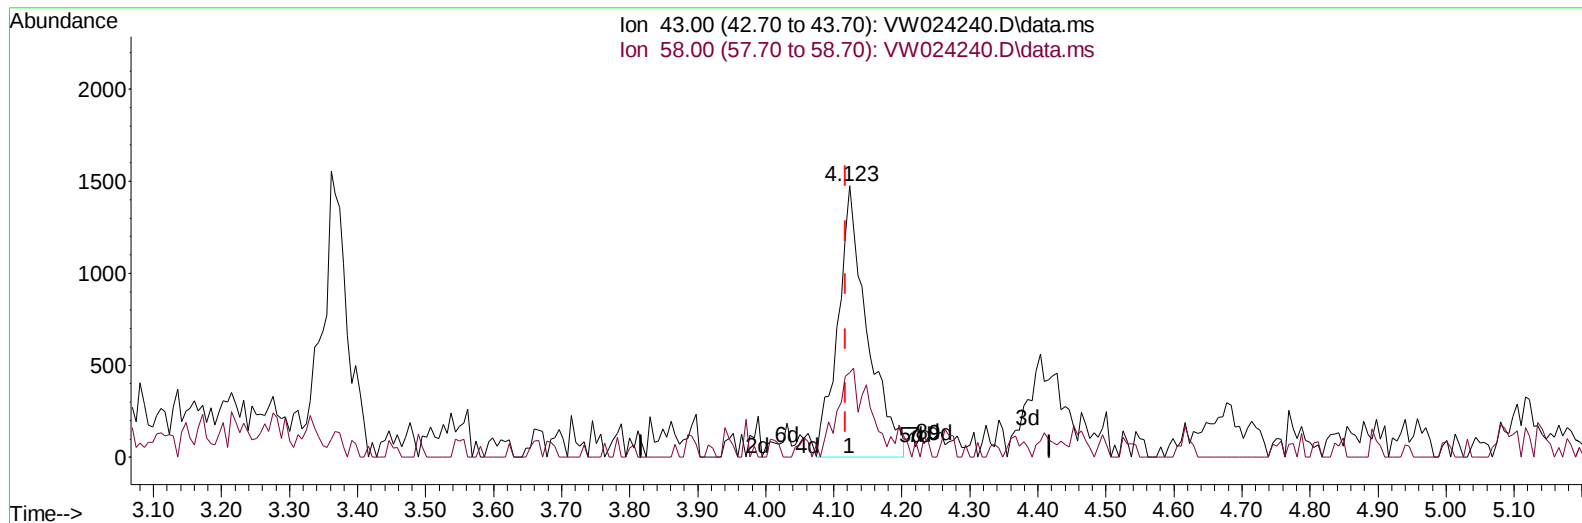

TIC: VW024240.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 5.38 ug/L m

response 4418

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	18.06
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
 Data File : VW024240.D
 Acq On : 15 Aug 2022 17:43
 Operator : SY/VA
 Sample : N4210-08
 Misc : 5.86g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC51

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:18:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 16 01:17:17 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/16/2022
 Supervised By :Semsettin Yesilyurt 08/16/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		286822	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		252995	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		87703	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		171167	28.550	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	114.200%		
7) Chloroethane-d5	2.873	69		111022	29.727	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	118.920%		
11) 1,1-Dichloroethene-d2	4.001	63		112436	16.456	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	65.840%		
21) 2-Butanone-d5	7.080	46		40844	36.618	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	73.240%		
24) Chloroform-d	7.647	84		215398	24.820	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	99.280%		
26) 1,2-Dichloroethane-d4	8.305	65		125528	26.053	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	104.200%		
32) Benzene-d6	8.269	84		403284	27.029	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	108.120%		
36) 1,2-Dichloropropane-d6	9.268	67		122285	27.758	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	111.040%		
41) Toluene-d8	10.323	98		351159	25.179	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	100.720%		
43) trans-1,3-Dichloroprop...	10.573	79		41963	21.747	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	87.000%		
47) 2-Hexanone-d5	10.921	63		32699	40.185	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	80.380%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		107626	25.181	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	100.720%		
66) 1,2-Dichlorobenzene-d4	13.853	152		87828	27.366	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	109.480%		
Target Compounds							
13) Acetone	4.123	43		4418m	5.380	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
Data File : VW024240.D
Acq On : 15 Aug 2022 17:43
Operator : SY/VA
Sample : N4210-08
Misc : 5.86g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC51

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:18:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 16 01:17:17 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/16/2022
Supervised By :Semsettin Yesilyurt 08/16/2022

