

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
 Data File : VW024243.D
 Acq On : 15 Aug 2022 18:57
 Operator : SY/VA
 Sample : N4210-06
 Misc : 5.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC49

Quant Time: Aug 16 01:19:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 16 01:17:17 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.841	114	292402	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.627	117	240827	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	70222	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.336	65	156844	25.662	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 102.640%		
7) Chloroethane-d5		2.873	69	99474	26.127	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 104.520%		
11) 1,1-Dichloroethene-d2		4.007	63	115561	16.590	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 66.360%		
21) 2-Butanone-d5		7.073	46	43187	37.980	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 75.960%		
24) Chloroform-d		7.646	84	222491	25.148	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 100.600%		
26) 1,2-Dichloroethane-d4		8.305	65	127508	25.958	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 103.840%		
32) Benzene-d6		8.274	84	392653	27.646	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 110.600%		
36) 1,2-Dichloropropane-d6		9.268	67	129631	30.912	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 123.640%#		
41) Toluene-d8		10.323	98	321091	24.187	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 96.760%		
43) trans-1,3-Dichloroprop...		10.579	79	40557	22.081	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 88.320%		
47) 2-Hexanone-d5		10.920	63	33218	42.886	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 85.780%		
56) 1,1,2,2-Tetrachloroeth...		12.688	84	119512	29.374	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 117.480%		
66) 1,2-Dichlorobenzene-d4		13.847	152	73355	28.546	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 114.200%		
Target Compounds							Qvalue
13) Acetone		4.123	43	4669	5.577	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
Data File : VW024243.D
Acq On : 15 Aug 2022 18:57
Operator : SY/VA
Sample : N4210-06
Misc : 5.77g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC49

Quant Time: Aug 16 01:19:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 16 01:17:17 2022
Response via : Initial Calibration

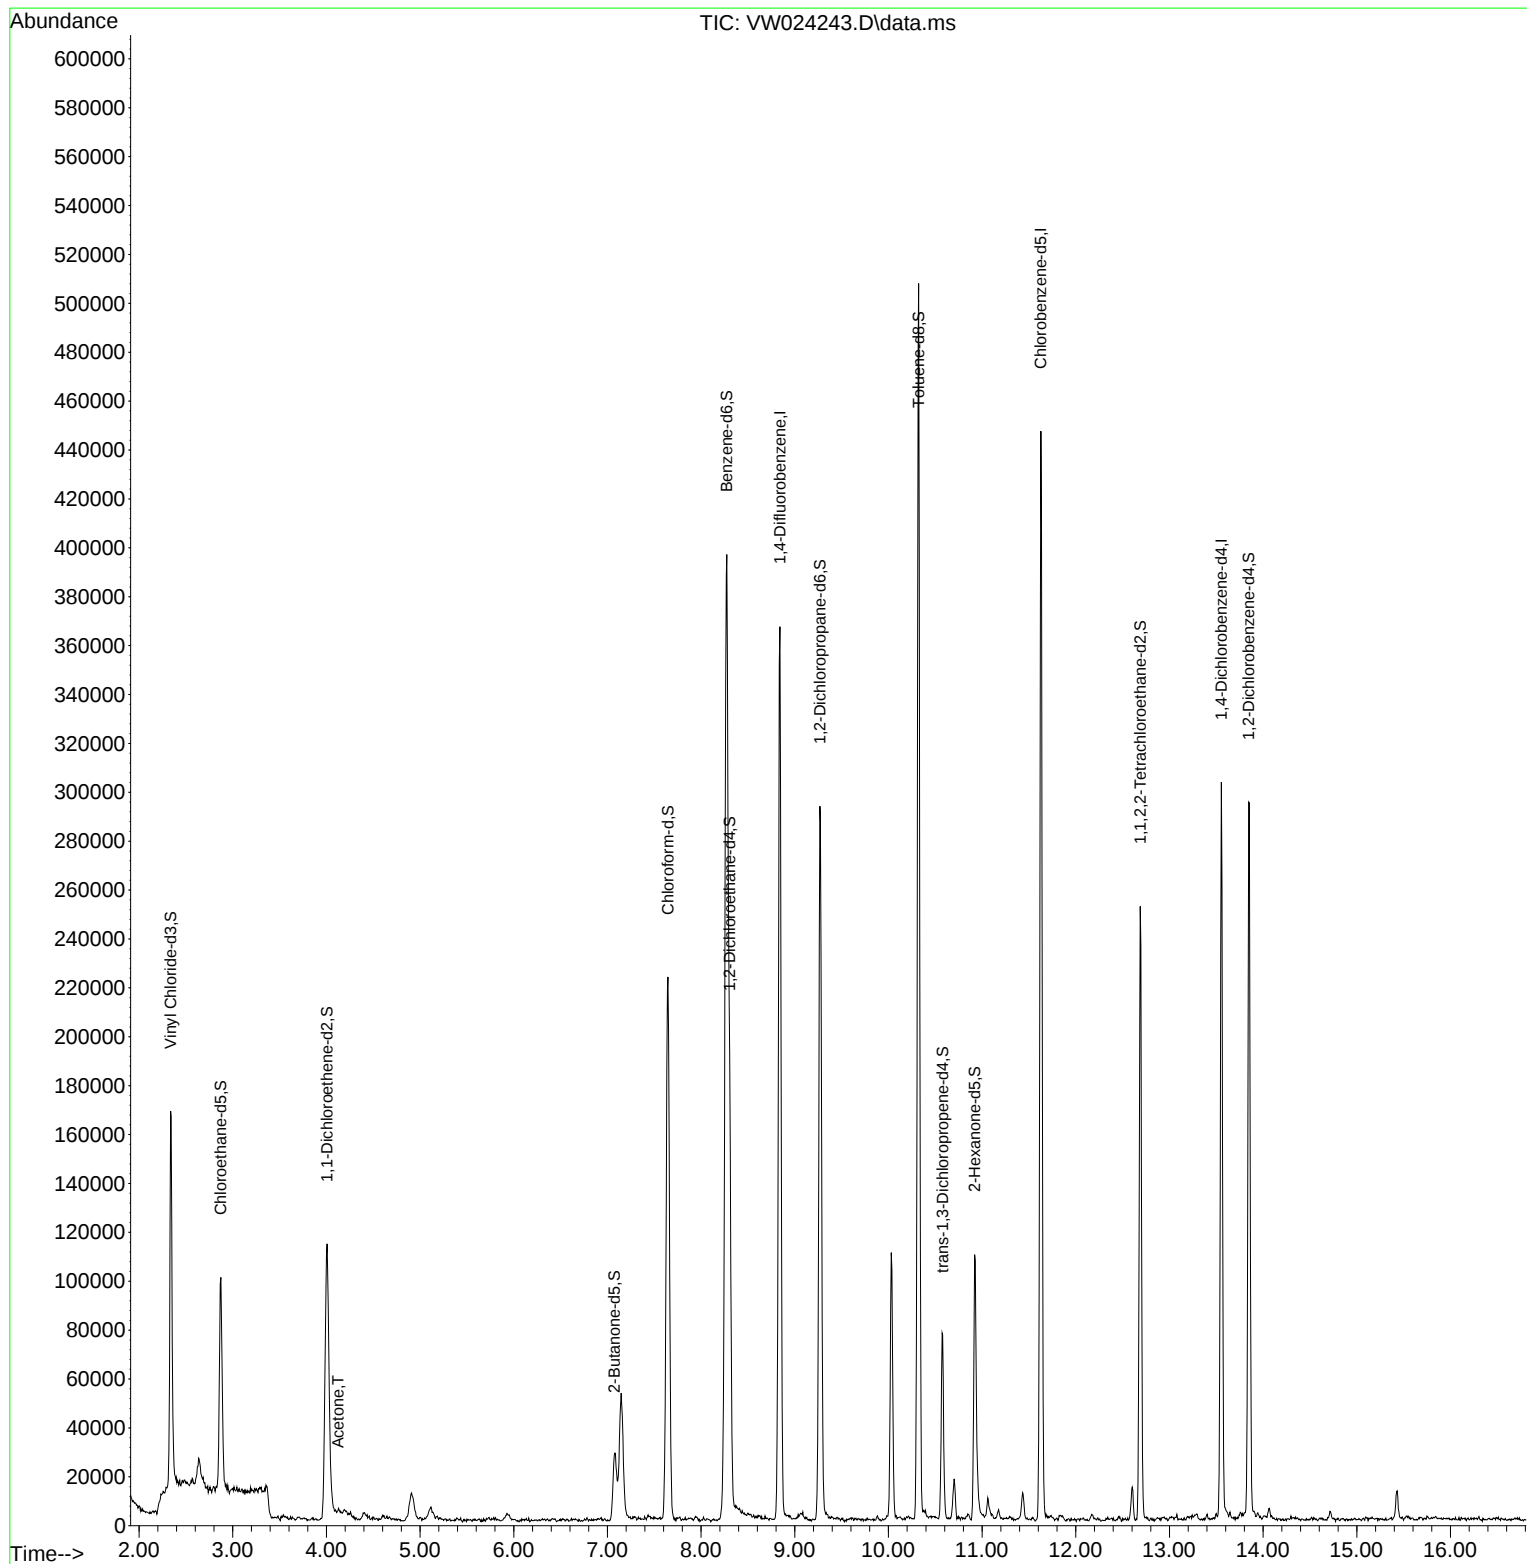

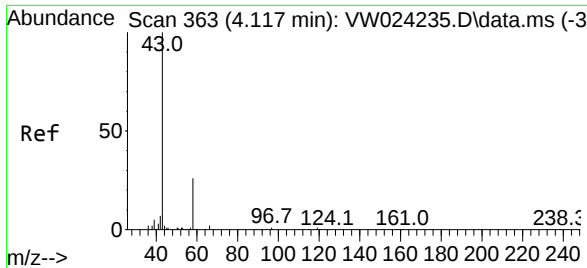

#13
 Acetone
 Concen: 5.577 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW024243.D
 Acq: 15 Aug 2022 18:57

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC49

Tgt Ion: 43 Resp: 4669
 Ion Ratio Lower Upper
 43 100
 58 25.3 0.0 31.8

