
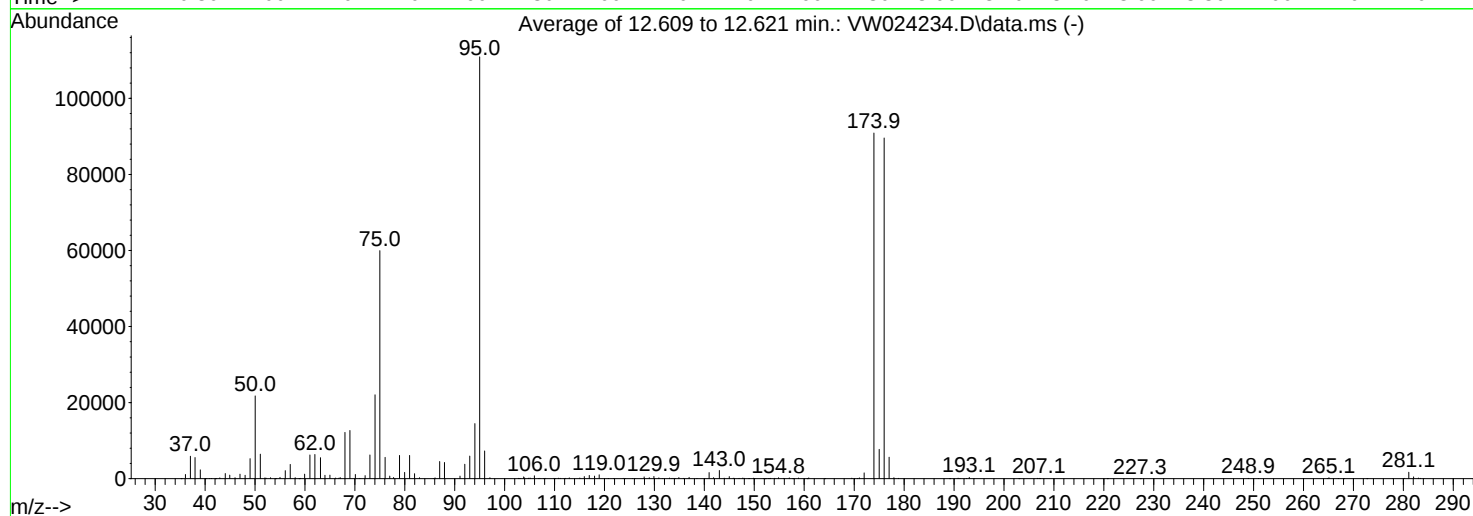


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081522\
 Data File : VW024234.D
 Acq On : 15 Aug 2022 11:39
 Operator : SY/VA
 Sample : BFB409
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB409

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Title : SFAM01.0
 Last Update : Tue Aug 16 01:17:17 2022

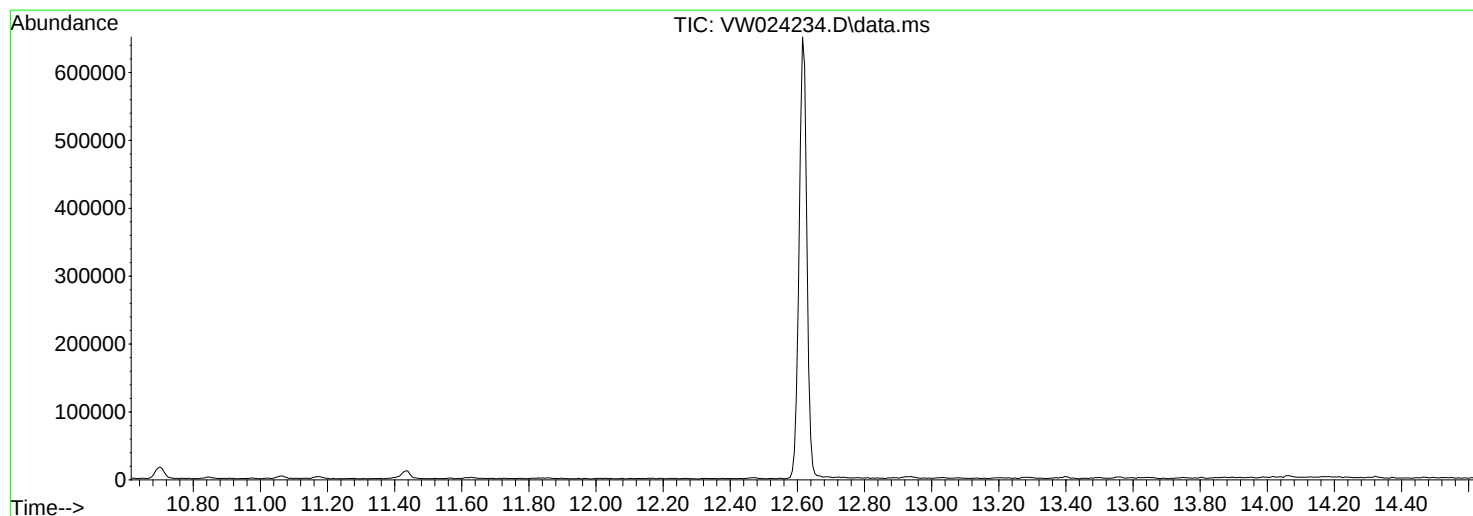

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	21747	PASS
75	95	30	80	54.1	59957	PASS
95	95	100	100	100.0	110925	PASS
96	95	5	9	6.6	7267	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.9	90893	PASS
175	174	5	9	8.5	7692	PASS
176	174	95	105	98.6	89587	PASS
177	176	5	10	6.3	5635	PASS

m/z	Abundance
36.40	77.0
37.90	66.0
38.80	170.0
40.00	312.0
42.00	66.0
42.70	87.0
43.80	297.0
44.80	87.0
47.00	125.0
49.30	52.0
53.40	57.0
55.00	79.0
61.10	69.0
68.80	60.0
73.50	56.0
150.60	53.0
269.80	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB409

m/z	Abundance
35.20	50.0
36.00	1054.0
37.10	5835.0
38.00	5369.0
39.00	2175.0
40.10	410.0
41.30	113.0
42.20	82.0
43.00	255.0
44.10	1219.0
45.00	854.0
46.10	192.0
47.10	1127.0
48.00	1038.0
49.00	5228.0
50.00	20208.0
51.00	6164.0
52.00	387.0
53.20	263.0
54.90	369.0
56.10	1976.0
57.00	3169.0
58.10	281.0
59.00	115.0
60.00	1187.0
61.00	5377.0
62.00	5345.0
63.10	5209.0
64.10	960.0
65.00	949.0
66.30	156.0
68.00	10464.0
69.00	11372.0
70.10	925.0
71.00	121.0
72.00	773.0
73.00	5312.0
74.10	19720.0
75.00	52376.0
76.10	5300.0
77.10	620.0
77.80	318.0
78.90	5691.0
79.90	1590.0
81.00	5848.0
81.90	1330.0
83.00	284.0
86.10	204.0
87.00	4103.0
88.00	3698.0
91.00	566.0
92.00	2965.0
93.00	5090.0
94.00	12537.0
95.00	96464.0
96.00	6385.0
97.00	261.0
102.70	86.0
103.10	107.0
103.80	661.0
104.70	201.0
105.10	228.0
106.00	644.0
106.80	80.0
108.10	146.0
110.20	139.0
110.70	224.0
112.20	75.0
113.00	193.0
115.00	101.0
116.00	493.0
117.00	656.0
118.10	534.0
119.00	846.0
120.80	81.0
121.90	59.0
124.20	55.0
125.60	79.0
126.10	114.0
128.00	422.0
129.10	261.0
129.90	586.0
131.00	146.0
133.00	198.0
133.50	243.0
134.20	69.0
134.90	193.0
135.80	87.0
137.00	341.0
138.50	76.0
141.00	1095.0
141.90	267.0

Instrument :
MSVOA_W
ClientSampleId :
BFB409

143.00	1930.0
144.00	75.0
145.10	563.0
145.80	221.0
146.90	112.0
148.00	282.0
148.90	95.0
150.10	179.0
152.20	57.0
153.20	115.0
154.90	211.0
156.00	93.0
157.10	172.0
158.80	115.0
160.60	67.0
161.10	83.0
169.60	120.0
170.10	127.0
170.70	181.0
172.00	1637.0
174.00	72624.0
175.00	6142.0
176.00	66504.0
177.00	4333.0
177.90	286.0
178.90	123.0
190.80	388.0
193.10	569.0
194.00	147.0
203.00	61.0
206.70	115.0
207.10	141.0
249.00	154.0
251.00	104.0
265.20	321.0
267.00	79.0
272.70	58.0
280.10	73.0
281.20	2532.0
282.10	770.0
283.00	362.0
284.10	85.0

Instrument :
MSVOA_W
ClientSampleId :
BFB409

m/z	Abundance
36.10	1307.0
37.00	6052.0
38.10	6659.0
39.10	2612.0
40.20	191.0
40.90	131.0
42.30	55.0
43.00	143.0
44.00	1434.0
45.00	1158.0
45.90	312.0
47.10	1619.0
48.00	972.0
49.00	5677.0
50.10	24048.0
51.00	7266.0
52.20	450.0
53.20	179.0
54.10	50.0
55.00	479.0
56.00	2120.0
57.00	4453.0
58.00	171.0
59.10	162.0
60.00	1267.0
61.00	7408.0
62.00	6639.0
63.10	6219.0
64.00	787.0
65.10	1053.0
66.10	211.0
66.80	349.0
67.10	414.0
68.00	13847.0
69.00	13795.0
70.10	1277.0
71.00	181.0
72.10	871.0
73.00	7070.0
74.00	25680.0
75.00	67728.0
76.00	6383.0
76.90	754.0
77.70	384.0
79.00	6841.0
80.00	1769.0
80.90	7164.0
82.00	1388.0
83.00	288.0
86.00	261.0
87.00	5204.0
87.90	4873.0
91.10	785.0
92.00	4502.0
93.00	6502.0
94.10	15855.0
95.00	125824.0
96.00	8164.0
97.00	258.0
102.80	127.0
103.80	706.0
105.10	301.0
106.00	884.0
107.00	124.0
107.80	94.0
109.80	160.0
110.80	174.0
112.10	158.0
113.00	174.0
114.90	145.0
115.80	571.0
116.90	1003.0
118.00	583.0
118.90	996.0
121.80	74.0
123.80	180.0
125.70	75.0
128.00	432.0
128.90	247.0
129.90	555.0
130.90	332.0
131.70	75.0
133.10	299.0
134.10	94.0
135.00	391.0
135.80	59.0
137.00	310.0
138.50	77.0
140.90	1891.0
141.90	246.0
143.00	2261.0
143.90	169.0

Instrument :
MSVOA_W
ClientSampleId :
BFB409

144.90	512.0
145.80	211.0
147.70	254.0
149.10	91.0
149.80	170.0
151.80	106.0
152.80	78.0
153.30	131.0
154.10	100.0
154.80	285.0
155.90	86.0
157.00	268.0
157.70	59.0
158.90	273.0
160.90	205.0
164.10	59.0
169.60	123.0
171.10	459.0
172.00	1621.0
173.90	95504.0
175.00	8325.0
176.00	98760.0
177.00	6471.0
178.00	199.0
178.90	88.0
189.10	54.0
191.20	132.0
193.00	344.0
206.80	129.0
207.30	104.0
220.70	55.0
227.30	65.0
248.90	153.0
251.00	50.0
265.00	317.0
268.00	51.0
277.90	147.0
280.20	80.0
281.00	1730.0
282.00	411.0
283.40	267.0
284.10	74.0

Instrument :
MSVOA_W
ClientSampleId :
BFB409

m/z	Abundance
36.00	958.0
37.00	5770.0
38.10	4890.0
39.00	2214.0
40.00	340.0
42.10	88.0
42.90	261.0
44.00	1359.0
45.00	1101.0
46.00	267.0
47.00	1170.0
48.10	662.0
49.00	4907.0
50.00	20984.0
51.10	5927.0
52.00	279.0
53.00	276.0
55.10	408.0
56.00	2230.0
57.10	3562.0
58.00	273.0
58.80	66.0
59.90	1077.0
61.00	6143.0
62.00	7073.0
63.10	5070.0
63.90	930.0
64.90	828.0
66.10	163.0
67.00	475.0
68.00	12201.0
69.00	12858.0
70.10	1057.0
72.00	765.0
73.00	6283.0
74.10	20744.0
75.00	59768.0
76.00	5067.0
77.00	651.0
77.80	251.0
78.90	5757.0
79.90	1602.0
80.90	5297.0
82.00	1238.0
82.90	213.0
85.70	96.0
86.10	130.0
87.00	4268.0
88.00	4226.0
91.10	679.0
92.00	3890.0
93.00	6203.0
94.10	15028.0
95.00	110488.0
96.00	7252.0
97.10	238.0
102.90	136.0
104.00	618.0
104.80	217.0
105.90	776.0
107.10	146.0
108.10	141.0
109.90	150.0
111.10	219.0
111.90	174.0
112.90	224.0
115.10	275.0
116.00	543.0
117.00	921.0
117.90	869.0
119.00	1146.0
121.90	67.0
123.70	91.0
124.10	121.0
127.90	595.0
128.90	302.0
129.90	639.0
130.80	199.0
133.00	77.0
133.90	271.0
134.80	261.0
135.80	119.0
136.90	347.0
140.90	1875.0
141.70	210.0
143.00	2278.0
143.80	100.0
144.10	84.0
145.00	552.0
146.00	207.0
147.00	148.0
147.70	240.0

Instrument :
MSVOA_W
ClientSampleId :
BFB409

149.00	77.0
149.90	243.0
153.00	87.0
154.10	118.0
154.80	299.0
155.80	56.0
156.90	189.0
158.90	169.0
160.90	307.0
169.50	96.0
171.00	232.0
172.00	1360.0
174.00	104552.0
175.00	8608.0
176.00	103496.0
177.00	6101.0
178.00	232.0
192.50	130.0
192.90	110.0
207.00	139.0
264.80	125.0
265.20	133.0
280.20	51.0
281.10	821.0
282.10	191.0
283.00	121.0

Instrument :
MSVOA_W
ClientSampleId :
BFB409