




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
Data File : VW029921.D
Acq On : 16 Aug 2024 11:12
Operator : SY/MD
Sample : P3504-10
Misc : 5.76g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYC8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/19/2024
Supervised By :Mahesh Dadoda 08/19/2024

Quant Time: Aug 17 00:34:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 17 00:33:10 2024
Response via : Initial Calibration

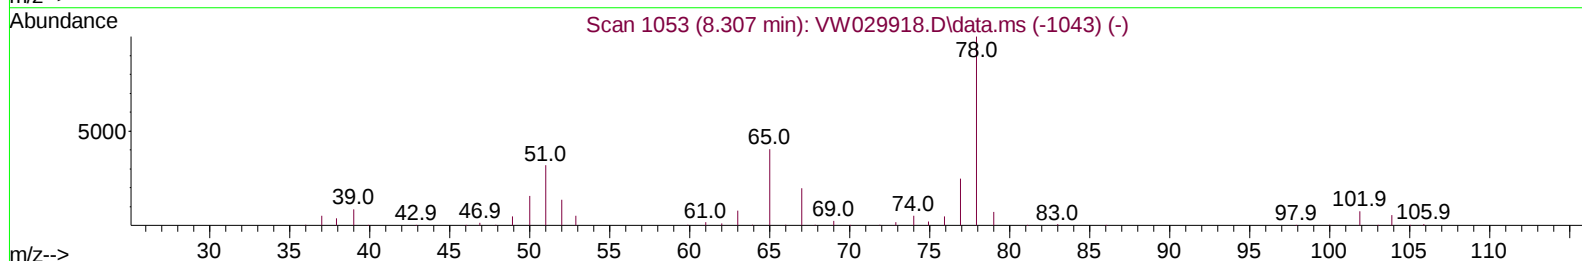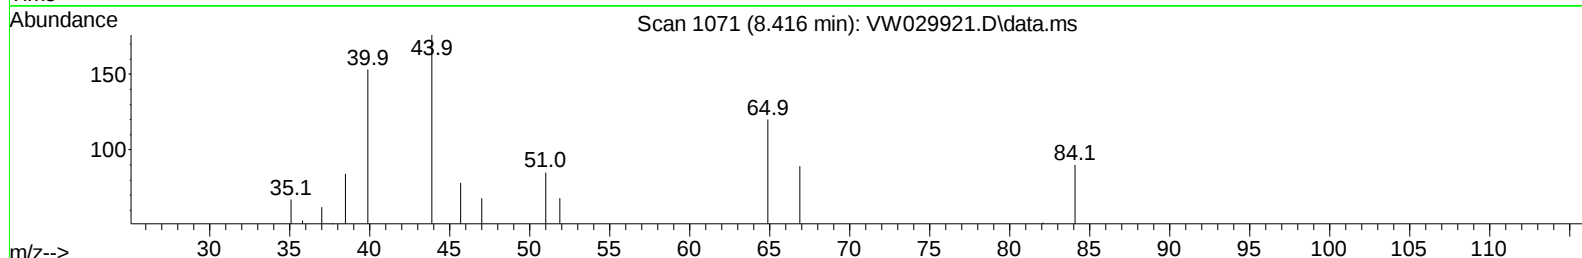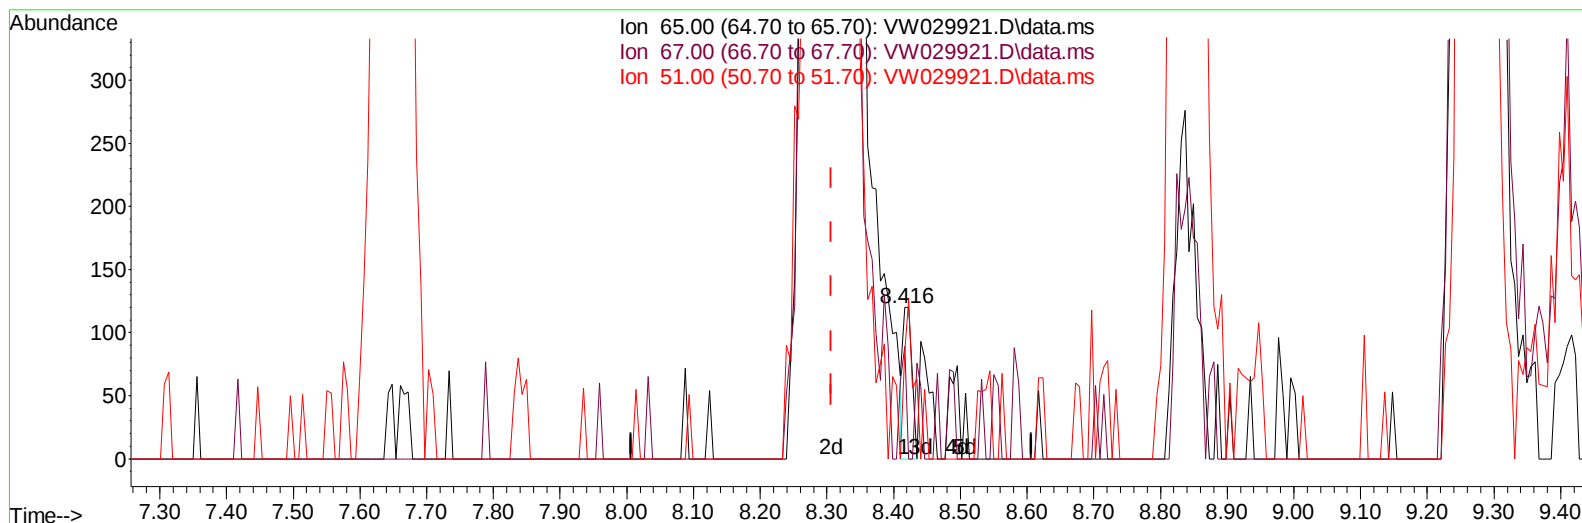

TIC: VW029921.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.416min (+ 0.110) 0.02 ug/L

response 112

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	49.11
51.00	120.50	108.04
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
 Data File : VW029921.D
 Acq On : 16 Aug 2024 11:12
 Operator : SY/MD
 Sample : P3504-10
 Misc : 5.76g/10mL/MSVOA_W/SoIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYC8

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:34:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 17 00:33:10 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
 Supervised By :Mahesh Dadoda 08/19/2024

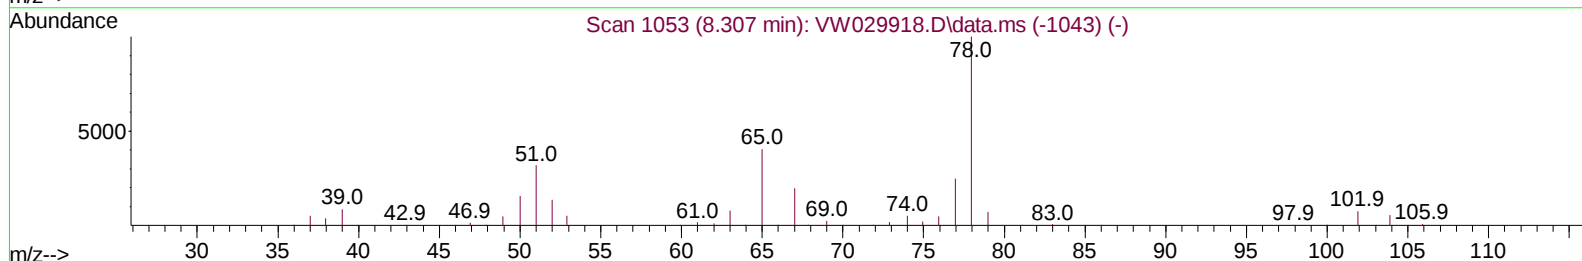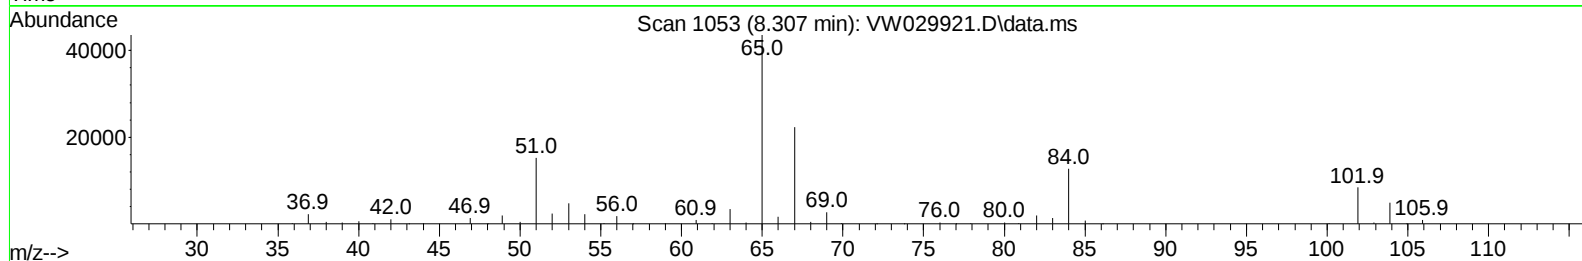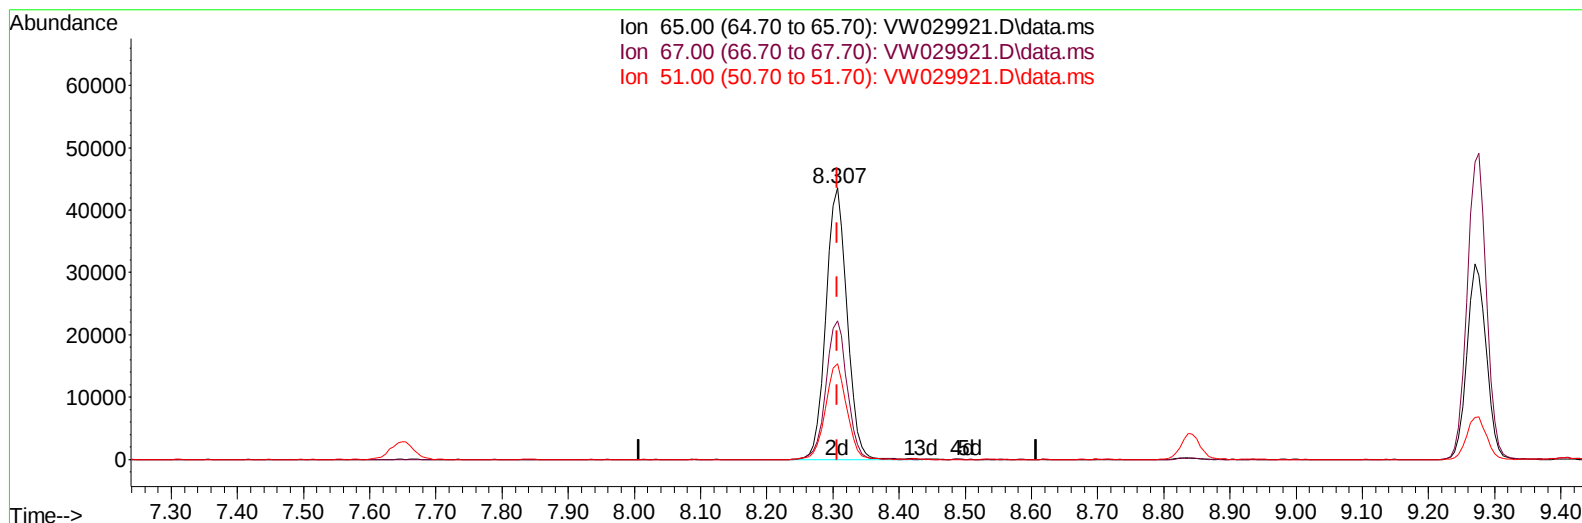

TIC: VW029921.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 18.18 ug/L m

response 96453

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.06#
51.00	120.50	0.13#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
 Data File : VW029921.D
 Acq On : 16 Aug 2024 11:12
 Operator : SY/MD
 Sample : P3504-10
 Misc : 5.76g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYC8

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:34:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 17 00:33:10 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
 Supervised By :Mahesh Dadoda 08/19/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		359799	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		324801	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		148321	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		76115	14.901	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	59.600%	
7) Chloroethane-d5	2.899	69		66287	18.177	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	72.720%	
11) 1,1-Dichloroethene-d2	4.021	65		33555	14.391	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	57.560%	
21) 2-Butanone-d5	7.081	46		39338	28.098	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	56.200%	
24) Chloroform-d	7.648	84		169975	18.249	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	73.000%	
26) 1,2-Dichloroethane-d4	8.307	65		96453m	18.181	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	72.720%	
32) Benzene-d6	8.276	84		305365	17.400	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	69.600%	
36) 1,2-Dichloropropane-d6	9.276	67		98684	17.611	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	70.440%	
41) Toluene-d8	10.325	98		283835	18.189	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	72.760%	
43) trans-1,3-Dichloroprop...	10.575	79		38397	16.934	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	67.720%	
47) 2-Hexanone-d5	10.922	63		31579	34.176	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	68.360%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		82950	19.936	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	79.760%	
66) 1,2-Dichlorobenzene-d4	13.848	152		87161	18.926	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	75.720%	
Target Compounds							
13) Acetone	4.131	43		24128	13.868	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
Data File : VW029921.D
Acq On : 16 Aug 2024 11:12
Operator : SY/MD
Sample : P3504-10
Misc : 5.76g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYC8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/19/2024
Supervised By :Mahesh Dadoda 08/19/2024

Quant Time: Aug 17 00:34:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 17 00:33:10 2024
Response via : Initial Calibration

