




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
 Data File : VW029934.D
 Acq On : 16 Aug 2024 16:24
 Operator : SY/MD
 Sample : P3504-21
 Misc : 5.86g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYA2

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:37:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 17 00:33:10 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
 Supervised By :Mahesh Dadoda 08/19/2024

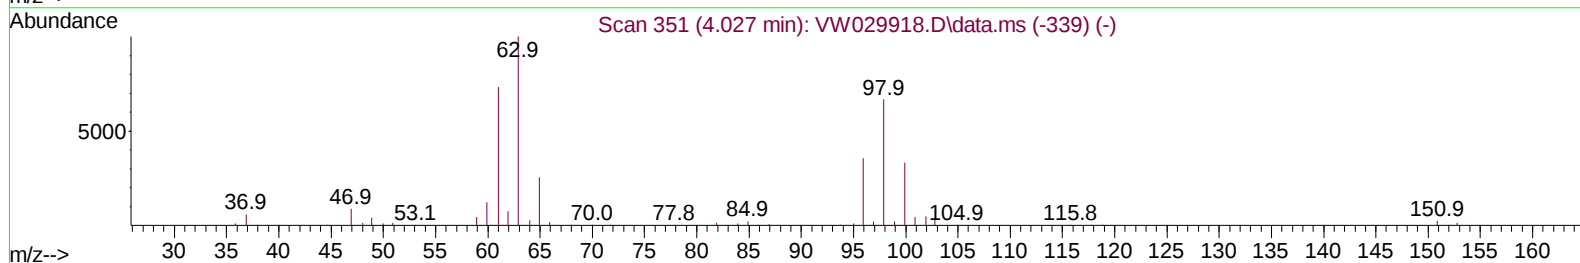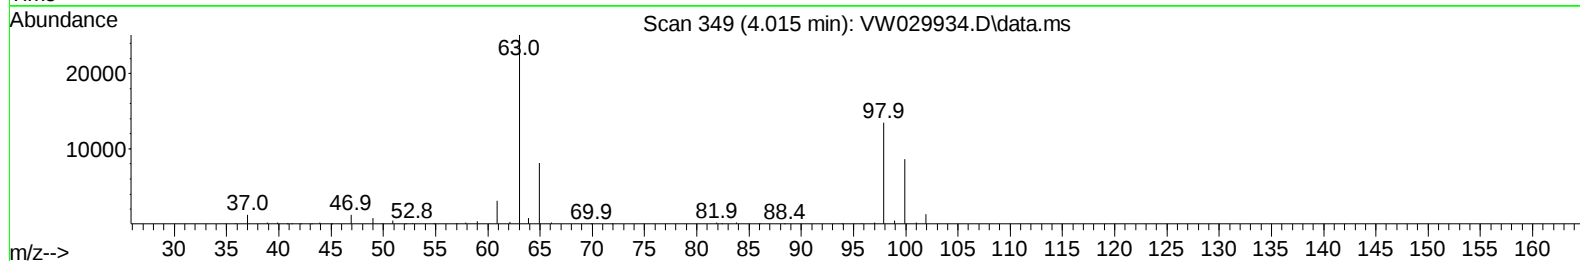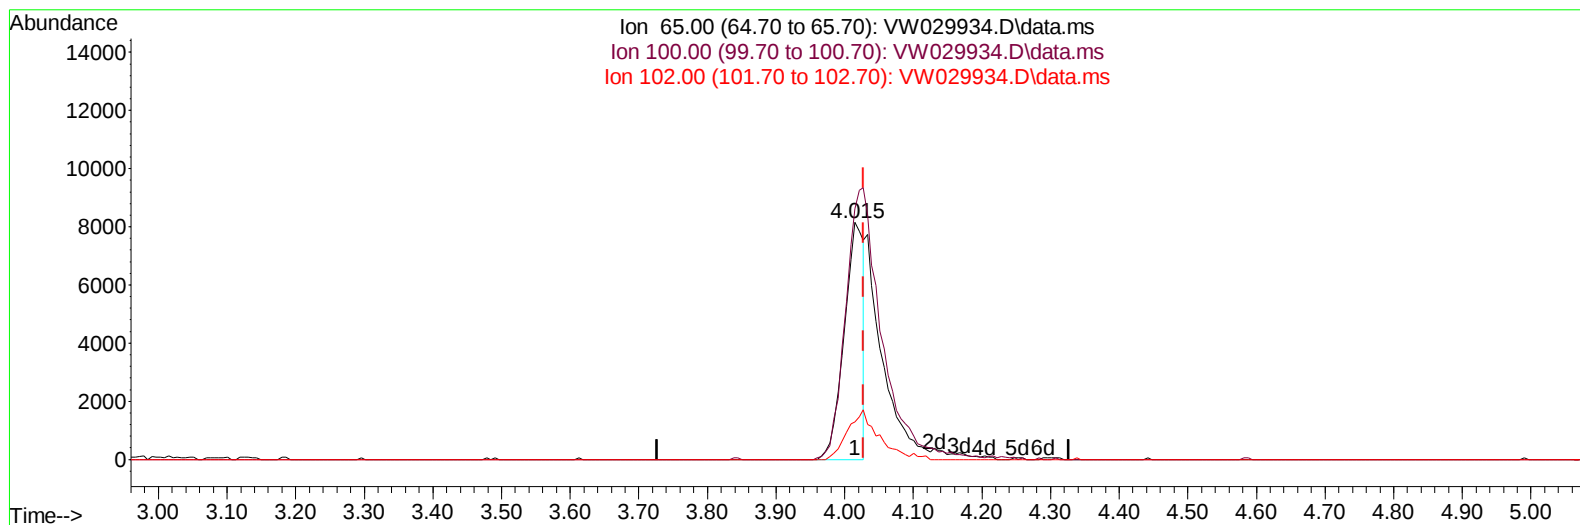

TIC: VW029934.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.015min (-0.012) 7.76 ug/L

response 16009

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	126.90	212.13#
102.00	18.40	32.29#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
Data File : VW029934.D
Acq On : 16 Aug 2024 16:24
Operator : SY/MD
Sample : P3504-21
Misc : 5.86g/10mL/MSVOA_W/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYA2

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:37:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 17 00:33:10 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
Supervised By :Mahesh Dadoda 08/19/2024

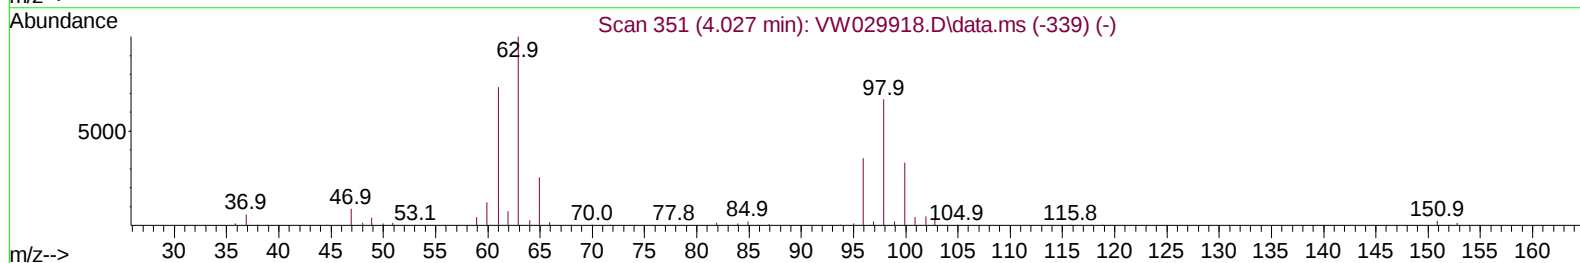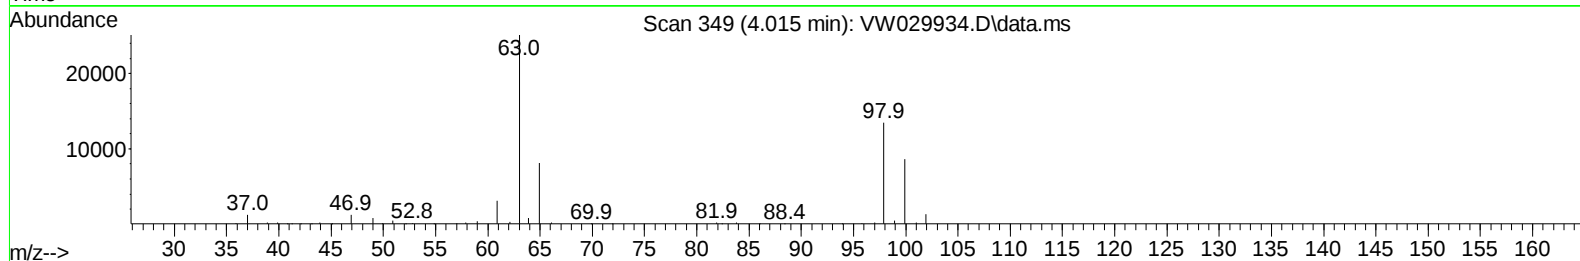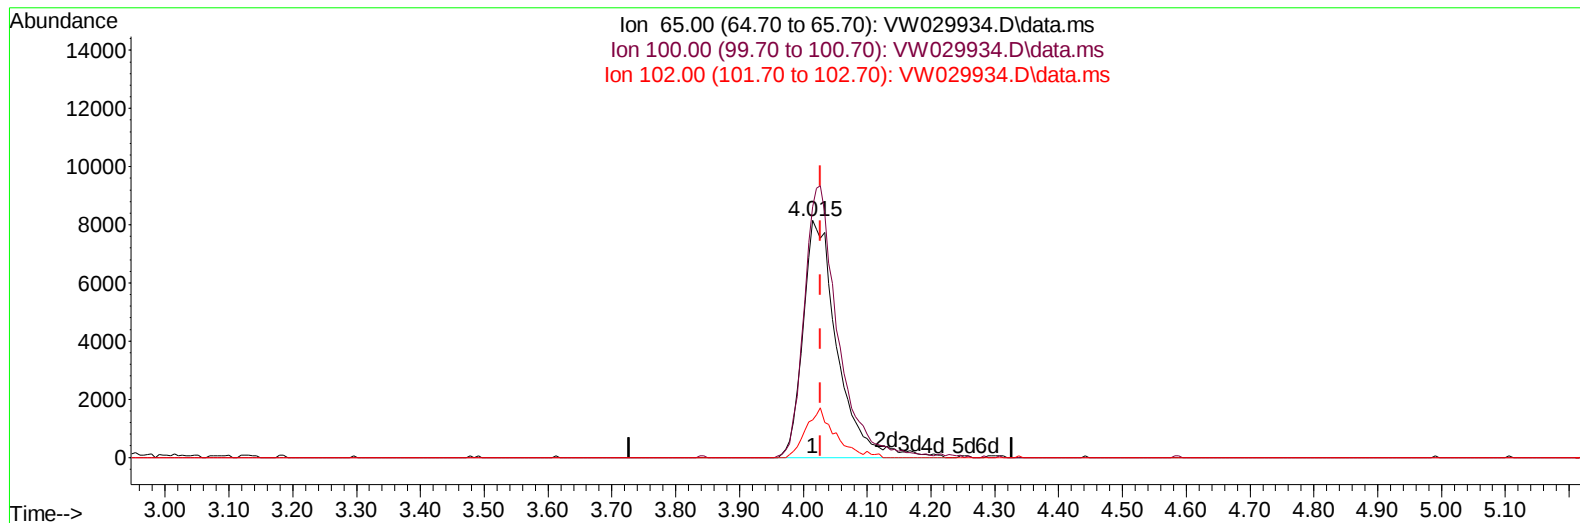

TIC: VW029934.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.015min (-0.012) 14.67 ug/L m

response 30282

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	126.90	112.15
102.00	18.40	17.07
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
Data File : VW029934.D
Acq On : 16 Aug 2024 16:24
Operator : SY/MD
Sample : P3504-21
Misc : 5.86g/10mL/MSVOA_W/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYA2

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:37:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 17 00:33:10 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
Supervised By :Mahesh Dadoda 08/19/2024

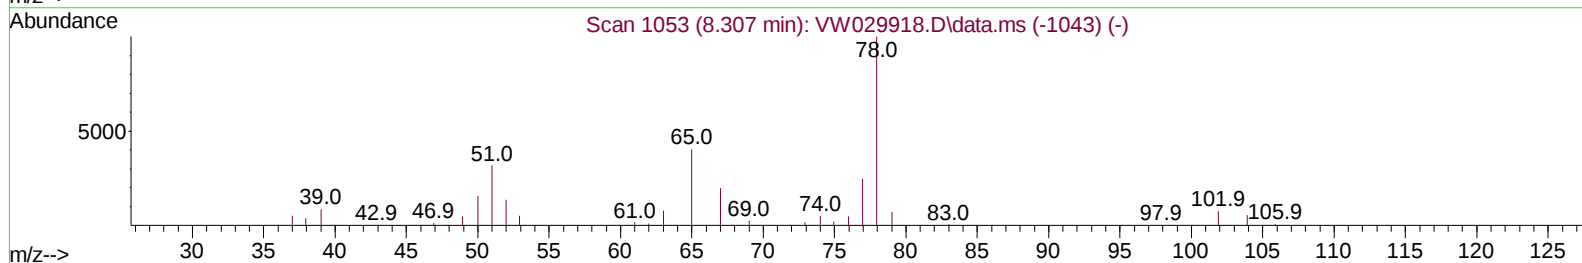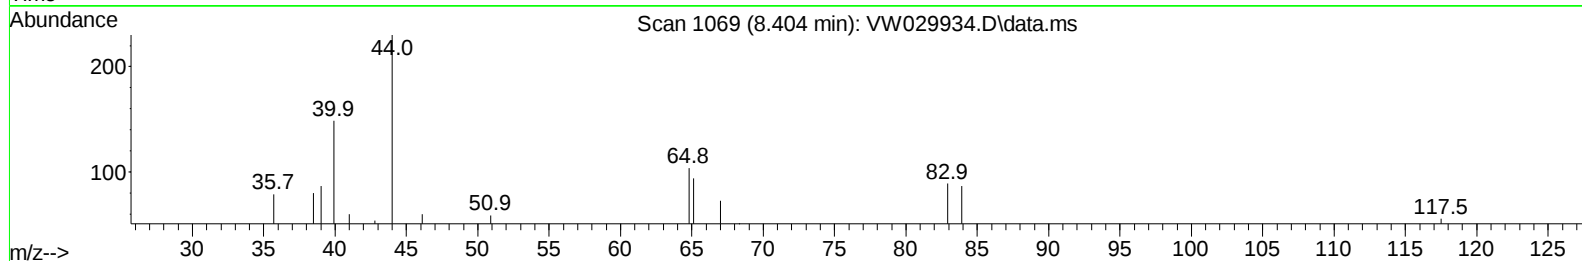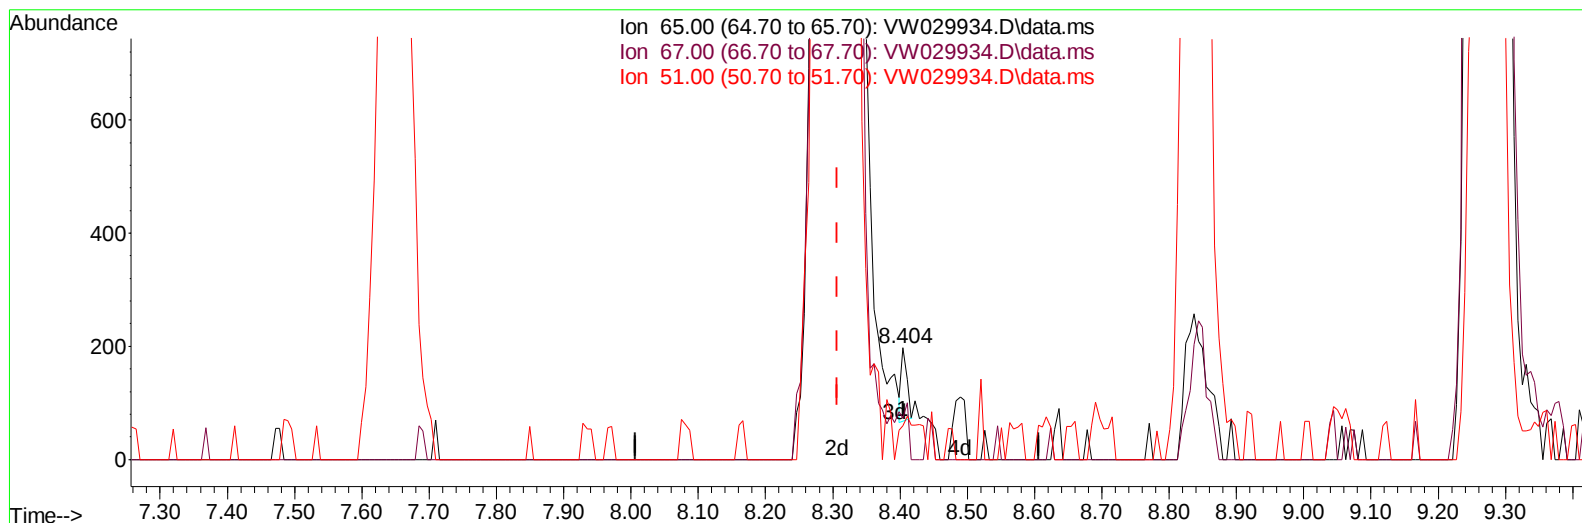

TIC: VW029934.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.404min (+ 0.098) 0.02 ug/L

response 75

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	49.33
51.00	120.50	121.33
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
 Data File : VW029934.D
 Acq On : 16 Aug 2024 16:24
 Operator : SY/MD
 Sample : P3504-21
 Misc : 5.86g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYA2

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:37:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 17 00:33:10 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
 Supervised By :Mahesh Dadoda 08/19/2024

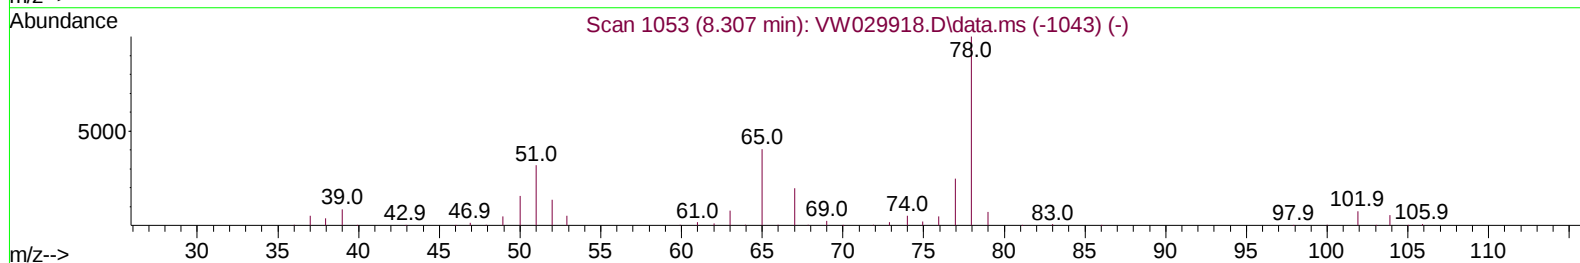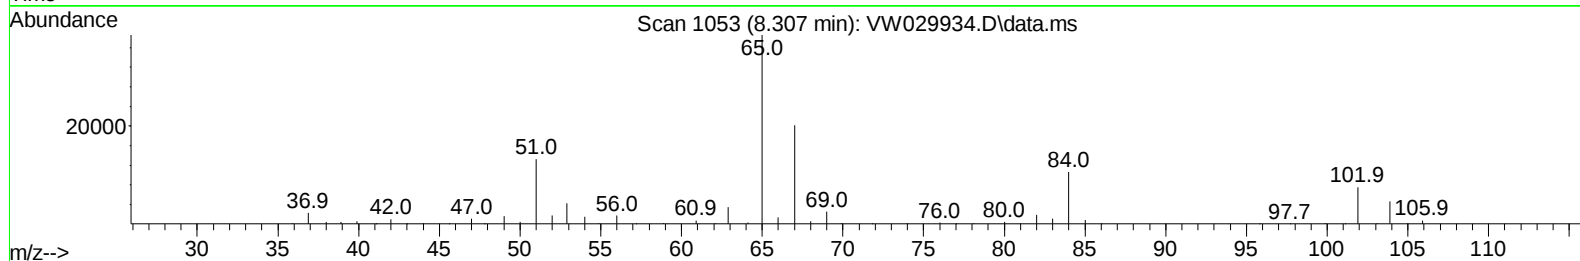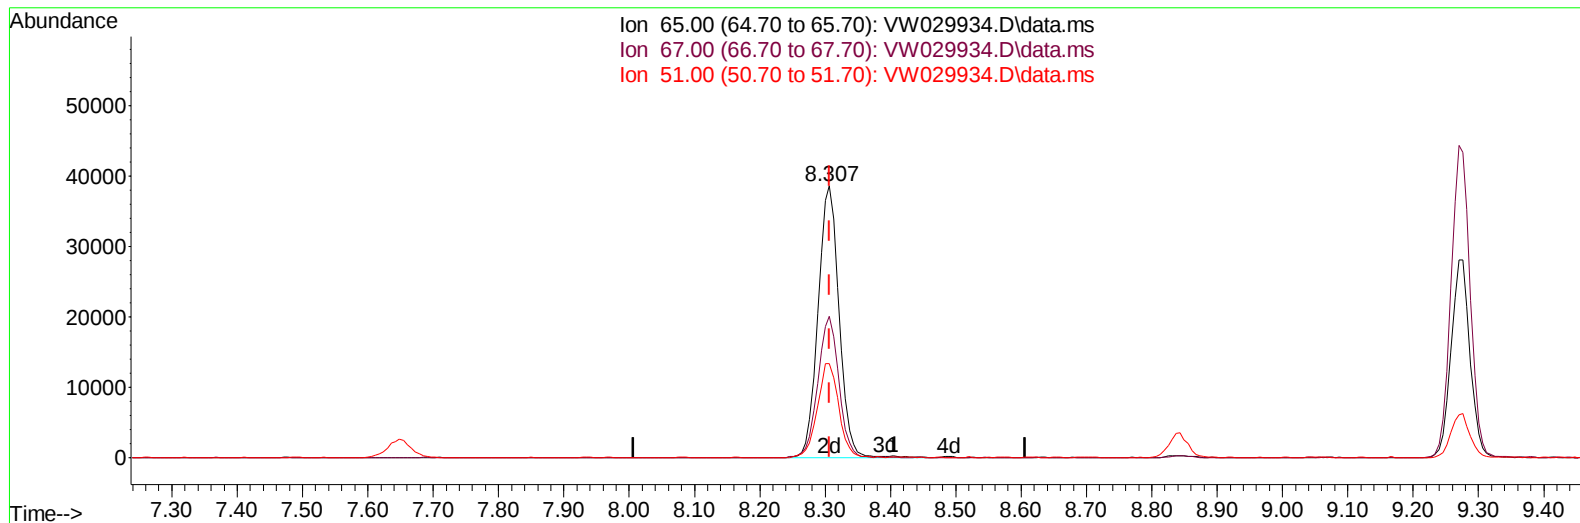

TIC: VW029934.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 18.32 ug/L m

response 86026

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.04#
51.00	120.50	0.11#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
 Data File : VW029934.D
 Acq On : 16 Aug 2024 16:24
 Operator : SY/MD
 Sample : P3504-21
 Misc : 5.86g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYA2

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:37:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 17 00:33:10 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
 Supervised By :Mahesh Dadoda 08/19/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		318521	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		290578	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		103616	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		66544	14.716	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	58.880%		
7) Chloroethane-d5	2.899	69		60944	18.878	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	75.520%		
11) 1,1-Dichloroethene-d2	4.015	65		30282m	14.670	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery =	58.680%		
21) 2-Butanone-d5	7.081	46		36973	29.831	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	59.660%		
24) Chloroform-d	7.642	84		155322	18.837	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	75.360%		
26) 1,2-Dichloroethane-d4	8.307	65		86026m	18.317	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	73.280%		
32) Benzene-d6	8.276	84		277585	17.680	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	70.720%		
36) 1,2-Dichloropropane-d6	9.270	67		89833	17.919	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	71.680%		
41) Toluene-d8	10.325	98		246619	17.666	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	70.680%		
43) trans-1,3-Dichloroprop...	10.575	79		33279	16.405	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	65.600%		
47) 2-Hexanone-d5	10.922	63		27522	33.294	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	66.580%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		71788	19.285	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	77.160%		
66) 1,2-Dichlorobenzene-d4	13.848	152		62534	19.436	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	77.760%		
Target Compounds							
13) Acetone	4.125	43		10577	6.867	ug/L	Qvalue 77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
Data File : VW029934.D
Acq On : 16 Aug 2024 16:24
Operator : SY/MD
Sample : P3504-21
Misc : 5.86g/10mL/MSVOA_W/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYA2

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:37:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 17 00:33:10 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
Supervised By :Mahesh Dadoda 08/19/2024

