




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
Data File : VW029937.D
Acq On : 16 Aug 2024 17:36
Operator : SY/MD
Sample : P3504-24
Misc : 5.72g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYF2

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:38:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 17 00:33:10 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
Supervised By :Mahesh Dadoda 08/19/2024

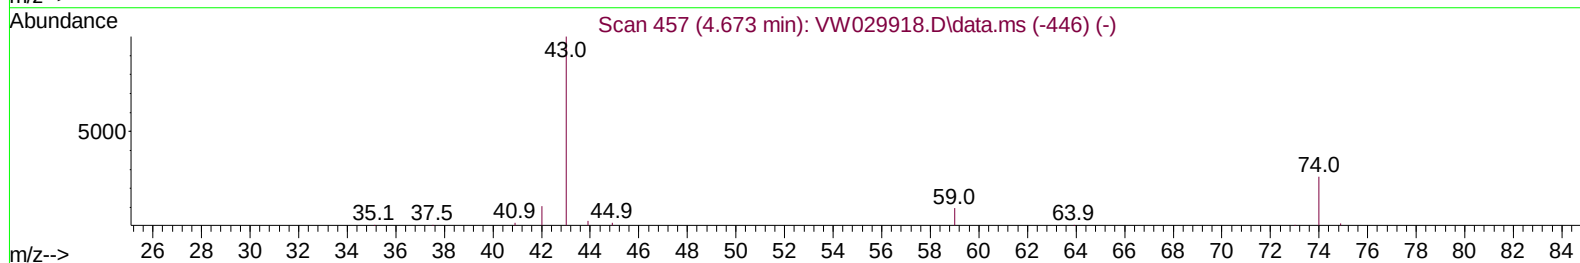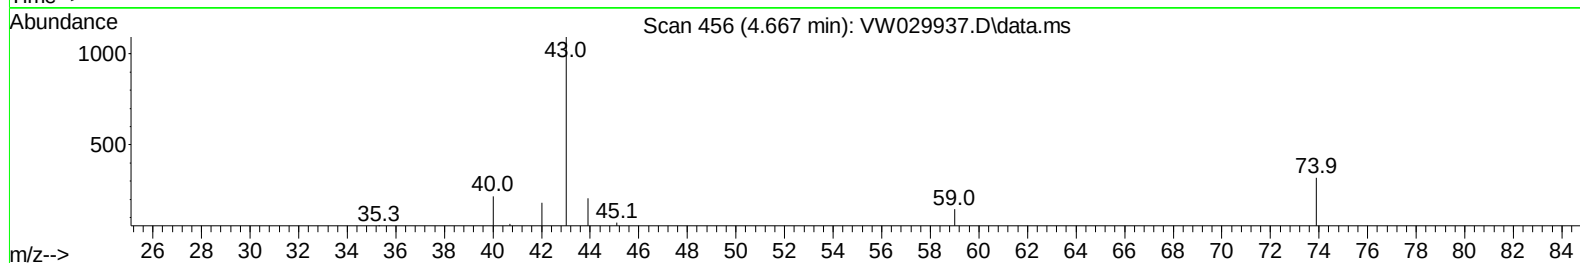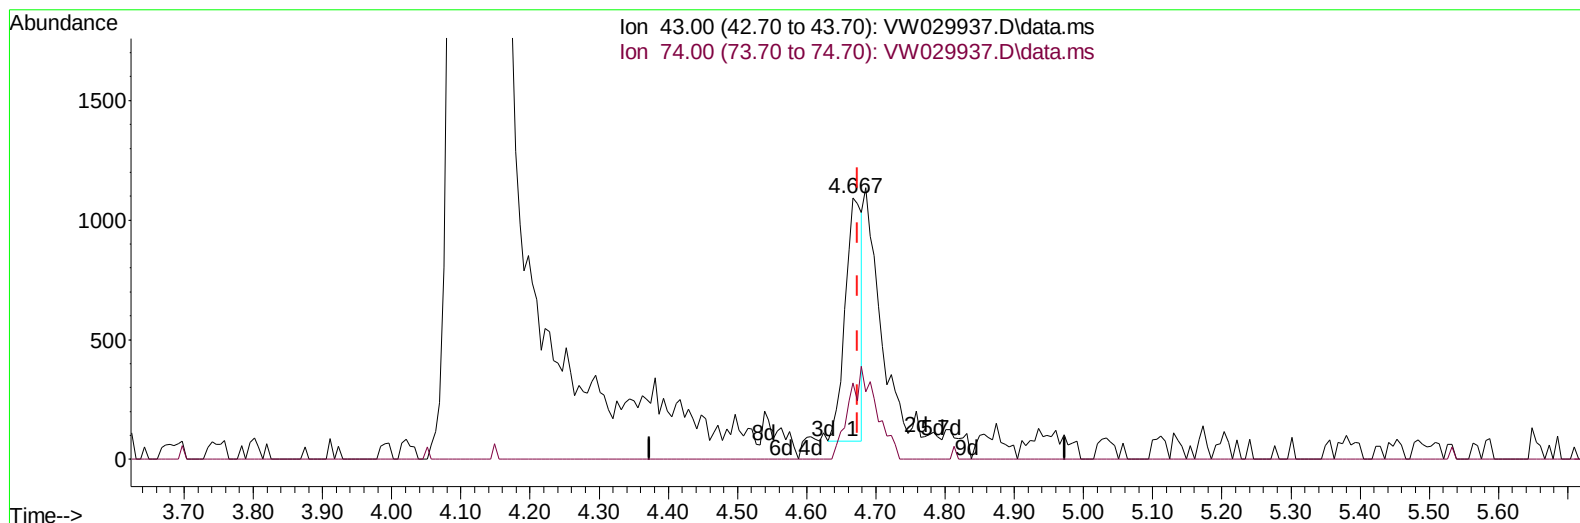

TIC: VW029937.D\data.ms

(15) Methyl Acetate (T)

4.667min (-0.006) 0.75 ug/L

response 1734

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	20.60	23.47
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
 Data File : VW029937.D
 Acq On : 16 Aug 2024 17:36
 Operator : SY/MD
 Sample : P3504-24
 Misc : 5.72g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYF2

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:38:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 17 00:33:10 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
 Supervised By :Mahesh Dadoda 08/19/2024

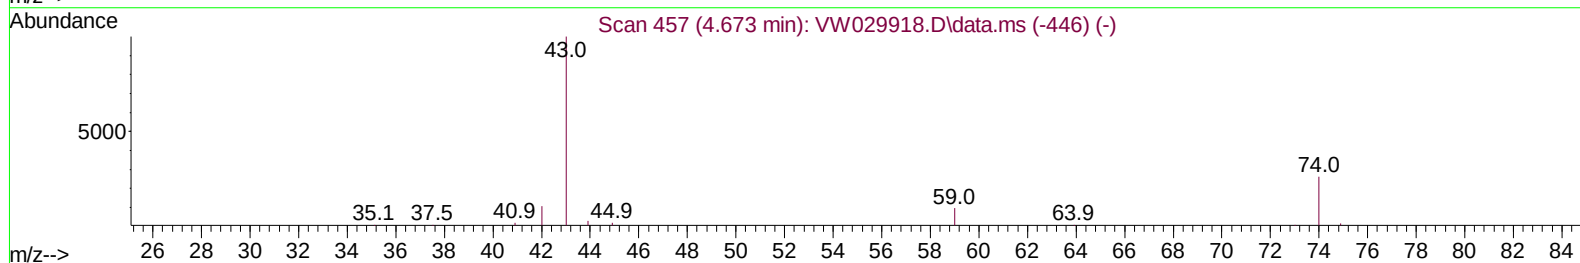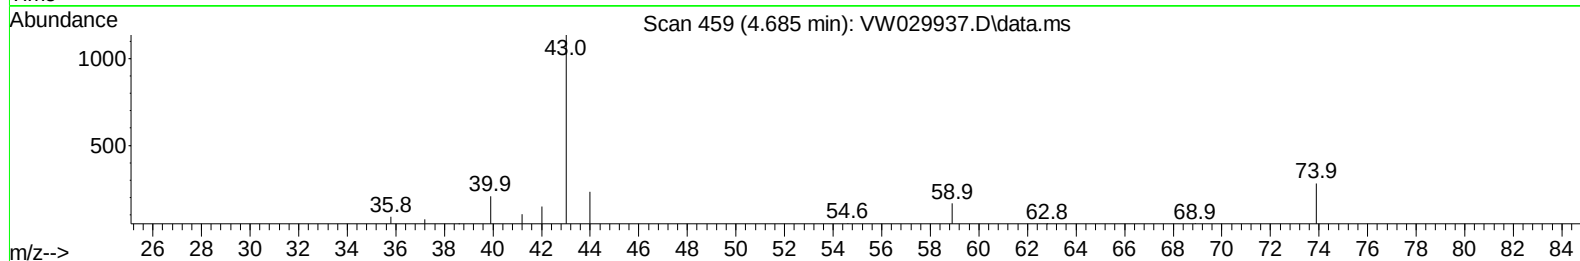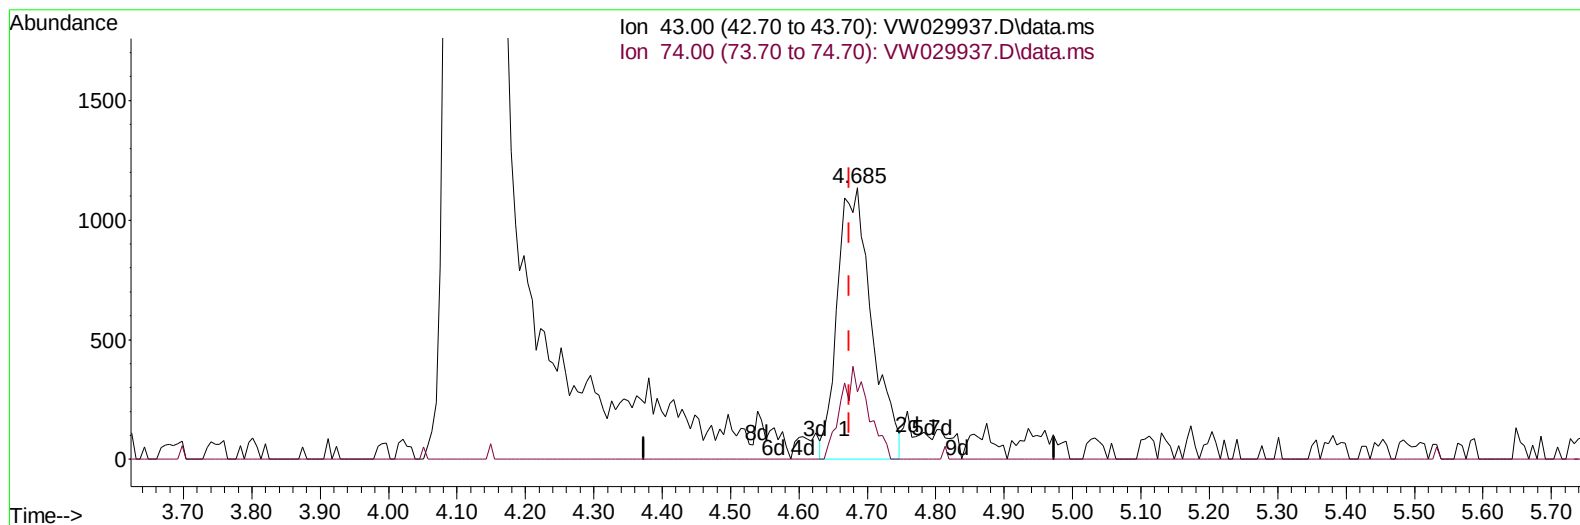

TIC: VW029937.D\data.ms

(15) Methyl Acetate (T)

4.685min (+ 0.012) 1.71 ug/L m

response 3960

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	20.60	10.28#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
 Data File : VW029937.D
 Acq On : 16 Aug 2024 17:36
 Operator : SY/MD
 Sample : P3504-24
 Misc : 5.72g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYF2

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:38:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 17 00:33:10 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/19/2024
 Supervised By :Mahesh Dadoda 08/19/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	287564	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	258289	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	112447	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	61080	14.962	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	59.840%	
7) Chloroethane-d5	2.893	69	54991	18.867	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.480%	
11) 1,1-Dichloroethene-d2	4.021	65	25294	13.573	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	54.280%	
21) 2-Butanone-d5	7.075	46	39642	35.428	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	70.860%	
24) Chloroform-d	7.648	84	140764	18.910	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	75.640%	
26) 1,2-Dichloroethane-d4	8.307	65	84960	20.038	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	80.160%	
32) Benzene-d6	8.276	84	251654	18.032	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	72.120%	
36) 1,2-Dichloropropane-d6	9.270	67	83599	18.760	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	75.040%	
41) Toluene-d8	10.325	98	215633	17.377	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	69.520%	
43) trans-1,3-Dichloroprop...	10.575	79	31512	17.476	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	69.920%	
47) 2-Hexanone-d5	10.922	63	30044	40.888	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	81.780%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	75202	22.728	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	90.920%	
66) 1,2-Dichlorobenzene-d4	13.848	152	59587	17.066	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	68.280%#	
Target Compounds						
						Qvalue
13) Acetone	4.118	43	90909	65.376	ug/L	96
15) Methyl Acetate	4.685	43	3960m	1.710	ug/L	
16) Methylene chloride	4.929	84	13524	2.250	ug/L	86
42) Toluene	10.386	91	6145	0.340	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
Data File : VW029937.D
Acq On : 16 Aug 2024 17:36
Operator : SY/MD
Sample : P3504-24
Misc : 5.72g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYF2

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/19/2024
Supervised By :Mahesh Dadoda 08/19/2024

Quant Time: Aug 17 00:38:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 17 00:33:10 2024
Response via : Initial Calibration

