

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
 Data File : VW029921.D
 Acq On : 16 Aug 2024 11:12
 Operator : SY/MD
 Sample : P3504-10
 Misc : 5.76g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYC8

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 08/19/2024
 Supervised By :Mahesh Dadoda 08/19/2024

Quant Time: Aug 17 00:34:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 17 00:33:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	359799	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	324801	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	148321	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	76115	14.901	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	59.600%		
7) Chloroethane-d5	2.899	69	66287	18.177	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.720%		
11) 1,1-Dichloroethene-d2	4.021	65	33555	14.391	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.560%		
21) 2-Butanone-d5	7.081	46	39338	28.098	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	56.200%		
24) Chloroform-d	7.648	84	169975	18.249	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	73.000%		
26) 1,2-Dichloroethane-d4	8.307	65	96453m	18.181	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	72.720%		
32) Benzene-d6	8.276	84	305365	17.400	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	69.600%		
36) 1,2-Dichloropropane-d6	9.276	67	98684	17.611	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	70.440%		
41) Toluene-d8	10.325	98	283835	18.189	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	72.760%		
43) trans-1,3-Dichloroprop...	10.575	79	38397	16.934	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	67.720%		
47) 2-Hexanone-d5	10.922	63	31579	34.176	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	68.360%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	82950	19.936	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	79.760%		
66) 1,2-Dichlorobenzene-d4	13.848	152	87161	18.926	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	75.720%		
Target Compounds					Qvalue	
13) Acetone	4.131	43	24128	13.868	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081624\
Data File : VW029921.D
Acq On : 16 Aug 2024 11:12
Operator : SY/MD
Sample : P3504-10
Misc : 5.76g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DCYC8

Quant Time: Aug 17 00:34:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 17 00:33:10 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Romaben Patel 08/19/2024
Supervised By :Mahesh Dadoda 08/19/2024

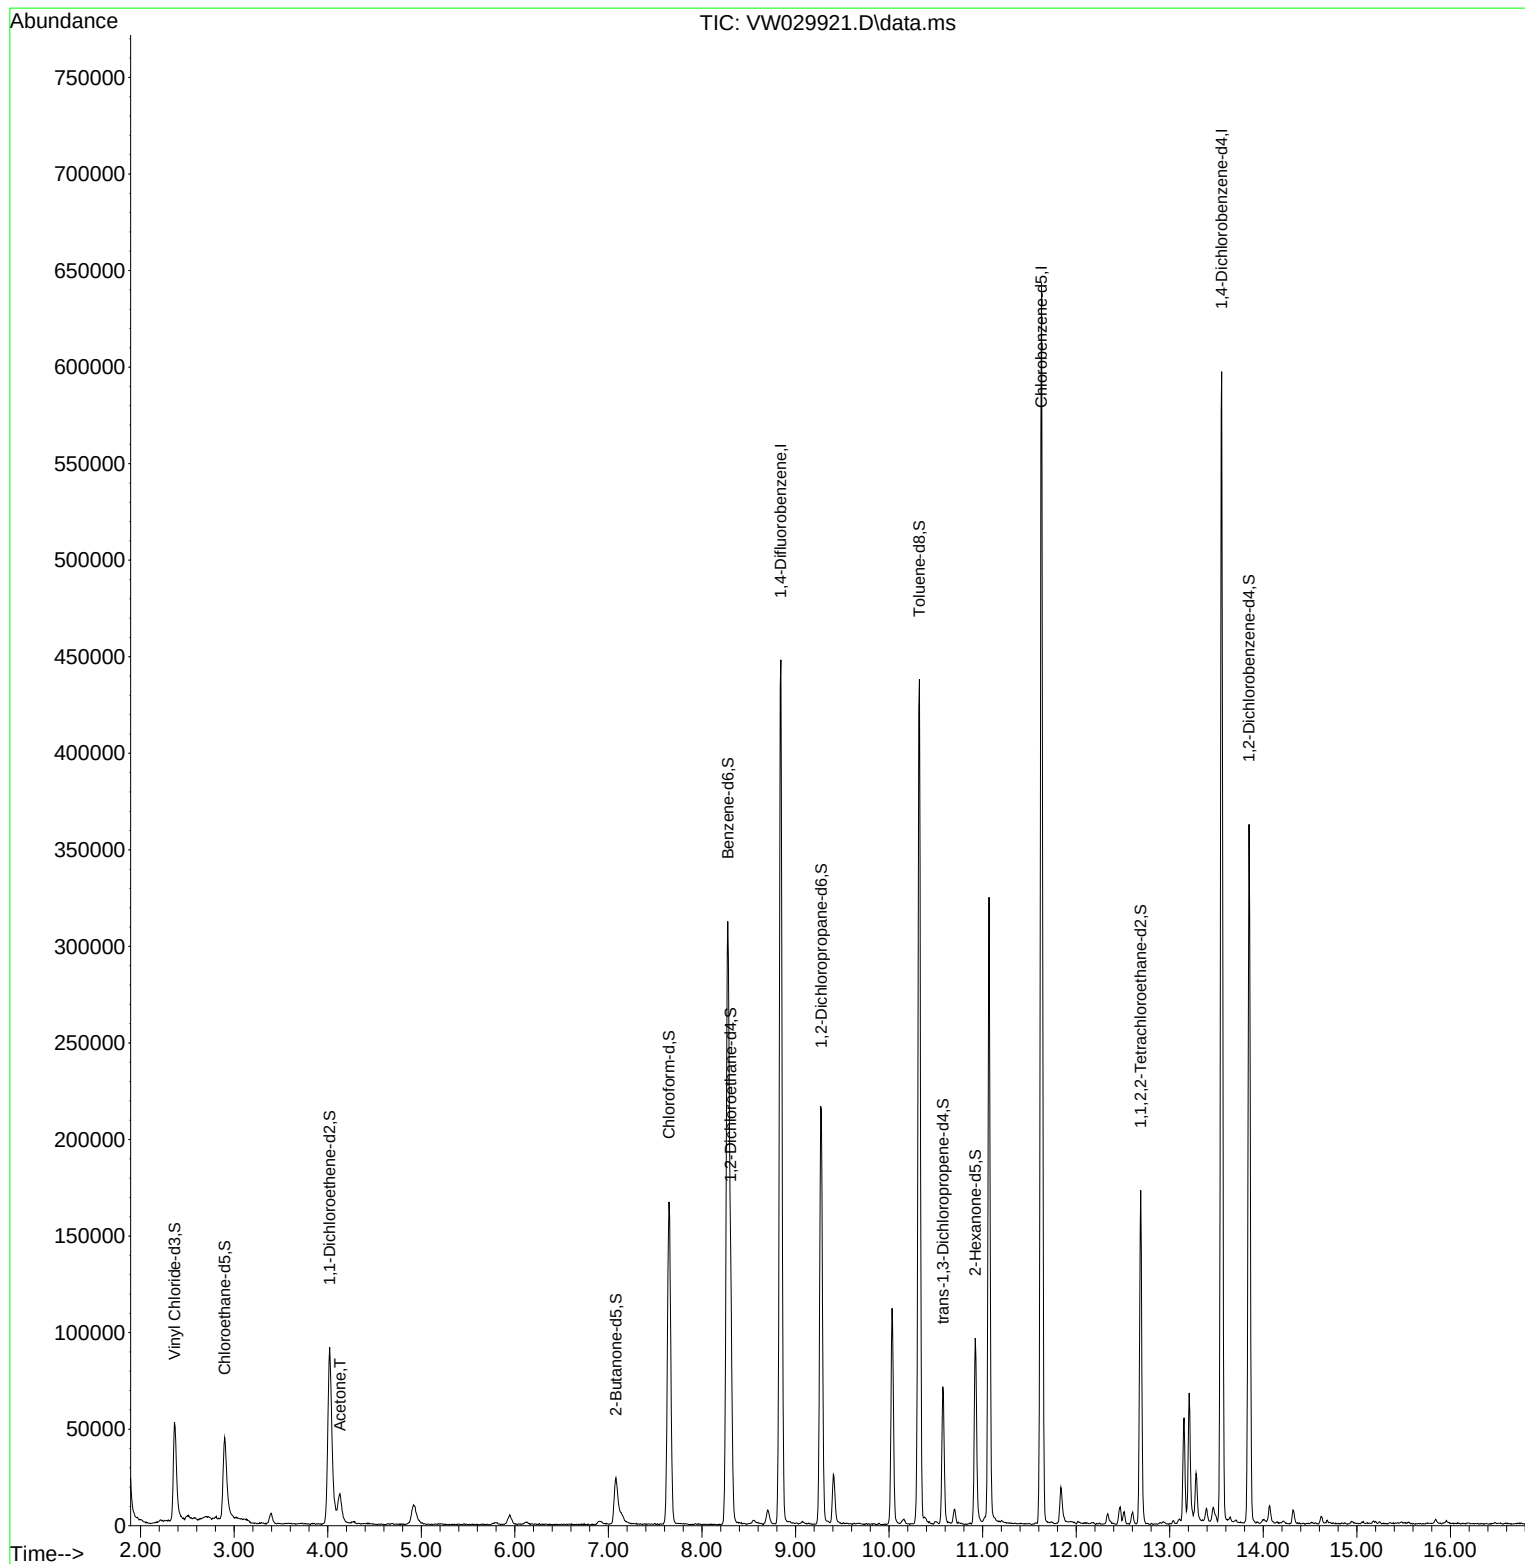

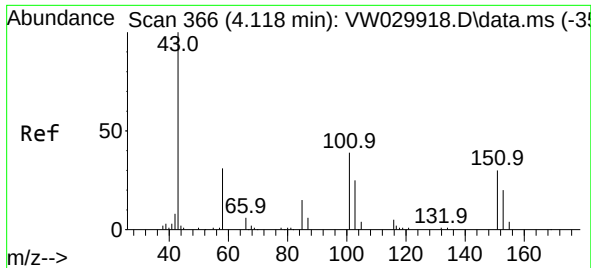

#13
 Acetone
 Concen: 13.868 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW029921.D
 Acq: 16 Aug 2024 11:12

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYC8

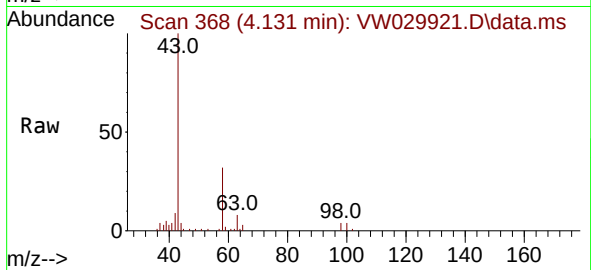

Tgt Ion: 43 Resp: 24128
 Ion Ratio Lower Upper
 43 100
 58 29.6 0.0 57.6

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 08/19/2024
 Supervised By :Mahesh Dadoda 08/19/2024

