

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081718\
 Data File : VW004719.D
 Acq On : 16 Aug 2018 01:54
 Operator : SY/AP
 Sample : J4448-01
 Misc : 5.76G/5ML/MSVOA W/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 TOD1-SB-01-0-2

Quant Time: Aug 16 05:49:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W080618S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 07 08:22:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	483693	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	803862	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	749274	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	313035	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	249140	46.53	ug/l	0.00
Spiked Amount			Recovery	=	93.06%	
35) Dibromofluoromethane	7.88	113	241946	45.14	ug/l	0.00
Spiked Amount			Recovery	=	90.28%	
50) Toluene-d8	10.33	98	778698	38.11	ug/l	0.00
Spiked Amount			Recovery	=	76.22%	
62) 4-Bromofluorobenzene	12.62	95	245890	33.41	ug/l	0.00
Spiked Amount			Recovery	=	66.82%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW081718\
Data File : VW004719.D
Acq On : 16 Aug 2018 01:54
Operator : SY/AP
Sample : J4448-01
Misc : 5.76G/5ML/MSVOA W/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
TOD1-SB-01-0-2

Quant Time: Aug 16 05:49:04 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W080618S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 07 08:22:01 2018
Response via : Initial Calibration

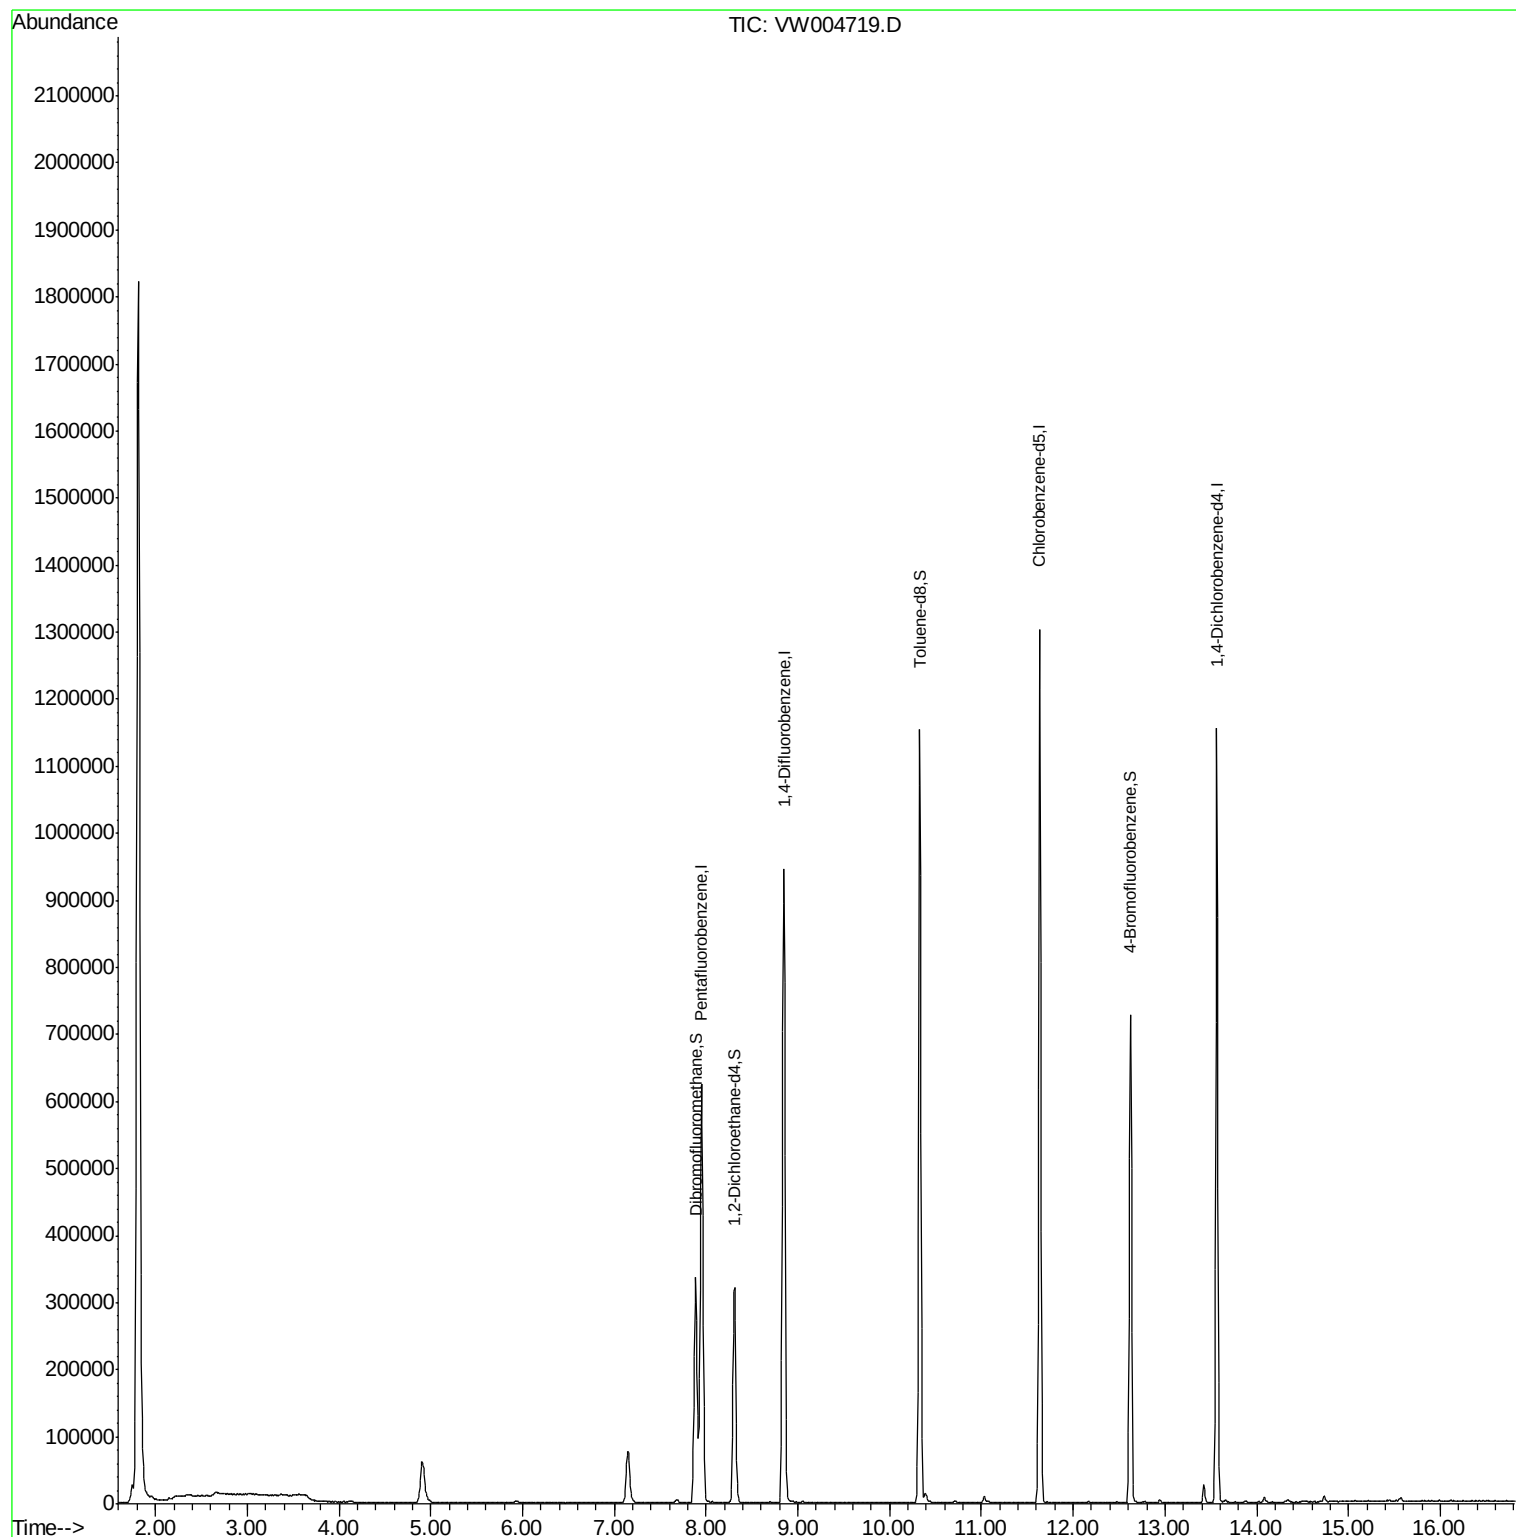

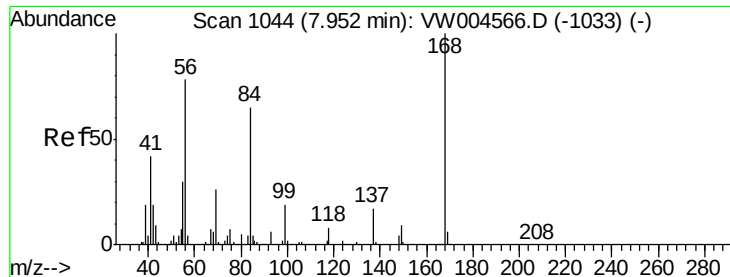

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.95 min Scan# 1044

Delta R.T. 0.00 min

Lab File: VW004719.D

Acq: 16 Aug 2018 01:54

Instrument :

MSVOA_W

ClientSampleId :


TOD1-SB-01-0-2

Tot Ion:168 Resp: 483693

Ion Ratio Lower Upper

168 100

99 54.5 44.1 66.1

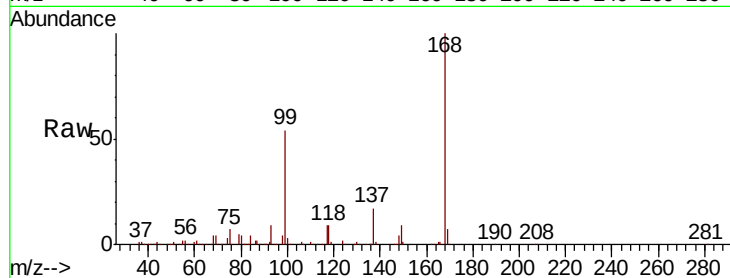

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

250000

200000



150000

100000

50000

0

Time-->

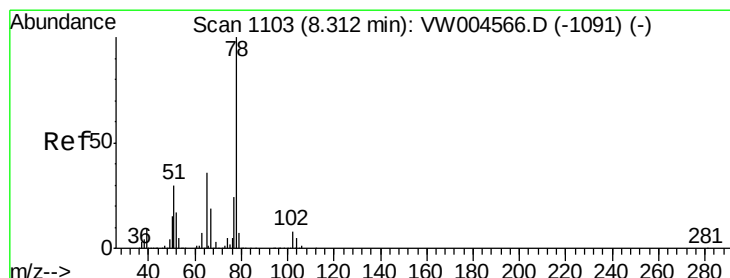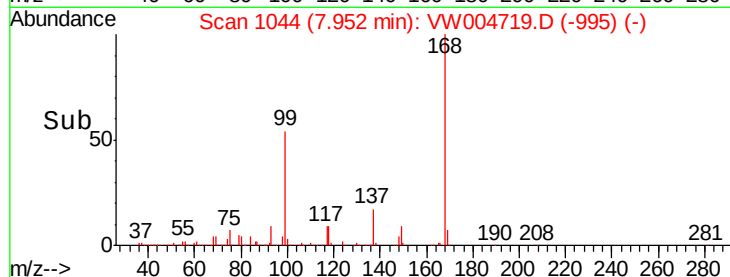

#33

1,2-Dichloroethane-d4

Concen: 46.53 ug/l

RT: 8.31 min Scan# 1103

Delta R.T. 0.00 min

Lab File: VW004719.D


Acq: 16 Aug 2018 01:54

Tgt Ion: 65 Resp: 249140

Ion Ratio Lower Upper

65 100

67 55.0 0.0 109.0

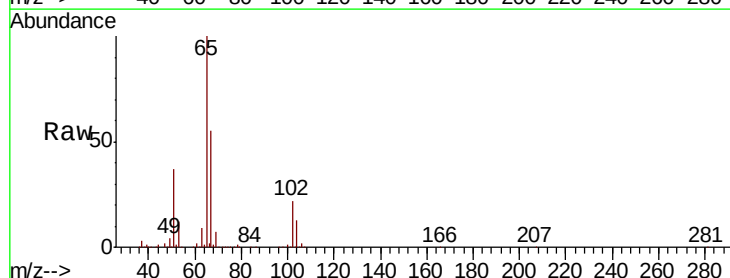

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW


8.31


100000

50000

0

Time-->

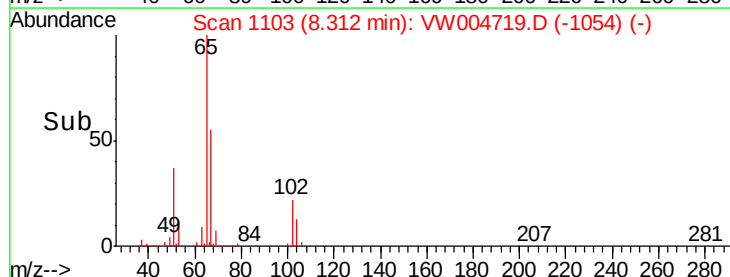


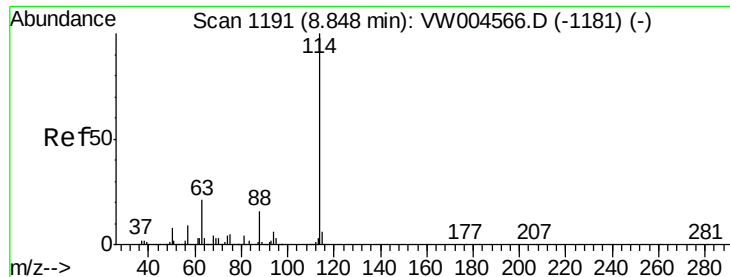




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.85 min Scan# 1191
 Delta R.T. 0.00 min
 Lab File: VW004719.D
 Acq: 16 Aug 2018 01:54

Instrument :
 MSVOA_W
 ClientSampleId :
 TOD1-SB-01-0-2

Tot Ion	Ratio	Lower	Upper
114	100		
63	20.6	0.0	42.4
88	15.7	0.0	31.2

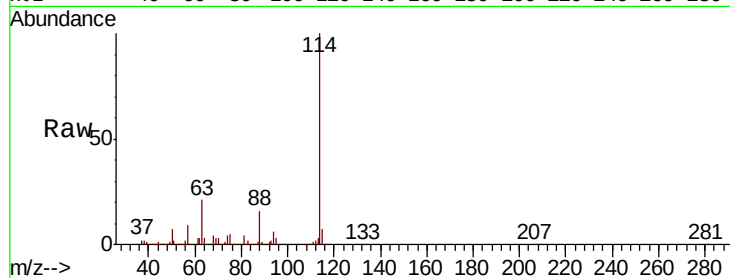


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

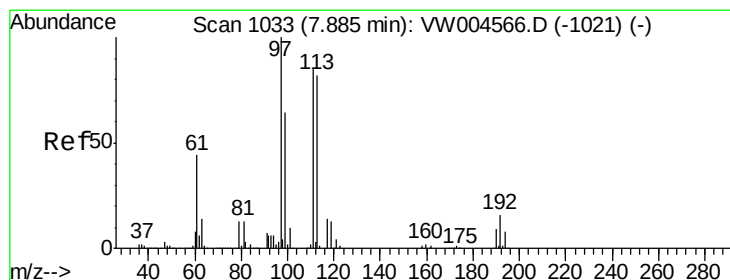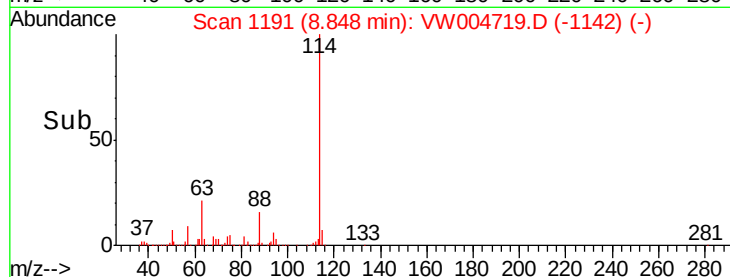
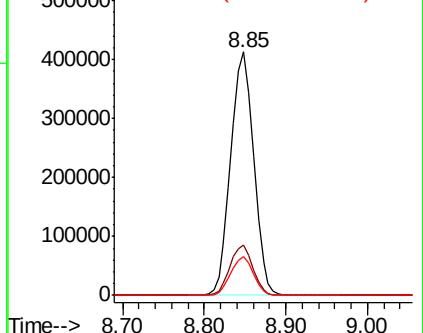



#35
 Dibromofluoromethane
 Concen: 45.14 ug/l
 RT: 7.88 min Scan# 1033
 Delta R.T. 0.00 min
 Lab File: VW004719.D
 Acq: 16 Aug 2018 01:54

Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.7	82.9	124.3
192	21.2	15.8	23.6

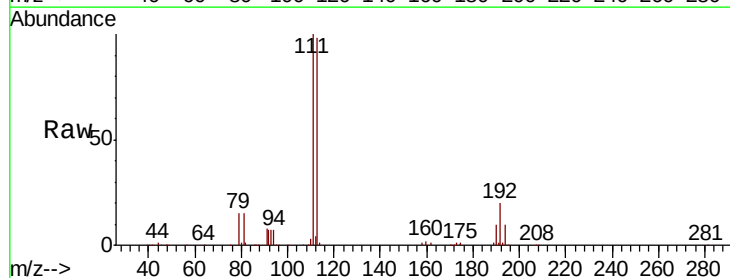

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

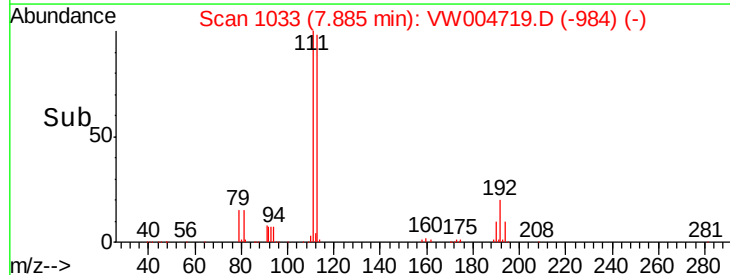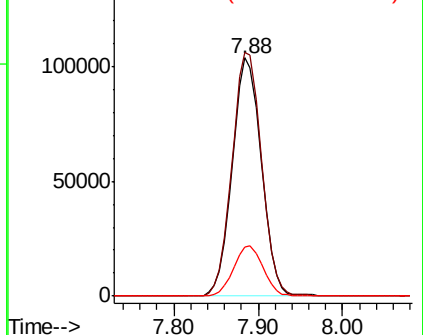

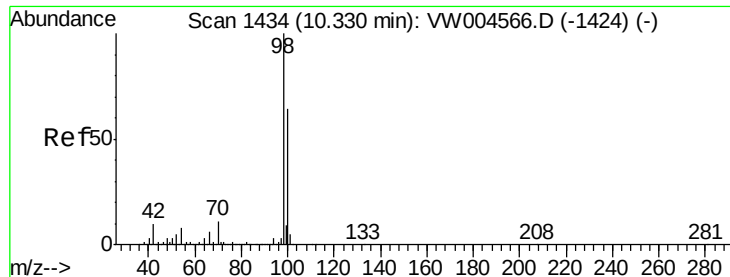

#50

Toluene-d8

Concen: 38.11 ug/l

RT: 10.33 min Scan# 1434

Delta R.T. 0.00 min

Lab File: VW004719.D

Acq: 16 Aug 2018 01:54

Instrument :

MSVOA_W

ClientSampleId :





TOD1-SB-01-0-2

Tot Ion: 98 Resp: 778698

Ion Ratio Lower Upper

98 100

100 62.9 51.4 77.2

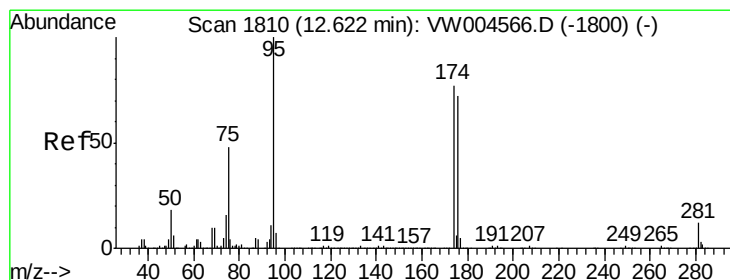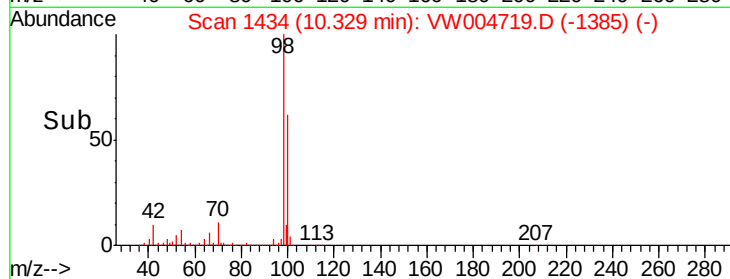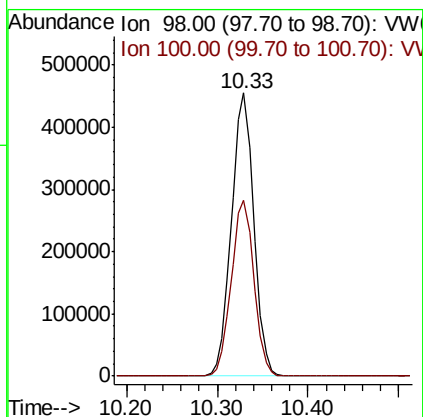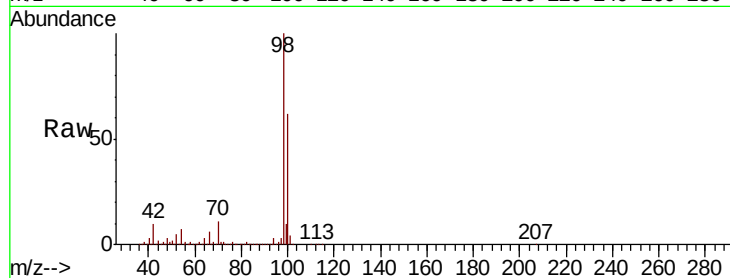

#62

4-Bromofluorobenzene

Concen: 33.41 ug/l

RT: 12.62 min Scan# 1810

Delta R.T. 0.00 min

Lab File: VW004719.D

Acq: 16 Aug 2018 01:54




Tgt Ion: 95 Resp: 245890


Ion Ratio Lower Upper

95 100

174 83.6 0.0 160.4

176 80.2 0.0 153.2


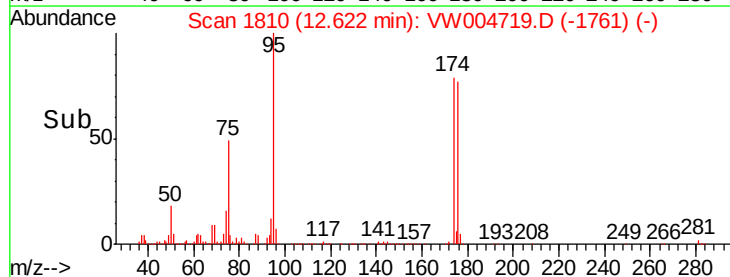
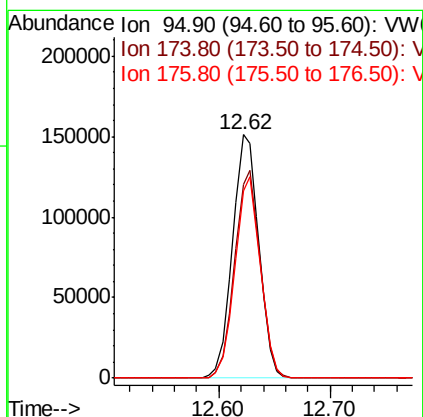
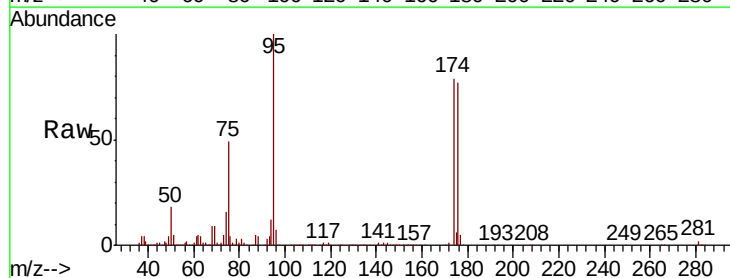


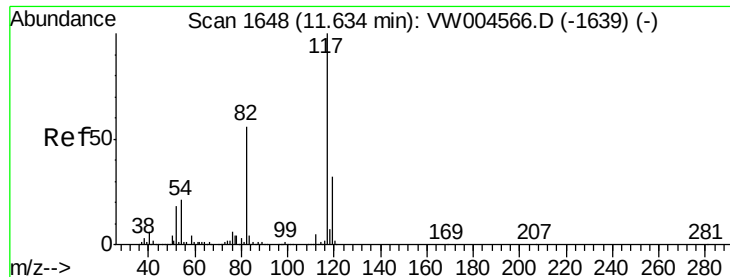

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.63 min Scan# 1648
Delta R.T. 0.00 min
Lab File: VW004719.D
Acq: 16 Aug 2018 01:54

Instrument :
MSVOA_W
ClientSampleId :
TOD1-SB-01-0-2

Tot Ion:117 Resp: 749274
Ion Ratio Lower Upper
117 100
82 56.1 45.3 67.9
119 32.3 26.2 39.4

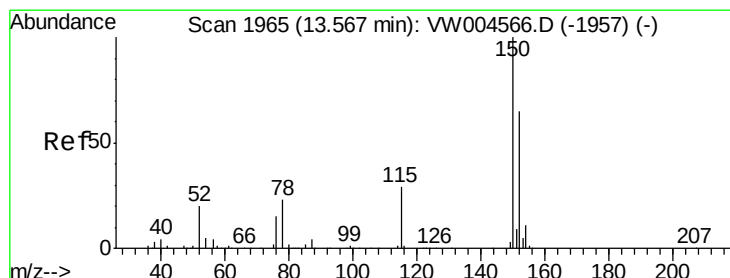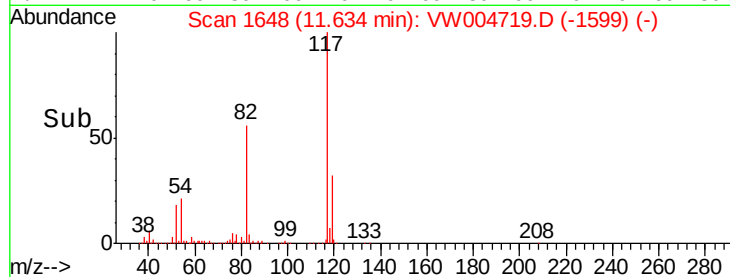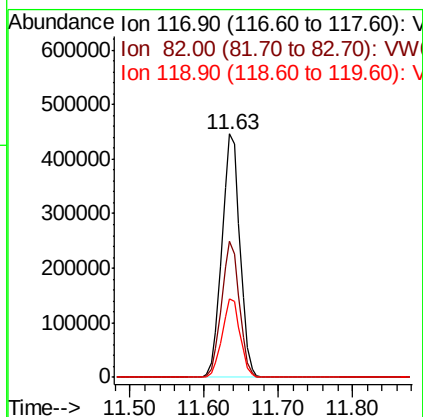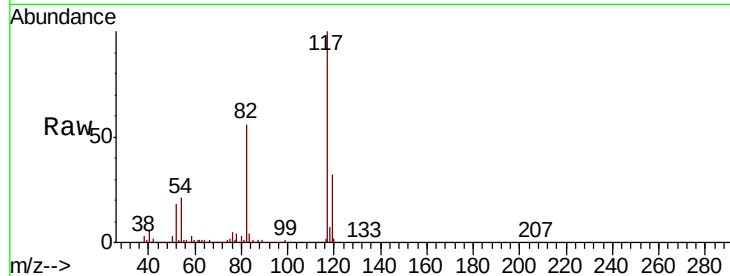

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.57 min Scan# 1965
Delta R.T. 0.00 min
Lab File: VW004719.D
Acq: 16 Aug 2018 01:54

Tgt Ion:152 Resp: 313035
Ion Ratio Lower Upper
152 100
115 56.5 29.1 87.3
150 155.5 0.0 349.6

